

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU053019\
 Data File : VU032376.D
 Acq On : 30 May 2019 13:04
 Operator : JC/SP
 Sample : K3017-24RE
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A51G2RE

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM052819WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.180	24	28	39	rBV5	11657	12439	0.48%	0.060%
2	1.396	88	95	106	rBV	328443	351567	13.56%	1.710%
3	1.672	173	181	198	rVB	266145	350281	13.51%	1.704%
4	1.878	241	245	256	rVB9	7577	10231	0.39%	0.050%
5	2.183	336	340	341	rBV3	5580	4271	0.16%	0.021%
6	2.267	355	366	376	rBV	595120	909960	35.10%	4.426%
7	2.318	376	382	403	rVB	162464	265342	10.23%	1.291%
8	2.447	412	422	442	rBV2	29046	56131	2.16%	0.273%
9	2.698	491	500	510	rBV3	19834	34707	1.34%	0.169%
10	2.830	530	541	543	rBV5	5532	7646	0.29%	0.037%
11	2.916	563	568	572	rBV2	504	582	0.02%	0.003%
12	2.939	572	575	580	rBV3	543	596	0.02%	0.003%
13	2.990	585	591	594	rBV4	769	970	0.04%	0.005%
14	3.010	594	597	600	rVV4	1123	563	0.02%	0.003%
15	3.119	626	631	635	rBV3	755	882	0.03%	0.004%
16	3.174	645	648	654	rBV2	535	623	0.02%	0.003%
17	3.228	660	665	669	rBV3	505	544	0.02%	0.003%
18	3.331	693	697	703	rVB3	564	614	0.02%	0.003%
19	3.373	703	710	711	rBV4	865	973	0.04%	0.005%
20	3.408	716	721	726	rVB3	572	739	0.03%	0.004%
21	3.450	726	734	735	rBV5	571	622	0.02%	0.003%
22	3.916	874	879	882	rVB3	767	670	0.03%	0.003%
23	4.174	946	959	978	rBV	224888	580536	22.39%	2.824%
24	4.640	1088	1104	1136	rBV2	514247	1242360	47.92%	6.042%
25	4.891	1177	1182	1192	rVV7	2648	3929	0.15%	0.019%
26	4.942	1196	1198	1203	rVB4	1122	788	0.03%	0.004%
27	4.987	1210	1212	1218	rVB5	1515	1500	0.06%	0.007%
28	5.334	1297	1320	1351	rBV2	876432	2592823	100.00%	12.611%
29	5.646	1415	1417	1420	rBV3	986	805	0.03%	0.004%
30	5.669	1422	1424	1431	rVB8	788	893	0.03%	0.004%
31	5.743	1443	1447	1450	rVV2	544	568	0.02%	0.003%
32	5.801	1460	1465	1469	rBV5	816	950	0.04%	0.005%
33	5.881	1475	1490	1526	rBV	775507	1582425	61.03%	7.696%
34	6.096	1554	1557	1561	rVB2	1644	1033	0.04%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\U053019\
 Data File : VU032376.D
 Acq On : 30 May 2019 13:04
 Operator : JC/SP
 Sample : K3017-24RE
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A51G2RE

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM052819WMA.M
 Title : VOC Analysis

35	6.180	1570	1583	1598	rBV3	14755	33218	1.28%	0.162%
36	6.325	1614	1628	1652	rVV2	556176	1128911	43.54%	5.491%
37	6.601	1708	1714	1718	rBV7	1274	1647	0.06%	0.008%
38	6.797	1771	1775	1779	rVB3	1045	904	0.03%	0.004%
39	6.871	1789	1798	1807	rBV7	2770	5084	0.20%	0.025%
40	6.945	1819	1821	1824	rVB4	1020	539	0.02%	0.003%
41	7.026	1842	1846	1850	rVB3	888	681	0.03%	0.003%
42	7.225	1896	1908	1930	rBV	288248	526557	20.31%	2.561%
43	7.408	1958	1965	1967	rBV5	2031	2229	0.09%	0.011%
44	7.469	1976	1984	1999	rVB7	3936	8815	0.34%	0.043%
45	7.563	1999	2013	2036	rBV	1164970	2064245	79.61%	10.040%
46	7.846	2091	2101	2124	rBV	199051	357790	13.80%	1.740%
47	8.042	2159	2162	2167	rVB4	1114	787	0.03%	0.004%
48	8.173	2192	2203	2217	rVB	10307	20430	0.79%	0.099%
49	8.228	2217	2220	2224	rBV3	884	802	0.03%	0.004%
50	8.309	2234	2245	2278	rBV	742767	1413848	54.53%	6.876%
51	8.469	2291	2295	2309	rVB	9036	15993	0.62%	0.078%
52	8.701	2364	2367	2373	rBV5	1280	1067	0.04%	0.005%
53	8.762	2381	2386	2389	rVB5	715	616	0.02%	0.003%
54	9.003	2456	2461	2463	rBV2	691	717	0.03%	0.003%
55	9.087	2473	2487	2524	rBV	1158979	1981023	76.40%	9.635%
56	9.305	2553	2555	2558	rBV2	918	715	0.03%	0.003%
57	9.379	2575	2578	2582	rBV4	1812	1610	0.06%	0.008%
58	9.469	2604	2606	2612	rVB4	889	696	0.03%	0.003%
59	9.543	2626	2629	2632	rBV2	843	709	0.03%	0.003%
60	9.714	2678	2682	2686	rBV2	948	947	0.04%	0.005%
61	9.784	2697	2704	2707	rBV5	1715	2084	0.08%	0.010%
62	9.942	2750	2753	2756	rBV2	707	545	0.02%	0.003%
63	10.032	2777	2781	2785	rBV3	1250	1237	0.05%	0.006%
64	10.167	2820	2823	2828	rVB4	1509	1354	0.05%	0.007%
65	10.193	2828	2831	2832	rBV3	1091	567	0.02%	0.003%
66	10.235	2838	2844	2848	rBV6	2789	3490	0.13%	0.017%
67	10.427	2891	2904	2926	rBV	843104	1353408	52.20%	6.583%
68	10.537	2936	2938	2941	rVB3	1086	552	0.02%	0.003%
69	10.607	2951	2960	2972	rVB4	11034	18523	0.71%	0.090%
70	10.656	2972	2975	2979	rBV4	1072	1034	0.04%	0.005%
71	10.765	3006	3009	3015	rBV3	924	759	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU053019\
 Data File : VU032376.D
 Acq On : 30 May 2019 13:04
 Operator : JC/SP
 Sample : K3017-24RE
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A51G2RE

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM052819WMA.M
 Title : VOC Analysis

72	10.861	3036	3039	3042	rBV2	714	545	0.02%	0.003%
73	10.929	3057	3060	3064	rVB	792	561	0.02%	0.003%
74	11.077	3102	3106	3109	rBV4	1200	1056	0.04%	0.005%
75	11.386	3199	3202	3205	rVV3	1078	735	0.03%	0.004%
76	11.405	3205	3208	3212	rVV4	904	769	0.03%	0.004%
77	11.479	3219	3231	3259	rBV	1050696	1721998	66.41%	8.375%
78	11.855	3337	3348	3370	rBV	1108399	1834508	70.75%	8.922%
79	12.180	3446	3449	3454	rBV5	1669	1675	0.06%	0.008%
80	12.218	3457	3461	3462	rBV3	1360	943	0.04%	0.005%
81	12.228	3462	3464	3467	rBV3	1251	698	0.03%	0.003%
82	12.289	3480	3483	3489	rBV6	1538	1587	0.06%	0.008%
83	12.434	3523	3528	3532	rBV7	1086	1299	0.05%	0.006%
84	12.472	3536	3540	3546	rVB5	3344	3812	0.15%	0.019%
85	12.524	3553	3556	3561	rBV3	1234	902	0.03%	0.004%
86	12.672	3597	3602	3608	rBV8	1995	2526	0.10%	0.012%
87	12.697	3608	3610	3614	rBV3	787	627	0.02%	0.003%
88	12.858	3658	3660	3664	rBV4	1593	1041	0.04%	0.005%
89	12.955	3687	3690	3692	rBV2	994	601	0.02%	0.003%
90	13.019	3705	3710	3712	rBV4	895	795	0.03%	0.004%
91	13.048	3712	3719	3724	rVV4	1304	1656	0.06%	0.008%
92	13.138	3745	3747	3753	rVB3	1116	786	0.03%	0.004%
93	13.193	3760	3764	3766	rBV2	1262	1028	0.04%	0.005%
94	13.276	3785	3790	3792	rBV3	1418	1303	0.05%	0.006%
95	13.511	3861	3863	3866	rBV2	1056	819	0.03%	0.004%
96	13.775	3943	3945	3948	rBV2	1127	765	0.03%	0.004%
97	13.839	3962	3965	3972	rVB5	1434	1342	0.05%	0.007%
98	13.929	3989	3993	3997	rBV3	1040	795	0.03%	0.004%
99	14.398	4136	4139	4142	rBV2	1035	680	0.03%	0.003%
100	14.498	4166	4170	4173	rBV3	1045	1077	0.04%	0.005%


Sum of corrected areas: 20560625

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU053019\
Data File : VU032376.D
Acq On : 30 May 2019 13:04
Operator : JC/SP
Sample : K3017-24RE
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A51G2RE

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM052819WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

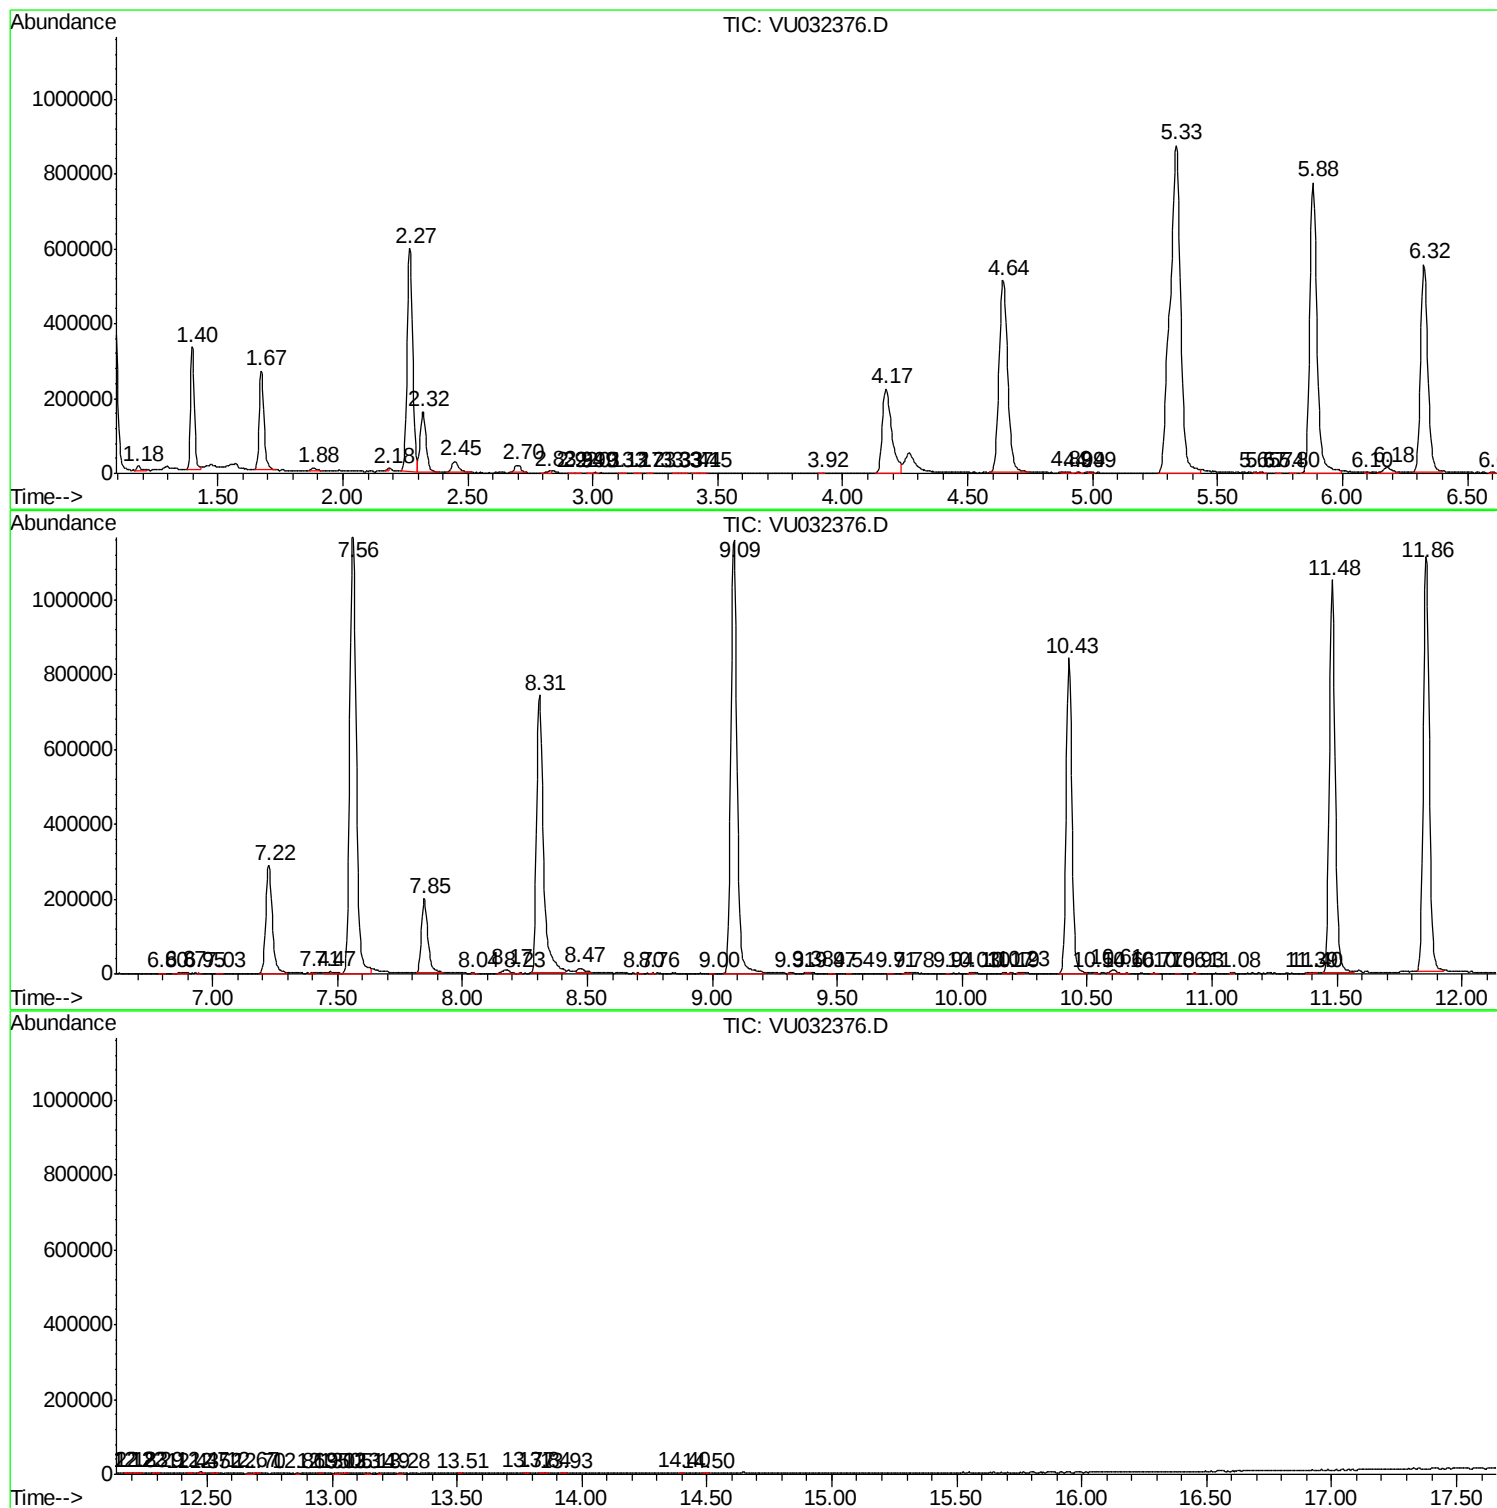

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU053019\
Data File : VU032376.D
Acq On : 30 May 2019 13:04
Operator : JC/SP
Sample : K3017-24RE
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A51G2RE

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM052819WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU053019\
Data File : VU032376.D
Acq On : 30 May 2019 13:04
Operator : JC/SP
Sample : K3017-24RE
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A51G2RE

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM052819WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc