


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU053019\
 Data File : VU032370.D
 Acq On : 30 May 2019 10:36
 Operator : JC/SP
 Sample : BFB47
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB47

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM052819WMA.M
 Title : VOC Analysis
 Last Update : Fri May 31 04:34:14 2019

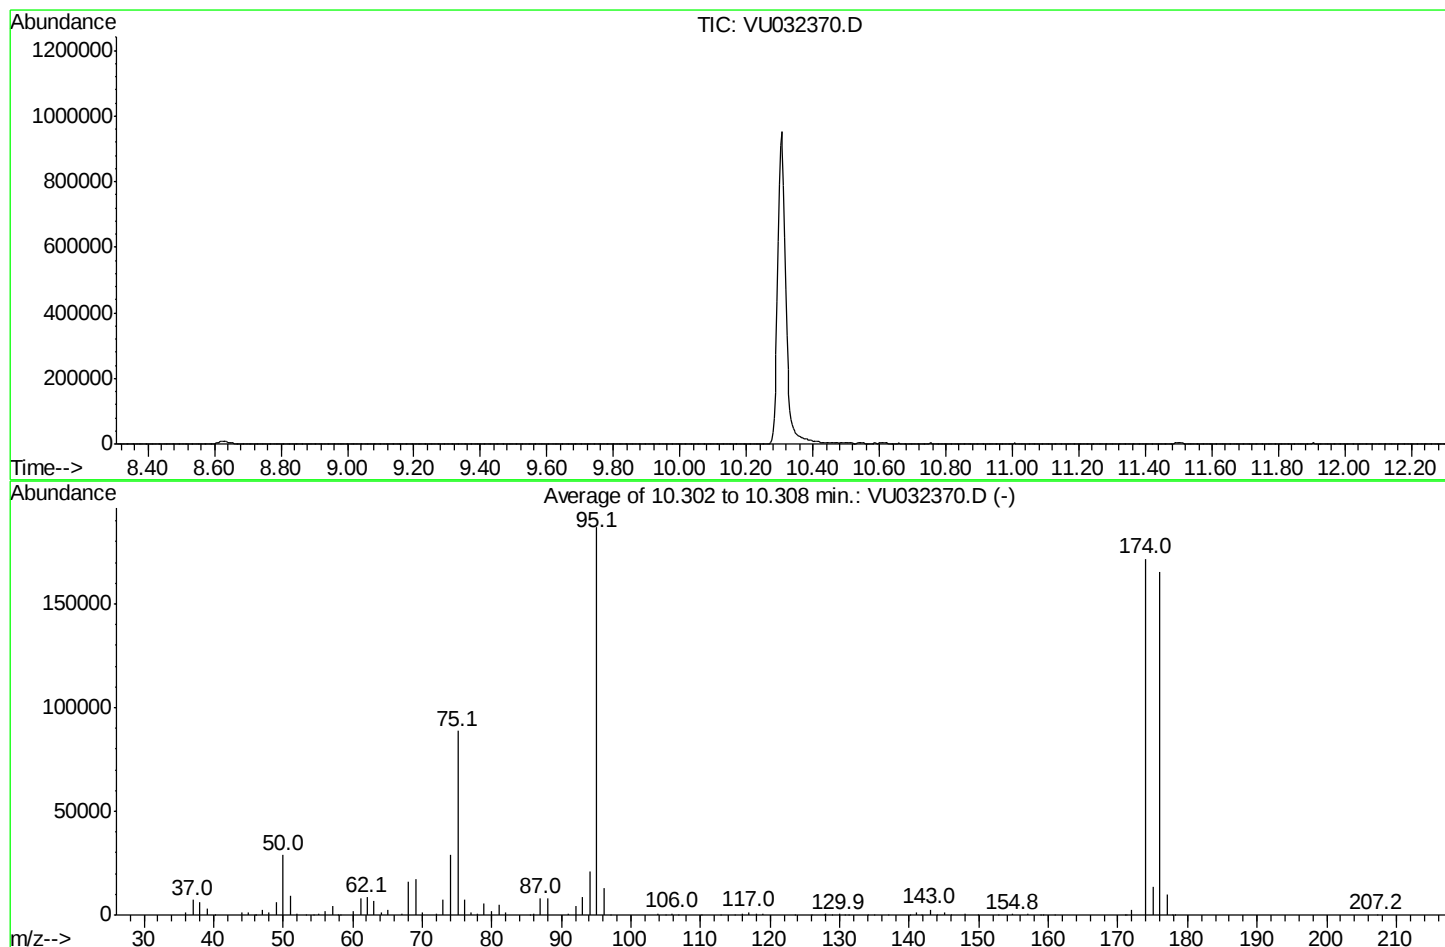

AutoFind: Scans 2865, 2866, 2867; Background Corrected with Scan 2853

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.5	29008	PASS
75	95	30	80	47.4	88704	PASS
95	95	100	100	100.0	186944	PASS
96	95	5	9	6.9	12891	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	91.9	171861	PASS
175	174	5	9	7.9	13626	PASS
176	174	95	101	96.1	165205	PASS
177	176	5	9	6.1	10122	PASS

Scan 2853 (10.263 min): VU032370.D
BFB47

m/z	Abundance
39.90	324.0
44.10	769.0
206.90	194.0

Instrument :
MSVOA_U
ClientSampleId :
BFB47

m/z	Abundance
36.00	1285.0
37.00	7221.0
38.00	6184.0
39.10	3223.0
40.00	393.0
44.00	1907.0
45.00	1391.0
45.90	231.0
46.20	196.0
47.00	2652.0
48.00	1040.0
49.10	6361.0
50.00	29008.0
51.00	9345.0
52.00	563.0
53.20	125.0
55.00	534.0
56.00	1998.0
57.00	4152.0
58.20	205.0
60.00	1844.0
61.10	7916.0
62.10	8260.0
63.10	7140.0
64.10	1360.0
65.10	2089.0
67.10	594.0
68.00	16375.0
69.10	17408.0
70.00	1348.0
72.00	866.0
73.00	7656.0
74.00	28952.0
75.10	88144.0
76.10	8002.0
77.00	1217.0
78.00	863.0
78.90	5894.0
80.00	1846.0
81.00	5261.0
81.90	1366.0
85.40	113.0
85.90	290.0
87.00	8250.0
88.00	7582.0
91.10	408.0
92.10	4416.0
93.10	8463.0
94.10	20592.0
95.10	186304.0
96.10	12756.0
97.00	236.0
104.00	670.0
105.00	361.0
106.00	576.0
106.80	253.0
112.90	133.0
114.90	258.0
116.00	649.0
117.00	1491.0
118.00	636.0
119.00	1036.0
125.90	158.0
127.70	583.0
128.90	228.0
129.90	516.0
130.80	291.0
134.10	107.0
135.00	260.0
136.90	332.0
140.00	201.0
140.90	1382.0
141.80	160.0
143.00	2837.0
144.00	228.0
145.00	1277.0
146.00	445.0
147.90	459.0
150.00	144.0
152.90	100.0
154.90	477.0
157.00	343.0
158.80	253.0
159.20	134.0
160.90	240.0
171.00	488.0
172.00	2646.0
174.00	165376.0
175.00	13474.0
176.00	159360.0
177.00	9874.0
177.90	167.0

Instrument :
MSVOA_U
ClientSampleId :
BFB47

m/z	Abundance
36.10	1462.0
37.10	7647.0
38.00	6105.0
39.10	3160.0
40.00	356.0
44.00	1799.0
45.00	1391.0
46.00	197.0
47.00	2690.0
48.00	995.0
49.10	6462.0
50.10	29768.0
51.00	9526.0
52.00	417.0
54.40	122.0
55.10	517.0
56.00	2110.0
57.10	4200.0
58.20	104.0
60.00	2043.0
61.10	7994.0
62.10	8837.0
63.10	7186.0
64.10	1494.0
65.10	2313.0
67.10	470.0
68.00	16720.0
69.10	17880.0
70.00	1397.0
72.00	925.0
73.00	7800.0
74.00	30080.0
75.10	91136.0
76.10	7896.0
77.00	1287.0
78.00	752.0
78.90	5884.0
80.00	1905.0
81.00	5398.0
81.90	1463.0
85.40	102.0
85.90	350.0
87.00	8029.0
88.00	8054.0
91.10	462.0
92.10	4308.0
93.10	9107.0
94.10	21792.0
95.10	193024.0
96.10	13305.0
97.00	330.0
103.90	656.0
105.10	305.0
106.00	678.0
106.80	279.0
113.00	199.0
114.90	278.0
115.90	685.0
117.00	1399.0
118.10	615.0
119.00	891.0
127.90	612.0
128.90	283.0
129.90	545.0
130.80	320.0
134.10	172.0
134.90	224.0
136.90	269.0
140.10	110.0
140.90	1475.0
141.80	194.0
143.00	2810.0
143.90	191.0
145.00	1161.0
146.00	241.0
147.90	438.0
150.00	233.0
154.80	567.0
157.00	360.0
158.80	347.0
160.90	291.0
170.90	448.0
171.30	463.0
172.00	2613.0
174.00	177600.0
175.00	14056.0
176.00	170880.0
177.00	10338.0
178.10	268.0

Instrument :
MSVOA_U
ClientSampleId :
BFB47

m/z	Abundance
36.10	1470.0
37.10	6797.0
38.00	5507.0
39.10	2707.0
40.20	302.0
44.00	1541.0
44.90	1290.0
46.10	236.0
47.00	2317.0
48.00	861.0
49.10	5964.0
50.10	28248.0
51.00	8958.0
52.00	290.0
54.40	112.0
55.10	469.0
56.00	2164.0
57.10	3797.0
57.90	114.0
60.00	1877.0
61.10	7530.0
62.10	8530.0
63.00	6732.0
64.00	1473.0
65.00	2196.0
68.00	15759.0
69.10	16912.0
70.00	1239.0
72.00	933.0
73.00	6999.0
74.10	28080.0
75.10	86832.0
76.10	7227.0
77.00	1201.0
77.90	711.0
78.90	5193.0
80.00	1811.0
81.00	5135.0
81.90	1390.0
86.00	351.0
87.00	7786.0
88.00	8075.0
90.90	553.0
92.10	4178.0
93.10	8563.0
94.10	21272.0
95.10	181504.0
96.10	12614.0
97.00	325.0
103.90	608.0
105.00	192.0
105.90	776.0
106.80	238.0
110.10	128.0
113.00	264.0
114.90	238.0
115.90	634.0
117.00	1062.0
118.10	553.0
118.90	631.0
123.60	104.0
127.90	640.0
129.00	335.0
130.00	595.0
130.80	234.0
131.20	136.0
134.00	176.0
134.80	187.0
136.90	263.0
140.10	100.0
141.00	1426.0
141.90	172.0
143.00	2442.0
143.90	173.0
145.00	887.0
145.90	184.0
148.00	361.0
149.90	299.0
152.70	108.0
154.80	525.0
157.00	295.0
158.80	275.0
160.90	265.0
171.20	452.0
172.00	2460.0
174.00	172608.0
175.00	13349.0
176.00	165376.0
177.00	10155.0
178.10	387.0
207.20	105.0

Instrument :
MSVOA_U
ClientSampleId :
BFB47