

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU053023\
 Data File : VU054321.D
 Acq On : 30 May 2023 18:08
 Operator : JC/MD
 Sample : 02936-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 54BR-20230524

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U052523W.M

Title : SW846 8260

Signal : TIC: VU054321.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.665	1020	1034	1051	rBV	26921	60783	4.64%	0.844%
2	4.809	1070	1079	1091	rBV2	7056	15125	1.16%	0.210%
3	5.282	1209	1226	1240	rBV	213008	451307	34.49%	6.269%
4	5.365	1240	1252	1280	rVB	336769	704999	53.87%	9.793%
5	5.693	1341	1354	1381	rBV	221112	458232	35.02%	6.365%
6	6.243	1511	1525	1551	rBV	484178	936468	71.56%	13.009%
7	6.539	1602	1617	1638	rBV	126241	241684	18.47%	3.357%
8	7.893	2023	2038	2063	rBV	748371	1308589	100.00%	18.178%
9	9.414	2497	2511	2535	rBV	657887	1109528	84.79%	15.413%
10	10.629	2875	2889	2909	rBV	511129	832231	63.60%	11.561%
11	11.806	3243	3255	3280	rBV	665659	1079779	82.51%	15.000%




Sum of corrected areas: 7198725

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU053023\
Data File : VU054321.D
Acq On : 30 May 2023 18:08
Operator : JC/MD
Sample : 02936-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
54BR-20230524

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U052523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

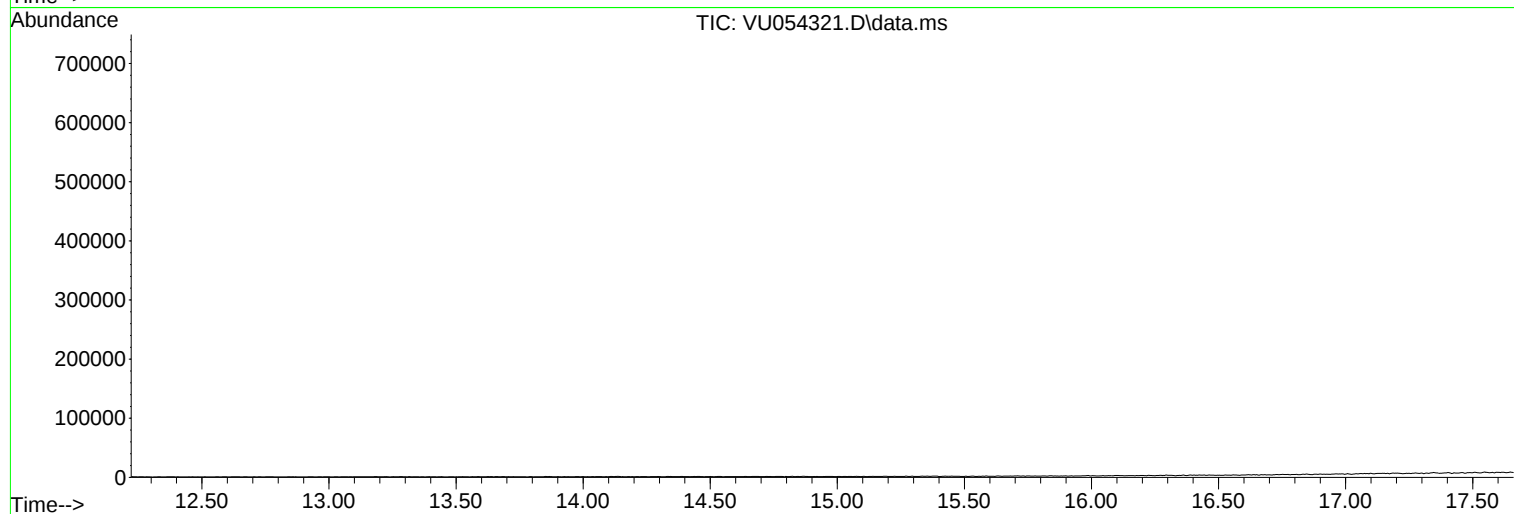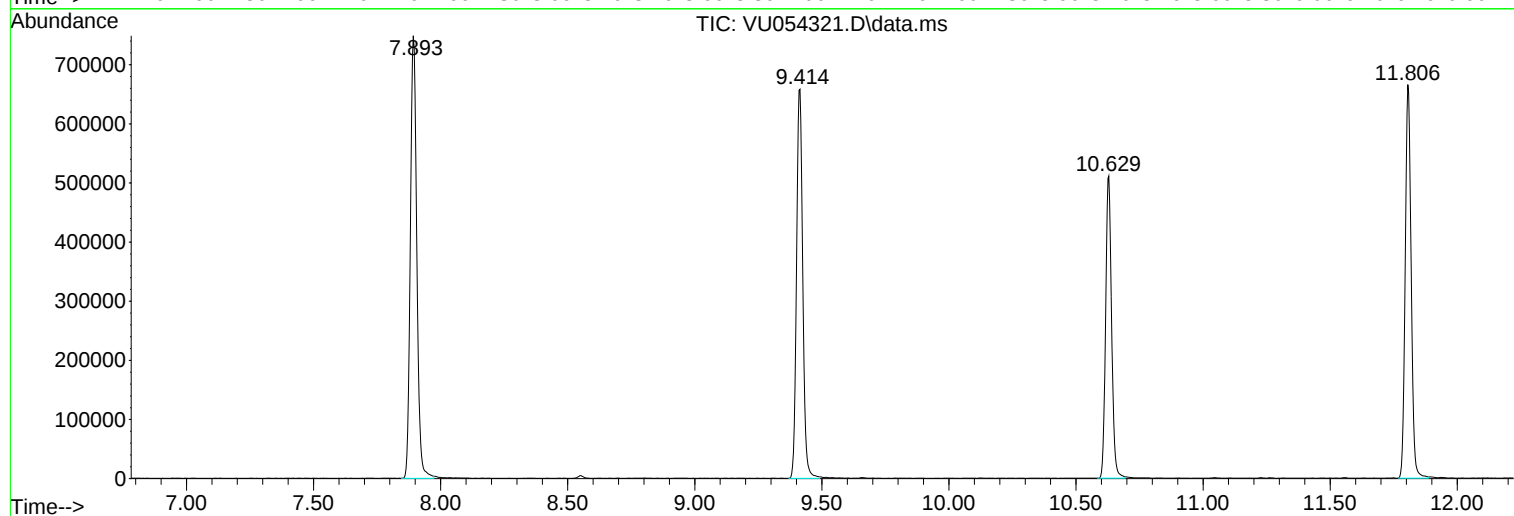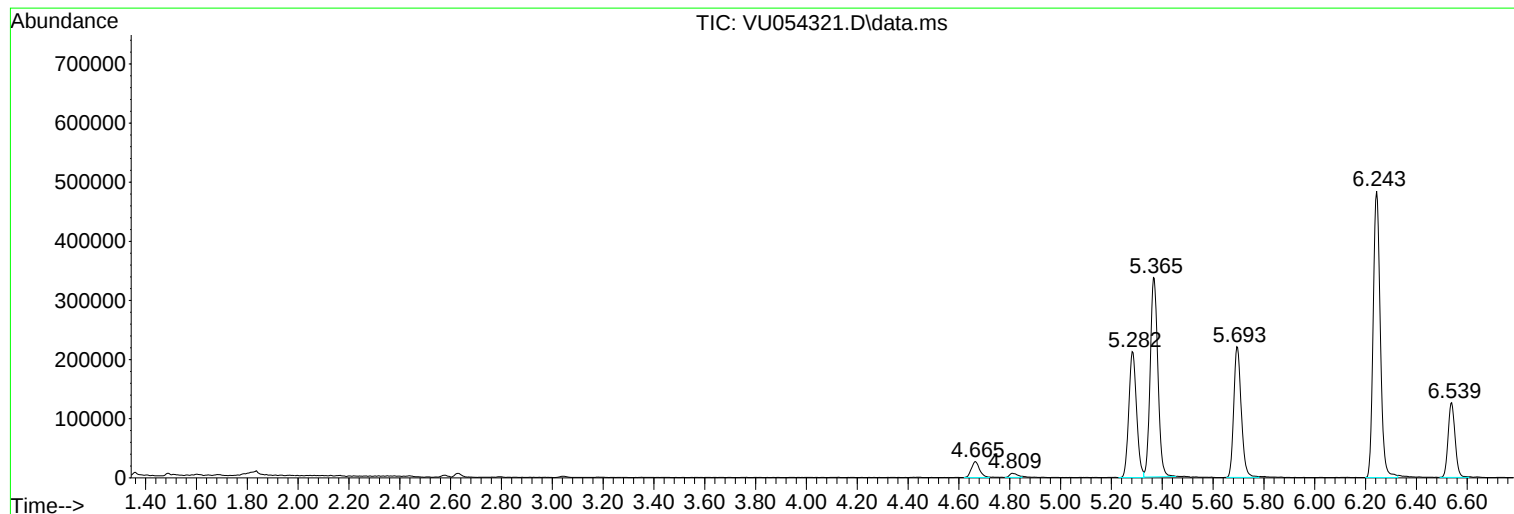

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU053023\
Data File : VU054321.D
Acq On : 30 May 2023 18:08
Operator : JC/MD
Sample : 02936-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
54BR-20230524

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U052523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU053023\
Data File : VU054321.D
Acq On : 30 May 2023 18:08
Operator : JC/MD
Sample : 02936-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
54BR-20230524

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U052523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------