

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU053024\
 Data File : VU059081.D
 Acq On : 30 May 2024 10:05
 Operator : MD/SY
 Sample : VU0530WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :

Quant Time: May 31 03:19:46 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri May 31 03:18:55 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.242	114	187474	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117	193730	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152	82181	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.595	65	53252	47.441	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	94.880%		
7) Chloroethane-d5	1.907	69	47942	49.860	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	99.720%		
11) 1,1-Dichloroethene-d2	2.560	63	73305	33.085	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	66.180%		
21) 2-Butanone-d5	4.611	46	102099	96.501	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	96.500%		
24) Chloroform-d	5.052	84	111845	50.052	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	100.100%		
26) 1,2-Dichloroethane-d4	5.692	65	71944	52.530	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	105.060%		
32) Benzene-d6	5.721	84	214230	48.181	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	96.360%		
36) 1,2-Dichloropropane-d6	6.682	67	75609	49.318	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	98.640%		
41) Toluene-d8	7.891	98	172344	45.659	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	91.320%		
43) trans-1,3-Dichloroprop...	8.174	79	29752	48.010	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	96.020%		
47) 2-Hexanone-d5	8.624	63	55777	78.675	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	78.680%		
56) 1,1,2,2-Tetrachloroeth...	10.749	84	116292	44.820	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	89.640%		
66) 1,2-Dichlorobenzene-d4	12.187	152	63274	51.593	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	103.180%		
Target Compounds					Qvalue	
37) 1,2-Dichloropropane	6.682	63	8035	4.045	ug/L #	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU053024\
Data File : VU059081.D
Acq On : 30 May 2024 10:05
Operator : MD/SY
Sample : VU0530WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :

Quant Time: May 31 03:19:46 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis
QLast Update : Fri May 31 03:18:55 2024
Response via : Initial Calibration

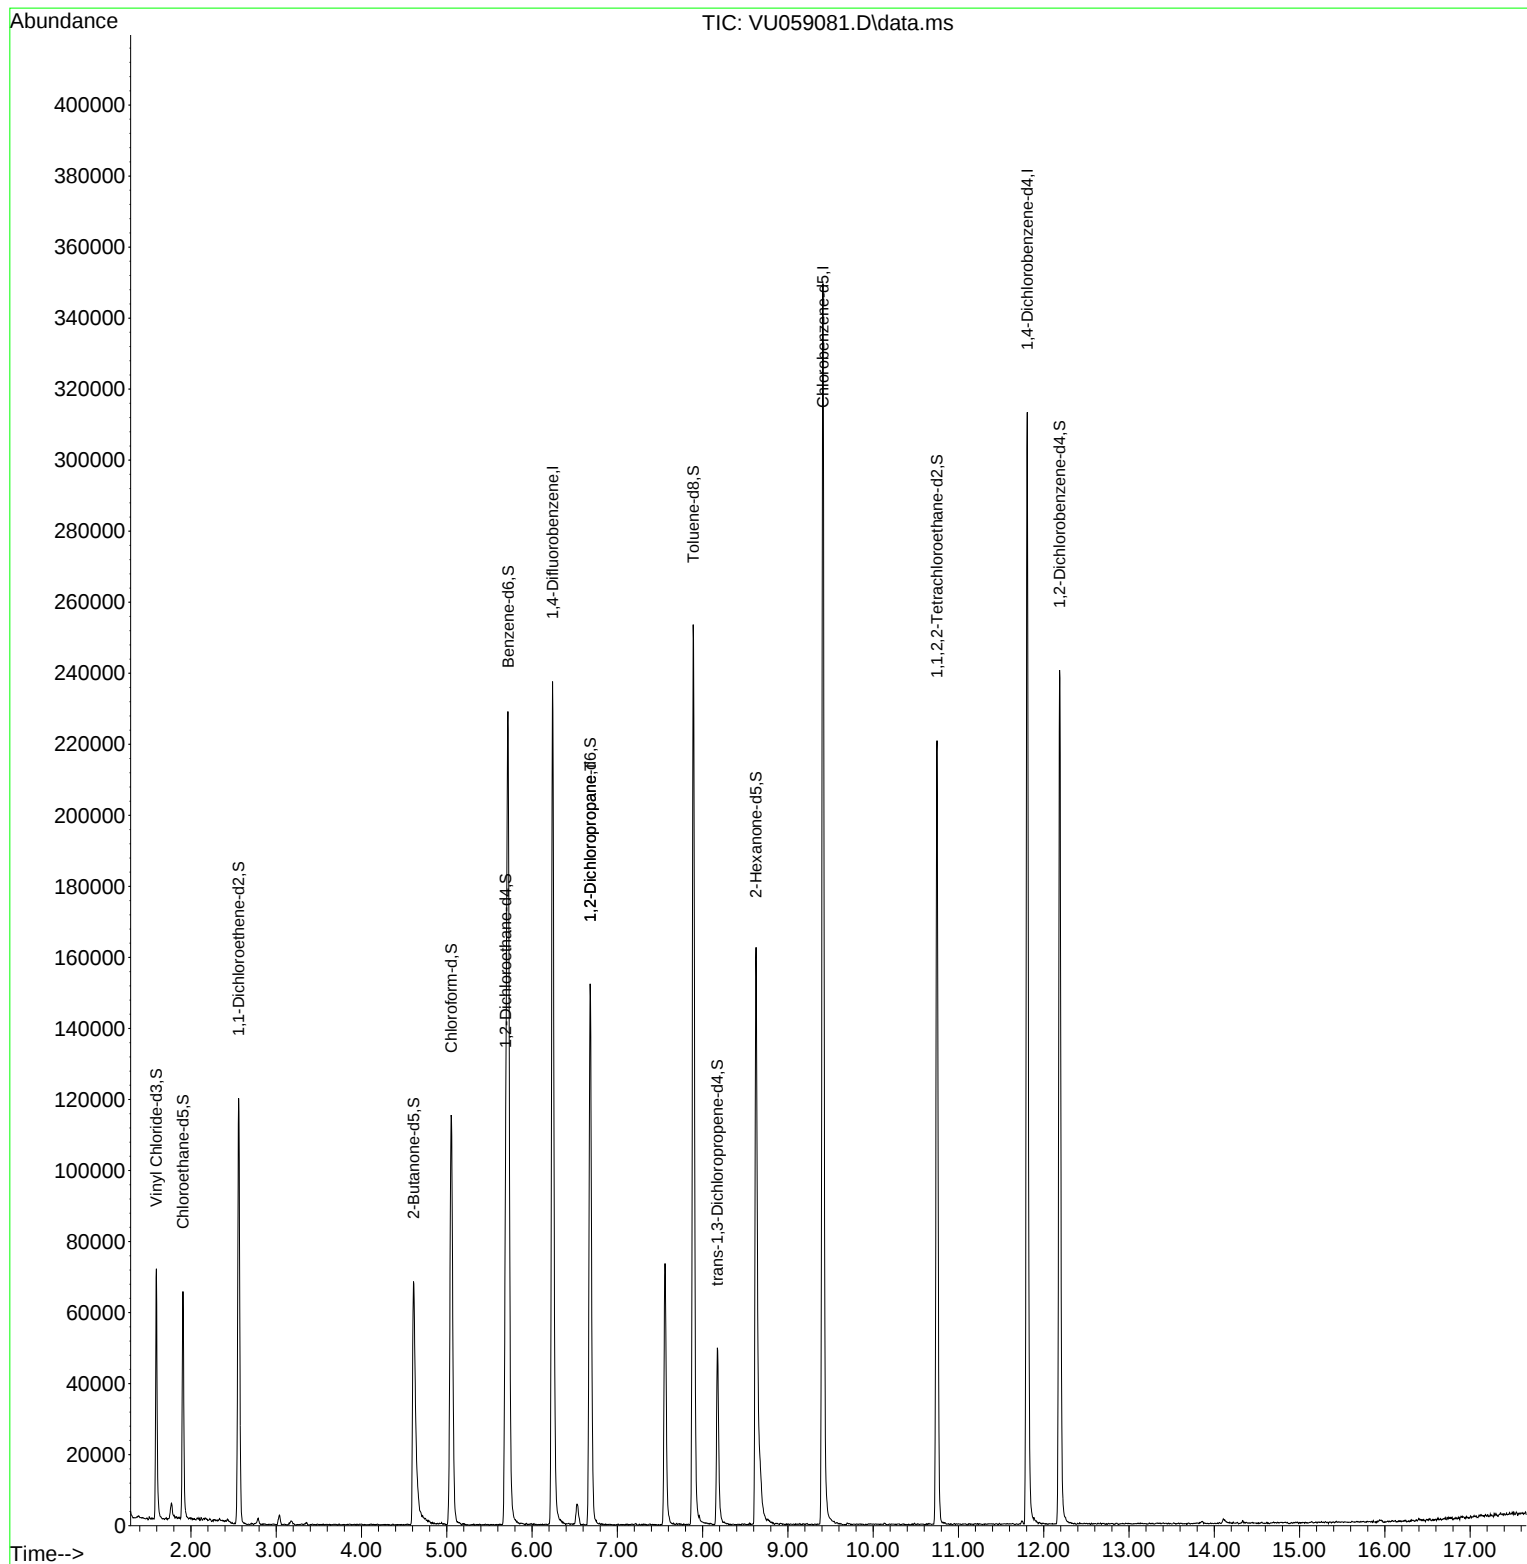

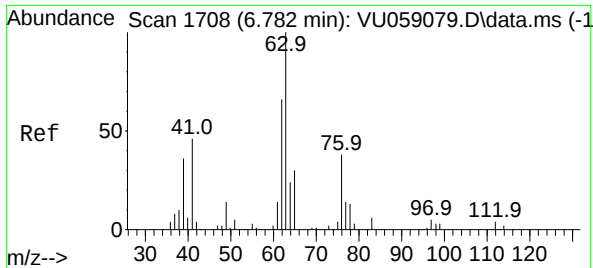

#37
 1,2-Dichloropropane
 Concen: 4.045 ug/L
 RT: 6.682 min Scan# 1
 Delta R.T. -0.100 min
 Lab File: VU059081.D
 Acq: 30 May 2024 10:05

Instrument :
 MSVOA_U
 ClientSampleId :

Tgt Ion: 63 Resp: 8035
 Ion Ratio Lower Upper
 63 100
 112 0.0 2.6 4.0#

