

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU053024\
 Data File : VU059094.D
 Acq On : 30 May 2024 15:12
 Operator : MD/SY
 Sample : P2623-07ME
 Misc : 5.45g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :

Quant Time: May 31 03:22:44 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri May 31 03:18:55 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.238	114	219014	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117	225771	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152	100884	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.592	65	62262	47.480	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	94.960%		
7) Chloroethane-d5	1.875	69	55622	49.516	ug/L	-0.03
Spiked Amount 50.000	Range 70 - 130		Recovery =	99.040%		
11) 1,1-Dichloroethene-d2	2.544	63	84182	32.523	ug/L	-0.02
Spiked Amount 50.000	Range 60 - 125		Recovery =	65.040%		
21) 2-Butanone-d5	4.615	46	112951	91.383	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	91.380%		
24) Chloroform-d	5.049	84	127314	48.770	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	97.540%		
26) 1,2-Dichloroethane-d4	5.689	65	85267	53.292	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	106.580%		
32) Benzene-d6	5.714	84	258974	49.978	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	99.960%		
36) 1,2-Dichloropropane-d6	6.679	67	89341	50.004	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	100.000%		
41) Toluene-d8	7.891	98	215153	48.911	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	97.820%		
43) trans-1,3-Dichloroprop...	8.174	79	36590	50.664	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	101.320%		
47) 2-Hexanone-d5	8.634	63	67700	81.941	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	81.940%		
56) 1,1,2,2-Tetrachloroeth...	10.753	84	135246	44.727	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	89.460%		
66) 1,2-Dichlorobenzene-d4	12.190	152	81229	53.954	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	107.900%		
Target Compounds						Qvalue
60) 1,2,3-Trichloropropane	11.807	75	14512	5.173	ug/L	# 68


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU053024\
Data File : VU059094.D
Acq On : 30 May 2024 15:12
Operator : MD/SY
Sample : P2623-07ME
Misc : 5.45g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :


Quant Time: May 31 03:22:44 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis
QLast Update : Fri May 31 03:18:55 2024
Response via : Initial Calibration

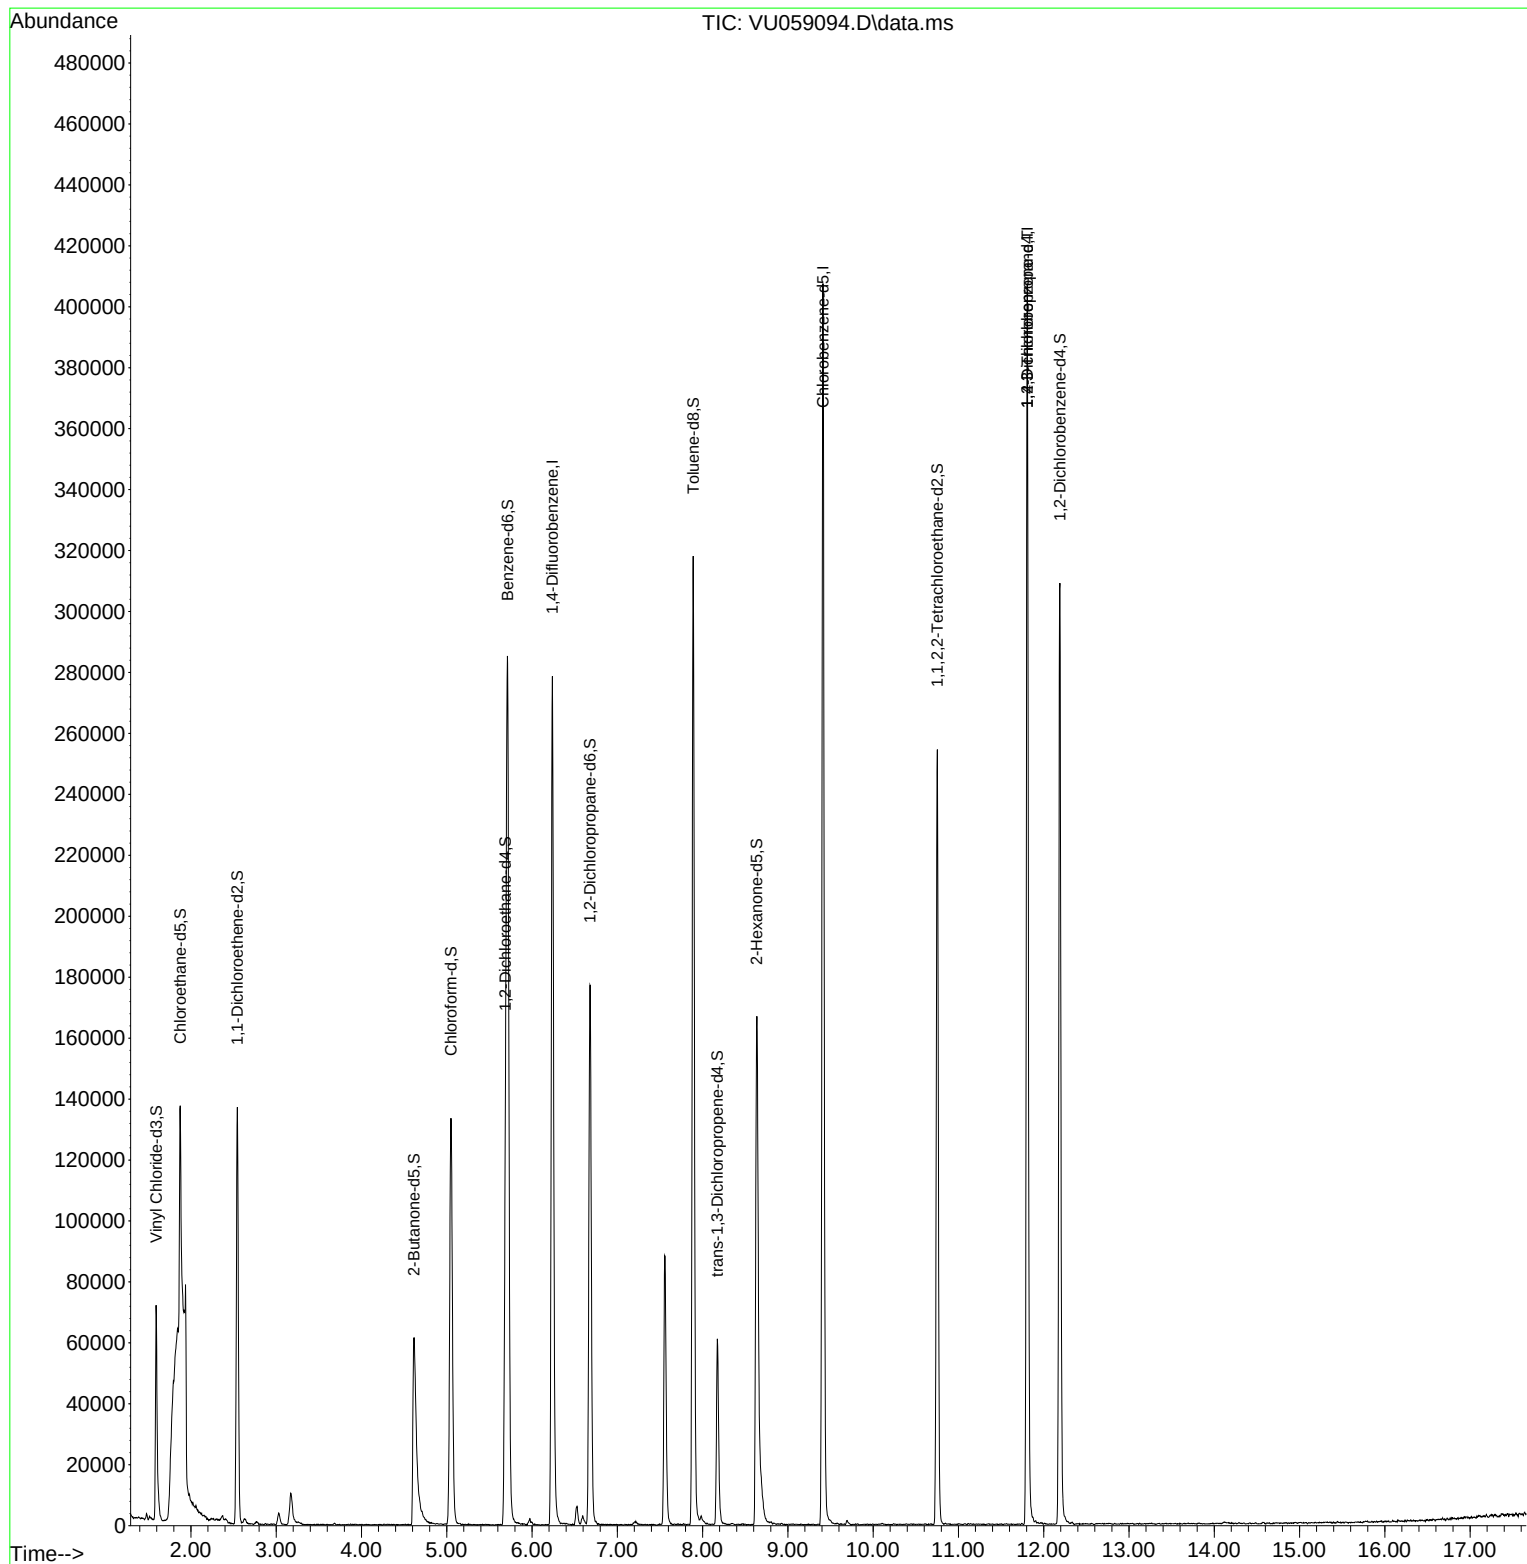

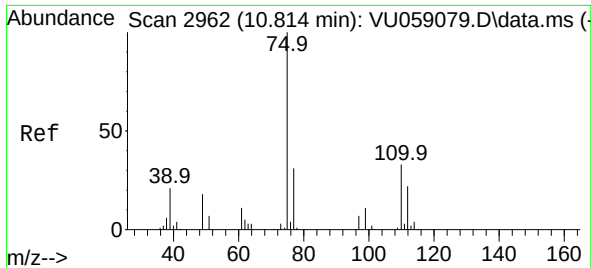

#60
1,2,3-Trichloropropane
Concen: 5.173 ug/L
RT: 11.807 min Scan# 31
Delta R.T. 0.994 min
Lab File: VU059094.D
Acq: 30 May 2024 15:12

Instrument :
MSVOA_U
ClientSampleId :

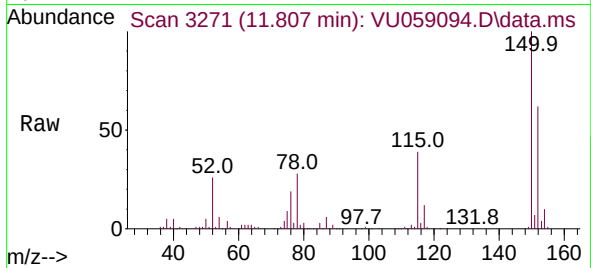

Tgt Ion: 75 Resp: 14512
Ion Ratio Lower Upper
75 100
77 31.7 26.2 39.2
110 1.0 28.4 42.6#

