

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU053024\
 Data File : VU059081.D
 Acq On : 30 May 2024 10:05
 Operator : MD/SY
 Sample : VU0530WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK060

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M

Title : VOC Analysis

Signal : TIC: VU059081.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.595	87	95	111	rBV	70401	85861	13.53%	1.673%
2	1.907	184	192	206	rBV	63639	83005	13.08%	1.618%
3	2.560	383	395	413	rBV	119773	194128	30.59%	3.783%
4	2.747	450	453	455	rBV2	365	301	0.05%	0.006%
5	3.039	535	544	552	rBV2	2839	4521	0.71%	0.088%
6	3.145	573	577	578	rBV	213	156	0.02%	0.003%
7	3.158	578	581	582	rBV2	407	230	0.04%	0.004%
8	3.232	602	604	606	rVB	77	35	0.01%	0.001%
9	3.251	606	610	613	rBV2	216	220	0.03%	0.004%
10	3.386	649	652	653	rBV	100	62	0.01%	0.001%
11	3.406	655	658	660	rVV	137	88	0.01%	0.002%
12	3.480	678	681	685	rBV2	272	298	0.05%	0.006%
13	3.512	689	691	695	rBV	186	171	0.03%	0.003%
14	3.644	730	732	734	rBV	184	114	0.02%	0.002%
15	3.740	756	762	765	rBV	391	420	0.07%	0.008%
16	3.894	807	810	811	rBV	136	76	0.01%	0.001%
17	3.949	824	827	832	rBV	333	296	0.05%	0.006%
18	3.975	832	835	837	rBV2	243	190	0.03%	0.004%
19	4.039	851	855	857	rBV2	173	97	0.02%	0.002%
20	4.091	869	871	873	rBV	141	37	0.01%	0.001%
21	4.113	873	878	882	rBV2	251	298	0.05%	0.006%
22	4.171	893	896	898	rBV	213	173	0.03%	0.003%
23	4.283	929	931	933	rBV2	177	113	0.02%	0.002%
24	4.328	943	945	949	rVB	172	137	0.02%	0.003%
25	4.370	952	958	962	rBV	317	422	0.07%	0.008%
26	4.412	968	971	973	rBV2	156	101	0.02%	0.002%
27	4.470	986	989	993	rBV2	188	144	0.02%	0.003%
28	4.512	999	1002	1005	rBV2	158	130	0.02%	0.003%
29	4.611	1021	1033	1064	rBV	68540	176016	27.74%	3.430%
30	4.833	1100	1102	1107	rBV2	322	245	0.04%	0.005%
31	4.965	1140	1143	1147	rBV3	223	199	0.03%	0.004%
32	4.994	1151	1152	1155	rBV	121	72	0.01%	0.001%
33	5.052	1155	1170	1192	rBV	115340	262067	41.30%	5.107%
34	5.193	1209	1214	1215	rBV2	385	273	0.04%	0.005%
35	5.203	1215	1217	1222	rVB2	297	207	0.03%	0.004%
36	5.245	1227	1230	1231	rBV	124	69	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU053024\
 Data File : VU059081.D
 Acq On : 30 May 2024 10:05
 Operator : MD/SY
 Sample : VU0530WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK060

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
 Title : VOC Analysis

37	5.290	1238	1244	1246	rBV	220	257	0.04%	0.005%
38	5.344	1255	1261	1263	rBV2	208	152	0.02%	0.003%
39	5.515	1309	1314	1317	rBV	270	273	0.04%	0.005%
40	5.618	1343	1346	1349	rBV2	237	204	0.03%	0.004%
41	5.717	1357	1377	1408	rBV2	228879	634557	100.00%	12.367%
42	5.920	1438	1440	1442	rBV	203	120	0.02%	0.002%
43	5.936	1442	1445	1449	rVB3	463	350	0.06%	0.007%
44	6.023	1469	1472	1476	rBV	329	190	0.03%	0.004%
45	6.242	1528	1540	1567	rBV	237117	454458	71.62%	8.857%
46	6.406	1588	1591	1594	rBV2	326	328	0.05%	0.006%
47	6.489	1615	1617	1619	rBV	267	152	0.02%	0.003%
48	6.528	1620	1629	1642	rVB5	5732	12004	1.89%	0.234%
49	6.682	1664	1677	1699	rBV2	152207	299504	47.20%	5.837%
50	6.859	1729	1732	1733	rBV	243	118	0.02%	0.002%
51	6.968	1763	1766	1769	rBV	185	92	0.01%	0.002%
52	6.991	1770	1773	1774	rBV2	166	100	0.02%	0.002%
53	7.065	1794	1796	1799	rBV2	137	116	0.02%	0.002%
54	7.097	1803	1806	1807	rBV	222	114	0.02%	0.002%
55	7.258	1852	1856	1860	rBV	270	230	0.04%	0.004%
56	7.290	1862	1866	1869	rVB2	254	204	0.03%	0.004%
57	7.309	1869	1872	1875	rBV	299	260	0.04%	0.005%
58	7.348	1882	1884	1887	rVB	199	71	0.01%	0.001%
59	7.377	1887	1893	1894	rBV	314	288	0.05%	0.006%
60	7.460	1916	1919	1922	rVB	142	94	0.01%	0.002%
61	7.486	1925	1927	1931	rVB	157	81	0.01%	0.002%
62	7.508	1931	1934	1935	rBV	143	66	0.01%	0.001%
63	7.518	1935	1937	1939	rBV	146	99	0.02%	0.002%
64	7.560	1939	1950	1970	rBV2	73527	132195	20.83%	2.576%
65	7.721	1997	2000	2001	rBV	253	156	0.02%	0.003%
66	7.775	2015	2017	2019	rBV	321	186	0.03%	0.004%
67	7.891	2041	2053	2073	rBV	253298	445786	70.25%	8.688%
68	8.123	2123	2125	2127	rBV	155	90	0.01%	0.002%
69	8.174	2131	2141	2160	rBV	49757	88815	14.00%	1.731%
70	8.344	2191	2194	2195	rBB	44	51	0.01%	0.001%
71	8.463	2228	2231	2236	rBV2	331	351	0.06%	0.007%
72	8.627	2271	2282	2319	rBV2	162415	340609	53.68%	6.638%
73	9.029	2404	2407	2412	rBV2	218	275	0.04%	0.005%
74	9.090	2423	2426	2428	rBV	262	130	0.02%	0.003%
75	9.344	2503	2505	2508	rBV	227	168	0.03%	0.003%
76	9.412	2514	2526	2565	rBV	349247	604540	95.27%	11.782%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU053024\
 Data File : VU059081.D
 Acq On : 30 May 2024 10:05
 Operator : MD/SY
 Sample : VU0530WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK060

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
 Title : VOC Analysis

77	9.653	2598	2601	2604	rBV2	141	104	0.02%	0.002%
78	9.695	2611	2614	2619	rBV3	415	425	0.07%	0.008%
79	9.913	2679	2682	2685	rBV2	229	166	0.03%	0.003%
80	10.132	2747	2750	2756	rVB3	383	446	0.07%	0.009%
81	10.325	2808	2810	2812	rBV2	122	63	0.01%	0.001%
82	10.415	2836	2838	2842	rVB2	177	103	0.02%	0.002%
83	10.447	2846	2848	2851	rBV2	181	110	0.02%	0.002%
84	10.749	2929	2942	2961	rBV	220663	365016	57.52%	7.114%
85	10.974	3009	3012	3017	rBV2	302	363	0.06%	0.007%
86	11.116	3053	3056	3058	rBV	324	210	0.03%	0.004%
87	11.183	3074	3077	3079	rBV	285	219	0.03%	0.004%
88	11.245	3093	3096	3099	rBV	280	227	0.04%	0.004%
89	11.296	3108	3112	3115	rBV	188	180	0.03%	0.004%
90	11.483	3165	3170	3173	rBV	415	427	0.07%	0.008%
91	11.743	3246	3251	3257	rBV5	891	1153	0.18%	0.022%
92	11.807	3260	3271	3293	rBV	313008	521015	82.11%	10.154%
93	12.058	3346	3349	3350	rBV	199	112	0.02%	0.002%
94	12.187	3377	3389	3418	rBV	240398	411436	64.84%	8.019%
95	12.560	3502	3505	3507	rBV2	340	188	0.03%	0.004%
96	12.759	3562	3567	3570	rBV	305	309	0.05%	0.006%




Sum of corrected areas: 5131078

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU053024\
Data File : VU059081.D
Acq On : 30 May 2024 10:05
Operator : MD/SY
Sample : VU0530WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK060

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

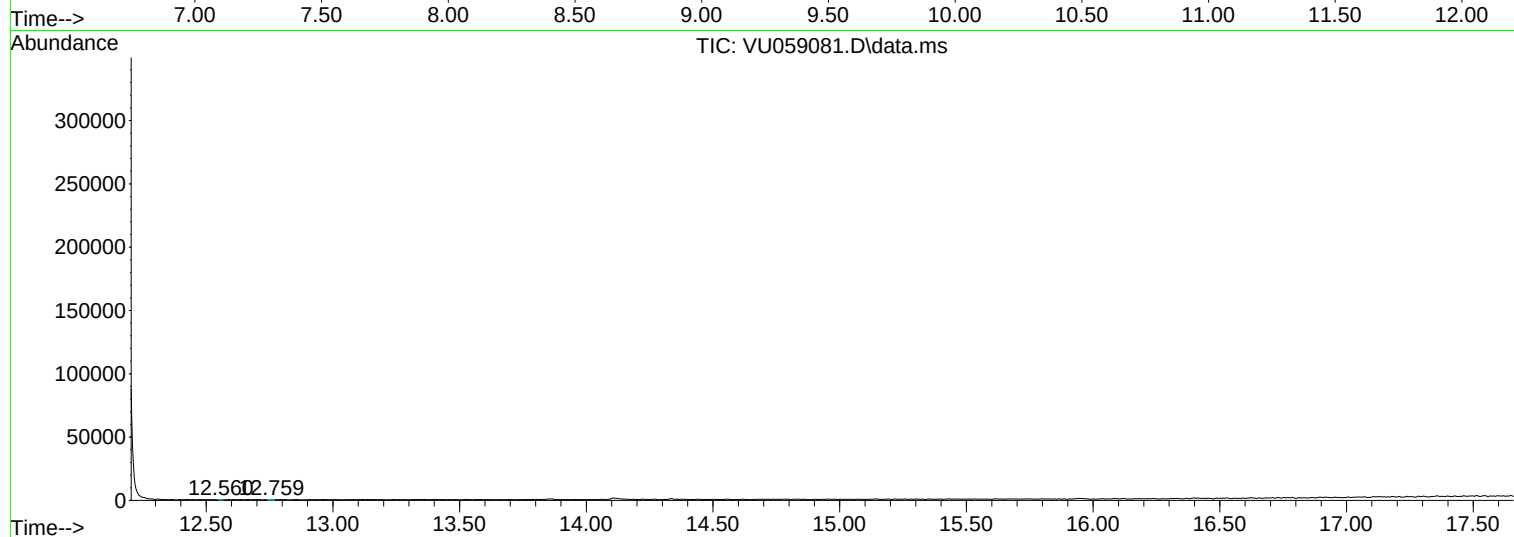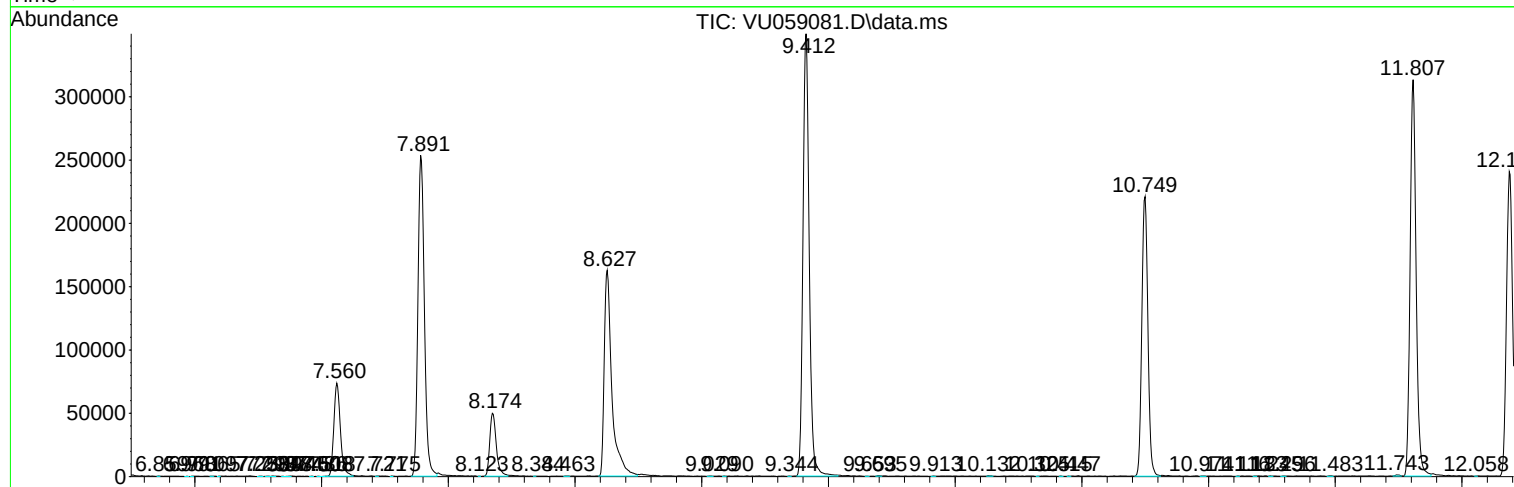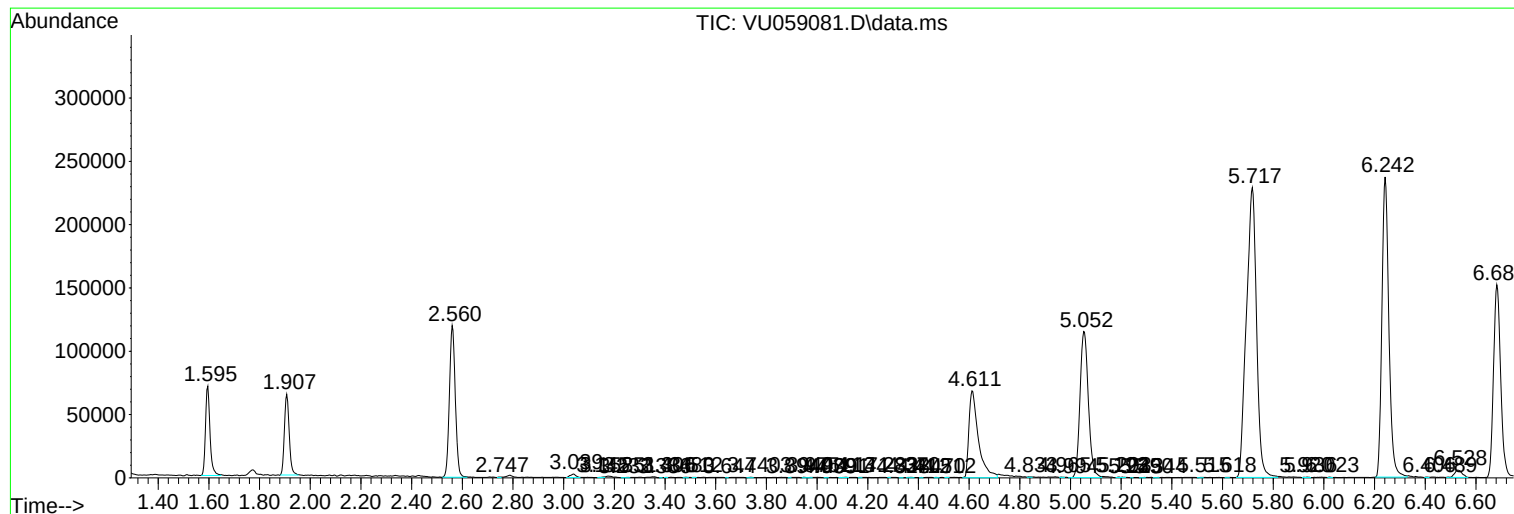

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU053024\
Data File : VU059081.D
Acq On : 30 May 2024 10:05
Operator : MD/SY
Sample : VU0530WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK060

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU053024\
Data File : VU059081.D
Acq On : 30 May 2024 10:05
Operator : MD/SY
Sample : VU0530WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK060

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc