


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU053024\
Data File : VU059078.D
Acq On : 30 May 2024 08:22
Operator : MD/SY
Sample : BFB056
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB056

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Title : VOC Analysis
Last Update : Sat Jun 01 01:17:21 2024

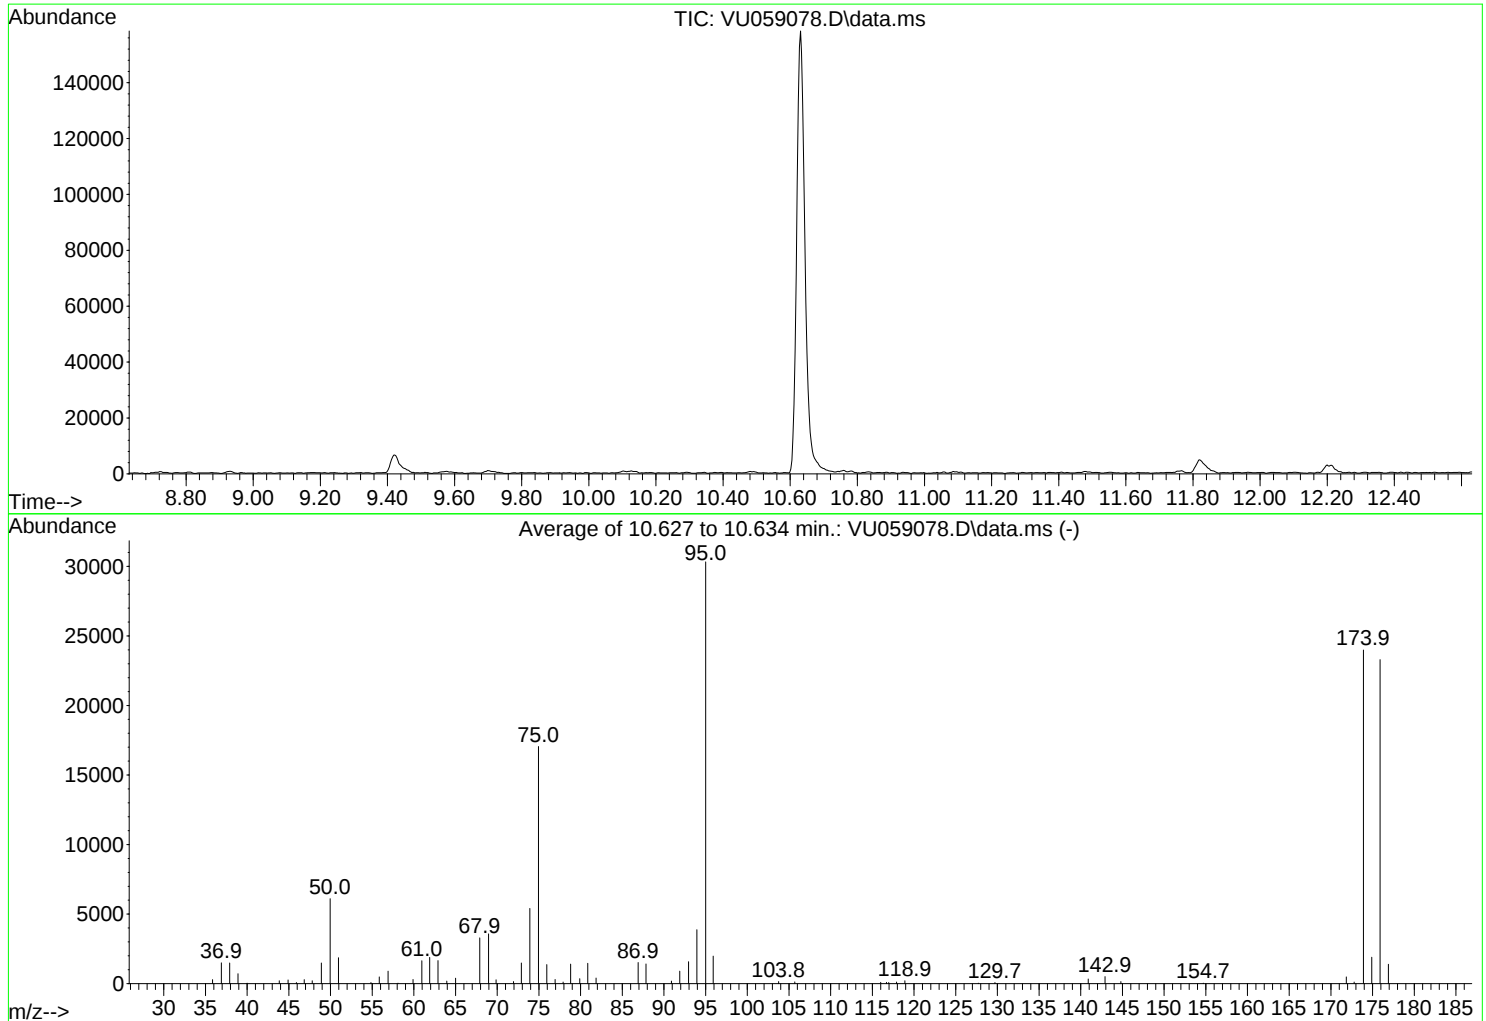

AutoFind: Scans 2904, 2905, 2906; Background Corrected with Scan 2893

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.2	6114	PASS
75	95	30	80	56.2	17047	PASS
95	95	100	100	100.0	30328	PASS
96	95	5	9	6.5	1977	PASS
173	174	0.00	2	0.5	112	PASS
174	95	50	120	79.1	23989	PASS
175	174	5	9	7.9	1893	PASS
176	174	95	101	97.1	23301	PASS
177	176	5	9	6.0	1388	PASS

m/z	Abundance
39.70	110.0
43.80	268.0

Instrument :
MSVOA_U
ClientSampleId :
BFB056

m/z	Abundance
35.90	280.0
36.90	1519.0
37.90	1490.0
38.90	698.0
40.00	113.0
43.90	430.0
44.90	261.0
45.90	109.0
46.90	317.0
47.80	207.0
48.90	1403.0
50.00	5992.0
50.90	1879.0
54.80	118.0
55.80	502.0
56.90	935.0
58.10	103.0
59.90	347.0
61.00	1647.0
61.90	1946.0
62.90	1669.0
64.00	184.0
65.00	369.0
67.90	3456.0
68.90	3830.0
69.80	329.0
72.00	153.0
72.90	1427.0
73.90	5458.0
75.00	17216.0
75.90	1354.0
77.00	289.0
78.80	1369.0
79.90	366.0
80.90	1459.0
81.80	360.0
86.90	1503.0
87.80	1394.0
90.90	196.0
91.90	913.0
92.90	1546.0
93.90	3835.0
95.00	30336.0
95.90	1896.0
103.70	123.0
105.70	109.0
116.00	148.0
117.00	101.0
117.90	110.0
118.80	238.0
129.70	132.0
140.90	301.0
142.90	481.0
144.80	125.0
171.80	471.0
173.90	23288.0
174.90	1871.0
175.90	22592.0
176.90	1403.0

Instrument :
MSVOA_U
ClientSampleId :
BFB056

m/z	Abundance
35.90	294.0
36.90	1529.0
37.90	1587.0
38.90	743.0
43.90	497.0
44.90	278.0
45.90	122.0
46.80	289.0
47.80	213.0
48.90	1569.0
49.90	6272.0
50.90	1912.0
54.90	116.0
55.90	475.0
56.90	915.0
59.90	313.0
60.90	1676.0
61.90	1972.0
62.90	1724.0
64.00	180.0
65.00	395.0
67.90	3314.0
68.90	3654.0
69.90	265.0
72.00	157.0
72.90	1537.0
73.90	5574.0
74.90	17664.0
75.90	1405.0
77.00	320.0
78.00	148.0
78.80	1425.0
79.90	369.0
80.90	1502.0
81.90	404.0
86.90	1539.0
87.80	1453.0
90.90	195.0
91.90	899.0
93.00	1642.0
94.00	4020.0
95.00	30992.0
95.90	2007.0
103.80	155.0
105.70	130.0
116.00	128.0
116.70	131.0
116.90	129.0
117.90	117.0
118.90	195.0
129.70	116.0
140.90	361.0
142.90	533.0
144.80	163.0
154.70	103.0
171.90	509.0
173.90	24760.0
174.90	1954.0
175.90	24016.0
176.90	1386.0

Instrument :
MSVOA_U
ClientSampleId :
BFB056

m/z	Abundance
35.90	282.0
36.90	1443.0
37.90	1388.0
38.90	710.0
39.70	114.0
43.90	491.0
44.90	262.0
46.80	265.0
47.80	207.0
48.90	1465.0
49.90	6077.0
51.00	1785.0
55.90	457.0
56.90	844.0
59.90	225.0
60.90	1621.0
61.90	1741.0
62.90	1571.0
63.90	185.0
65.00	404.0
67.90	3088.0
69.00	3249.0
69.90	237.0
71.90	128.0
72.90	1495.0
73.90	5176.0
74.90	16260.0
76.00	1342.0
76.90	273.0
77.80	195.0
78.80	1428.0
79.90	333.0
80.80	1407.0
81.90	454.0
86.90	1503.0
87.90	1393.0
90.90	171.0
91.90	865.0
93.00	1556.0
94.00	3769.0
95.00	29656.0
95.90	2029.0
103.80	177.0
105.70	154.0
116.70	153.0
117.90	129.0
119.00	184.0
127.70	117.0
140.90	327.0
142.90	522.0
144.80	157.0
171.90	475.0
172.80	335.0
173.90	23920.0
174.90	1855.0
175.90	23296.0
176.90	1376.0

Instrument :
MSVOA_U
ClientSampleId :
BFB056