

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU053120\
 Data File : VU038453.D
 Acq On : 31 May 2020 07:23
 Operator : JC/MD
 Sample : L2788-15
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFXB9

Quant Time: Jun 01 06:31:56 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR053120WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Mon Jun 01 06:27:31 2020
 Response via : Initial Calibration

Manual Integrations
 APPROVED

MMDadoda
 6/1/2020 4:21:46 PM

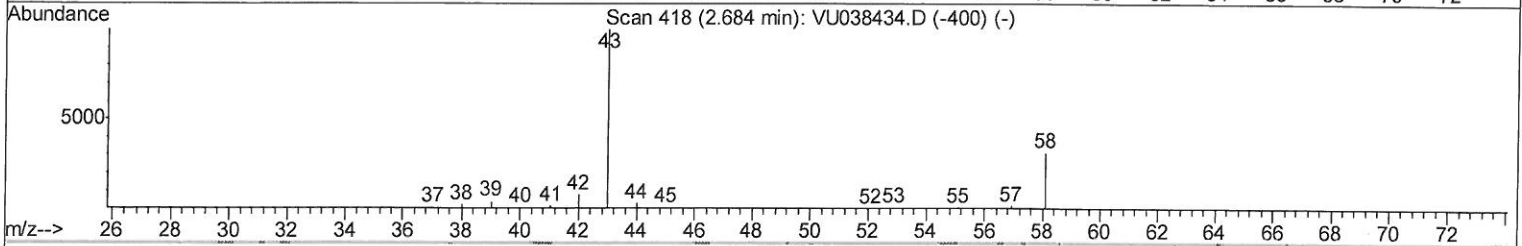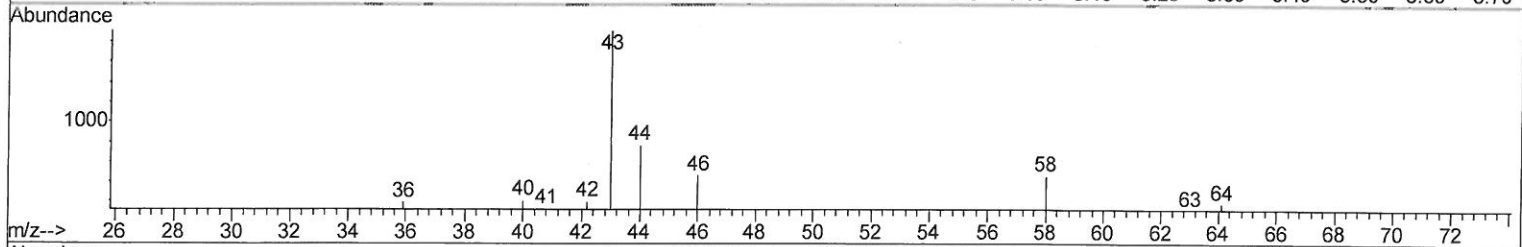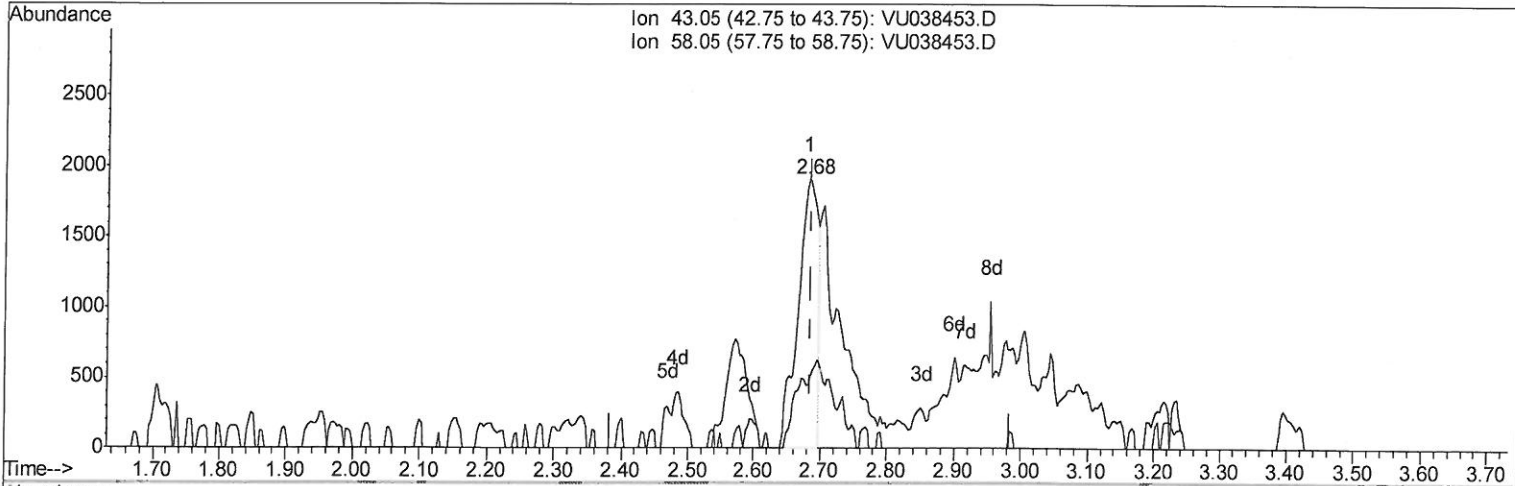

TIC: VU038453.D

(13) Acetone (T)
 2.681min (-0.003) 0.98ug/L
 response 4003

Ion	Exp%	Act%
43.05	100	100
58.05	32.80	16.66
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU053120\
 Data File : VU038453.D
 Acq On : 31 May 2020 07:23
 Operator : JC/MD
 Sample : L2788-15
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFXB9

Quant Time: Jun 01 06:31:56 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR053120WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Mon Jun 01 06:27:31 2020
 Response via : Initial Calibration

Manual Integrations
 APPROVED

MMDadoda
 6/1/2020 4:21:46 PM

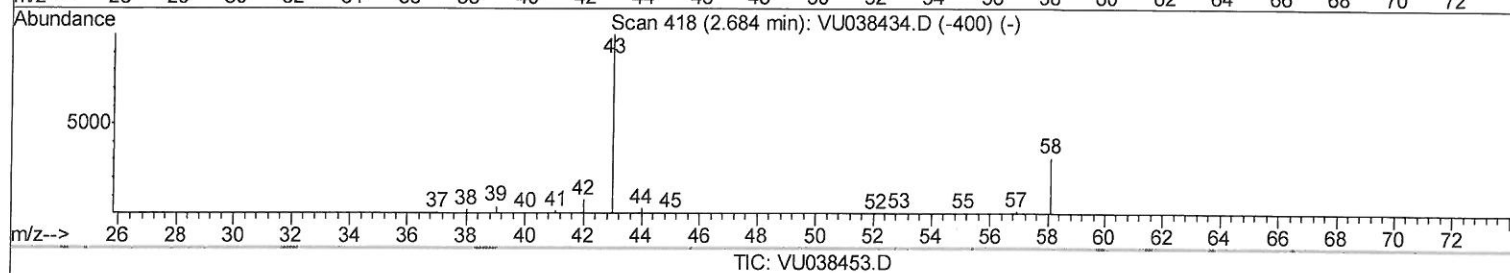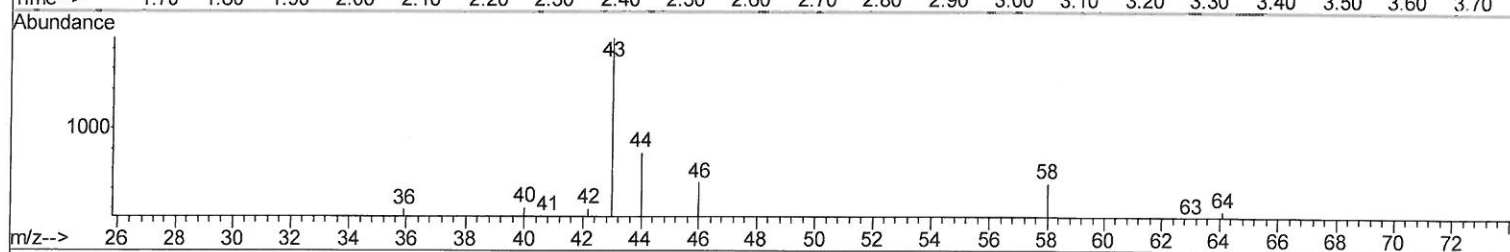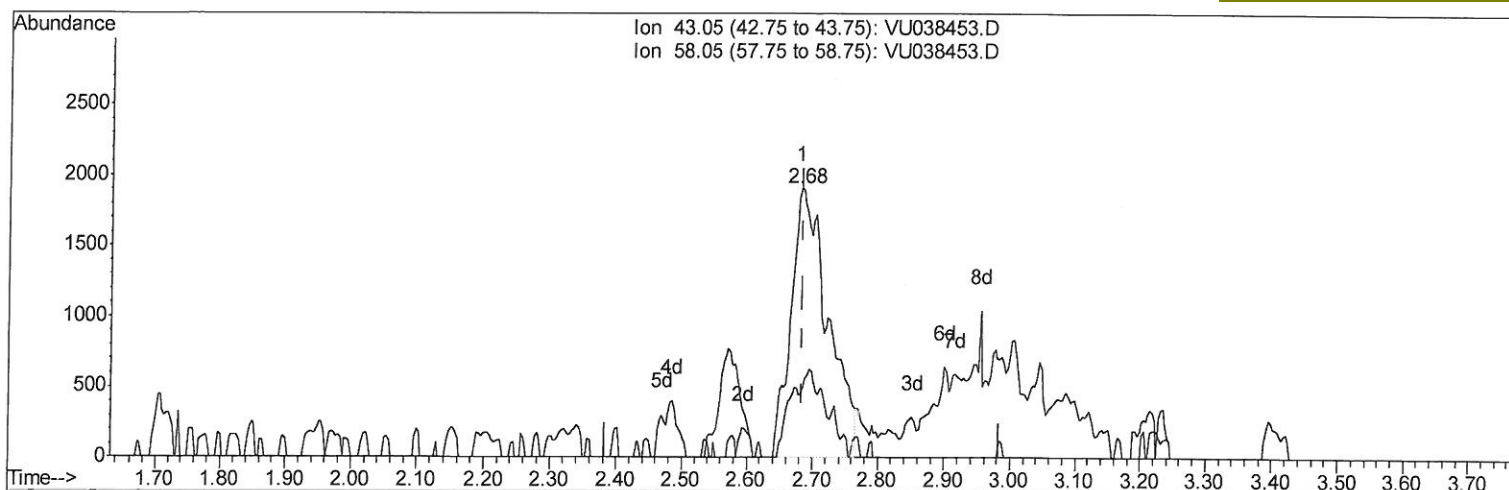

(13) Acetone (T)

2.681min (-0.003) 1.83ug/L m

response 7481

Ion	Exp%	Act%
43.05	100	100
58.05	32.80	8.92
0.00	0.00	0.00
0.00	0.00	0.00

> 06/01/2020

Quantitation Report (QT Reviewed)

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU053120\
 Data File : VU038453.D
 Acq On : 31 May 2020 07:23
 Operator : JC/MD
 Sample : L2788-15
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 Client Sample ID :
 BFXB9

Quant Time: Jun 01 08:24:42 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR053120WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Mon Jun 01 06:27:31 2020
 Response via : Initial Calibration

Manual Integrations
 APPROVED

MMDadoda
 6/1/2020 4:21:46 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.28	114	317563	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.44	117	308534	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.82	152	146728	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.61	65	93976	4.57	ug/L	0.00
Spiked Amount 5.000	Range 40 - 130		Recovery = 91.40%			
7) Chloroethane-d5	1.93	69	79038	5.00	ug/L	0.00
Spiked Amount 5.000	Range 65 - 130		Recovery = 100.00%			
11) 1,1-Dichloroethene-d2	2.59	63	141102	3.49	ug/L	0.00
Spiked Amount 5.000	Range 60 - 125		Recovery = 69.80%			
20) 2-Butanone-d5	4.68	46	363539	58.23	ug/L	0.00
Spiked Amount 50.000	Range 40 - 130		Recovery = 116.46%			
24) Chloroform-d	5.10	84	194753	5.04	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery = 100.80%			
26) 1,2-Dichloroethane-d4	5.74	65	116710	5.32	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery = 106.40%			
32) Benzene-d6	5.76	84	384319	4.99	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery = 99.80%			
36) 1,2-Dichloropropane-d6	6.72	67	120074	5.07	ug/L	0.00
Spiked Amount 5.000	Range 60 - 140		Recovery = 101.40%			
41) Toluene-d8	7.92	98	315933	4.57	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery = 91.40%			
43) trans-1,3-Dichloropropene-	8.20	79	46385	4.55	ug/L	0.00
Spiked Amount 5.000	Range 55 - 130		Recovery = 91.00%			
46) 2-Hexanone-d5	8.66	63	306256	60.88	ug/L	0.00
Spiked Amount 50.000	Range 45 - 130		Recovery = 121.76%			
57) 1,1,2,2-Tetrachloroethane-	10.77	84	108133	5.38	ug/L	0.00
Spiked Amount 5.000	Range 65 - 120		Recovery = 107.60%			
64) 1,2-Dichlorobenzene-d4	12.20	152	132535	5.24	ug/L	0.00
Spiked Amount 5.000	Range 80 - 120		Recovery = 104.80%			

Target Compounds

					Ovalue
10) 1,1,2-Trichloro-1,2,2-trif	2.60	101	4633	0.241 ug/L	# 78
13) Acetone	2.68	43	7481m	1.831 ug/L	100
22) cis-1,2-Dichloroethene	4.71	96	29170	1.285 ug/L	94
34) Trichloroethene	6.57	95	39220	1.756 ug/L	89
47) Tetrachloroethene	8.57	164	13736	0.847 ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU053120\
Data File : VU038453.D
Acq On : 31 May 2020 07:23
Operator : JC/MD
Sample : L2788-15
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFXB9

Quant Time: Jun 01 08:24:42 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR053120WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Mon Jun 01 06:27:31 2020
Response via : Initial Calibration

Manual Integrations
APPROVED

MMDadoda
6/1/2020 4:21:46 PM

