

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU053120\
 Data File : VU038414.D
 Acq On : 30 May 2020 15:38
 Operator : JC/MD
 Sample : L2749-10
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK01

Quant Time: Jun 01 03:10:05 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR053120WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Mon Jun 01 02:37:32 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.28	114	324459	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.44	117	315929	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.83	152	153785	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.61	65	104379	4.97	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	99.40%
7) Chloroethane-d5	1.93	69	79257	4.91	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	98.20%
11) 1,1-Dichloroethene-d2	2.59	63	148901	3.60	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	72.00%
20) 2-Butanone-d5	4.68	46	318328	49.90	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	99.80%
24) Chloroform-d	5.10	84	183480	4.65	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.00%
26) 1,2-Dichloroethane-d4	5.74	65	111797	4.99	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	99.80%
32) Benzene-d6	5.76	84	391635	4.97	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.40%
36) 1,2-Dichloropropane-d6	6.72	67	117864	4.86	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	97.20%
41) Toluene-d8	7.92	98	339021	4.79	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	95.80%
43) trans-1,3-Dichloropropene-	8.20	79	48274	4.63	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	92.60%
46) 2-Hexanone-d5	8.66	63	271251	52.66	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	105.32%
57) 1,1,2,2-Tetrachloroethane-	10.77	84	99326	4.82	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	96.40%
64) 1,2-Dichlorobenzene-d4	12.20	152	130979	4.94	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	98.80%


Target Compounds					Ovalue
16) Methylene chloride	3.08	84	1653	0.073 ug/L	80


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU053120\
Data File : VU038414.D
Acq On : 30 May 2020 15:38
Operator : JC/MD
Sample : L2749-10
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK01

Quant Time: Jun 01 03:10:05 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR053120WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Mon Jun 01 02:37:32 2020
Response via : Initial Calibration

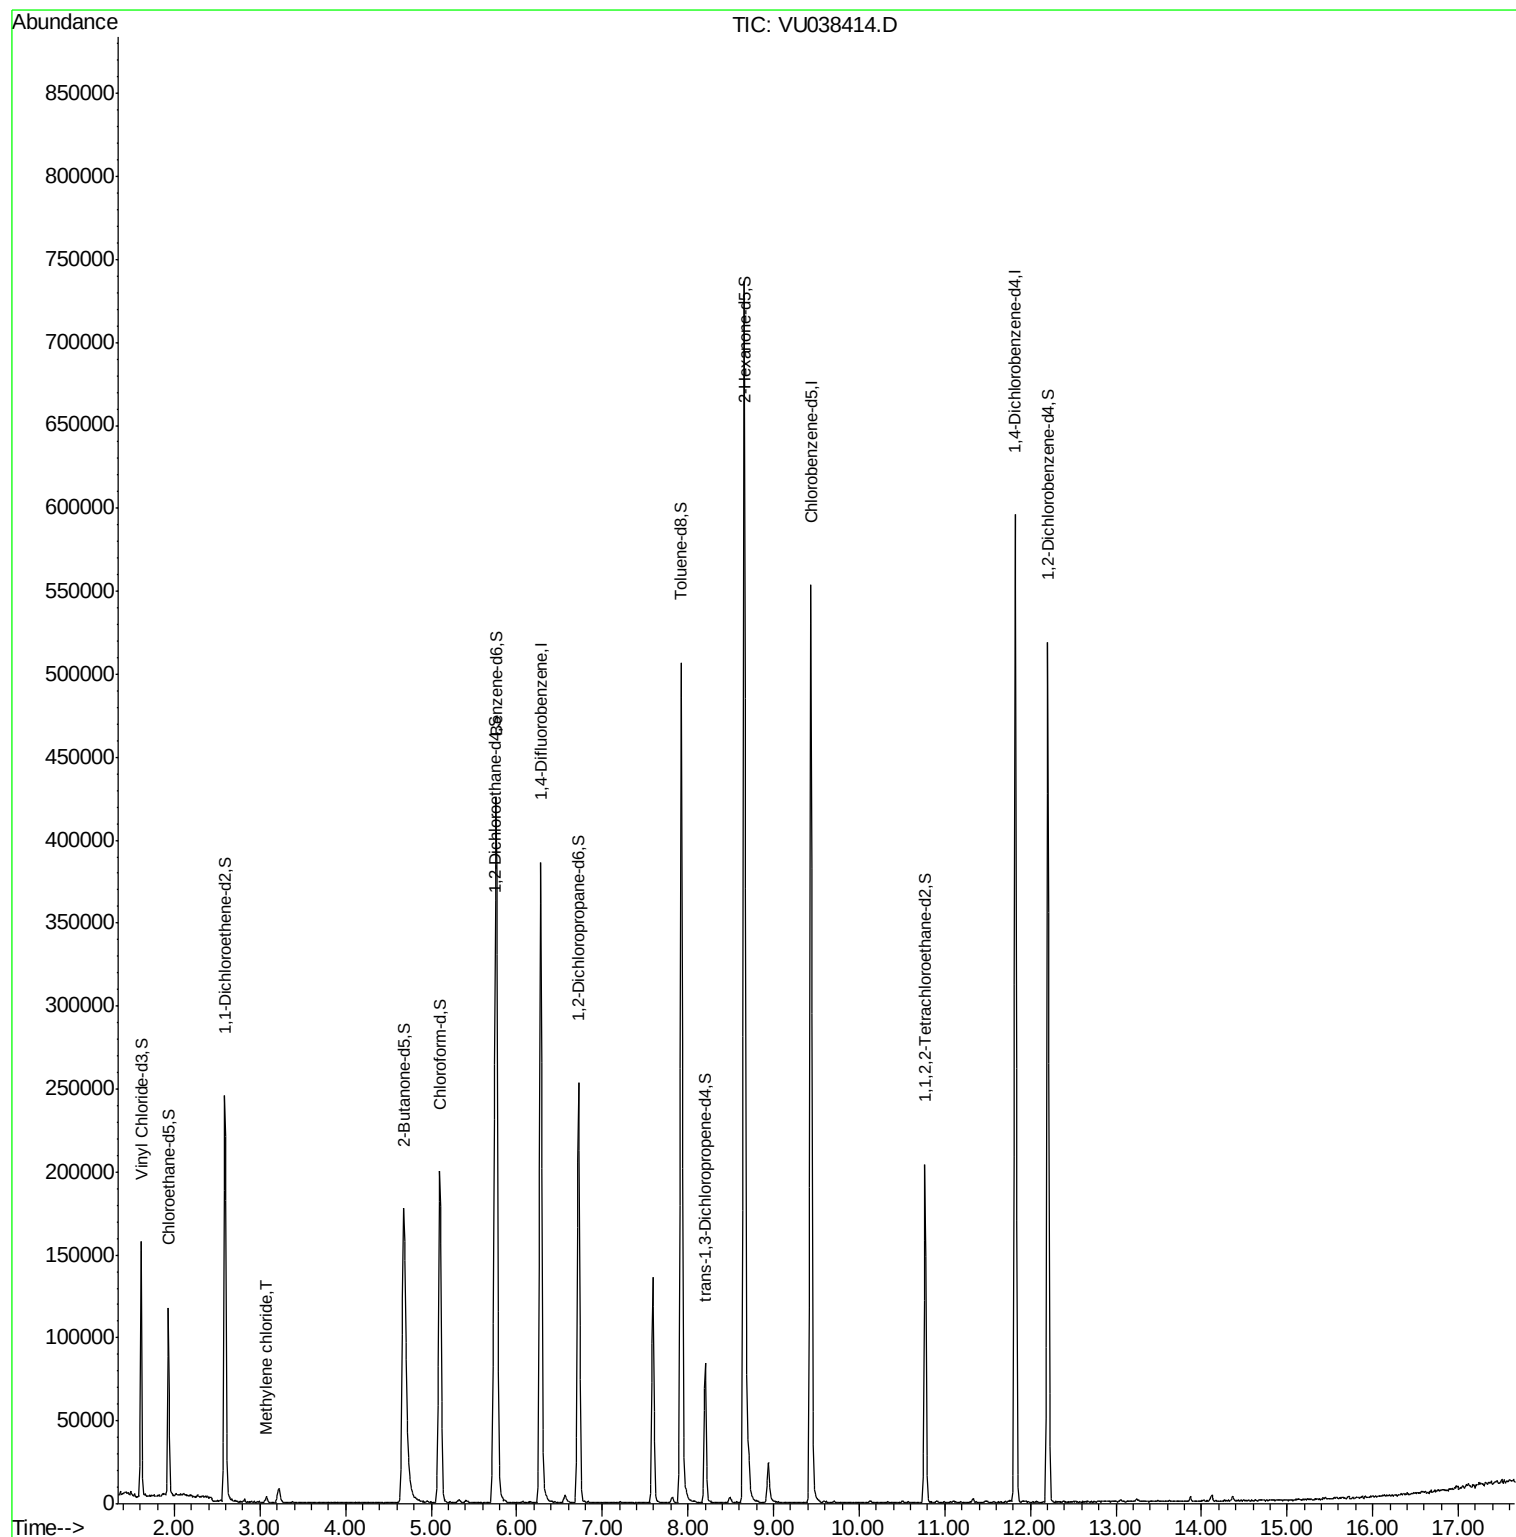

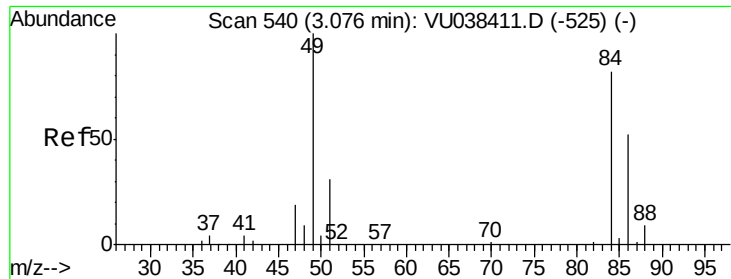

#16
 Methylene chloride
 Concen: 0.073 ug/L
 RT: 3.08 min Scan# 540
 Delta R.T. -0.00 min
 Lab File: VU038414.D
 Acq: 30 May 2020 15:38

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK01

Tot Ion: 84 Resp: 1653
 Ion Ratio Lower Upper
 84 100
 86 54.3 45.0 83.6
 49 95.4 85.5 158.9

