

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU053120\
 Data File : VU038427.D
 Acq On : 30 May 2020 20:38
 Operator : JC/MD
 Sample : L2787-06
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFX84

Quant Time: Jun 01 04:50:29 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR053120WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Mon Jun 01 02:37:32 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.28	114	319730	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.44	117	313240	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.83	152	150096	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.61	65	101551	4.91	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	98.20%
7) Chloroethane-d5	1.93	69	81263	5.11	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	102.20%
11) 1,1-Dichloroethene-d2	2.59	63	145842	3.58	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	71.60%
20) 2-Butanone-d5	4.67	46	359090	57.12	ug/L	-0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	114.24%
24) Chloroform-d	5.10	84	195987	5.04	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	100.80%
26) 1,2-Dichloroethane-d4	5.74	65	119401	5.41	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	108.20%
32) Benzene-d6	5.76	84	405793	5.19	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	103.80%
36) 1,2-Dichloropropane-d6	6.72	67	123404	5.13	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	102.60%
41) Toluene-d8	7.92	98	336051	4.79	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	95.80%
43) trans-1,3-Dichloropropene-	8.20	79	50525	4.88	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	97.60%
46) 2-Hexanone-d5	8.65	63	309781	60.66	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	121.32%
57) 1,1,2,2-Tetrachloroethane-	10.77	84	109220	5.35	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	107.00%
64) 1,2-Dichlorobenzene-d4	12.20	152	139770	5.40	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	108.00%


Target Compounds					Ovalue
13) Acetone	2.68	43	20344	4.945 ug/L	72


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU053120\
Data File : VU038427.D
Acq On : 30 May 2020 20:38
Operator : JC/MD
Sample : L2787-06
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFX84

Quant Time: Jun 01 04:50:29 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR053120WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Mon Jun 01 02:37:32 2020
Response via : Initial Calibration

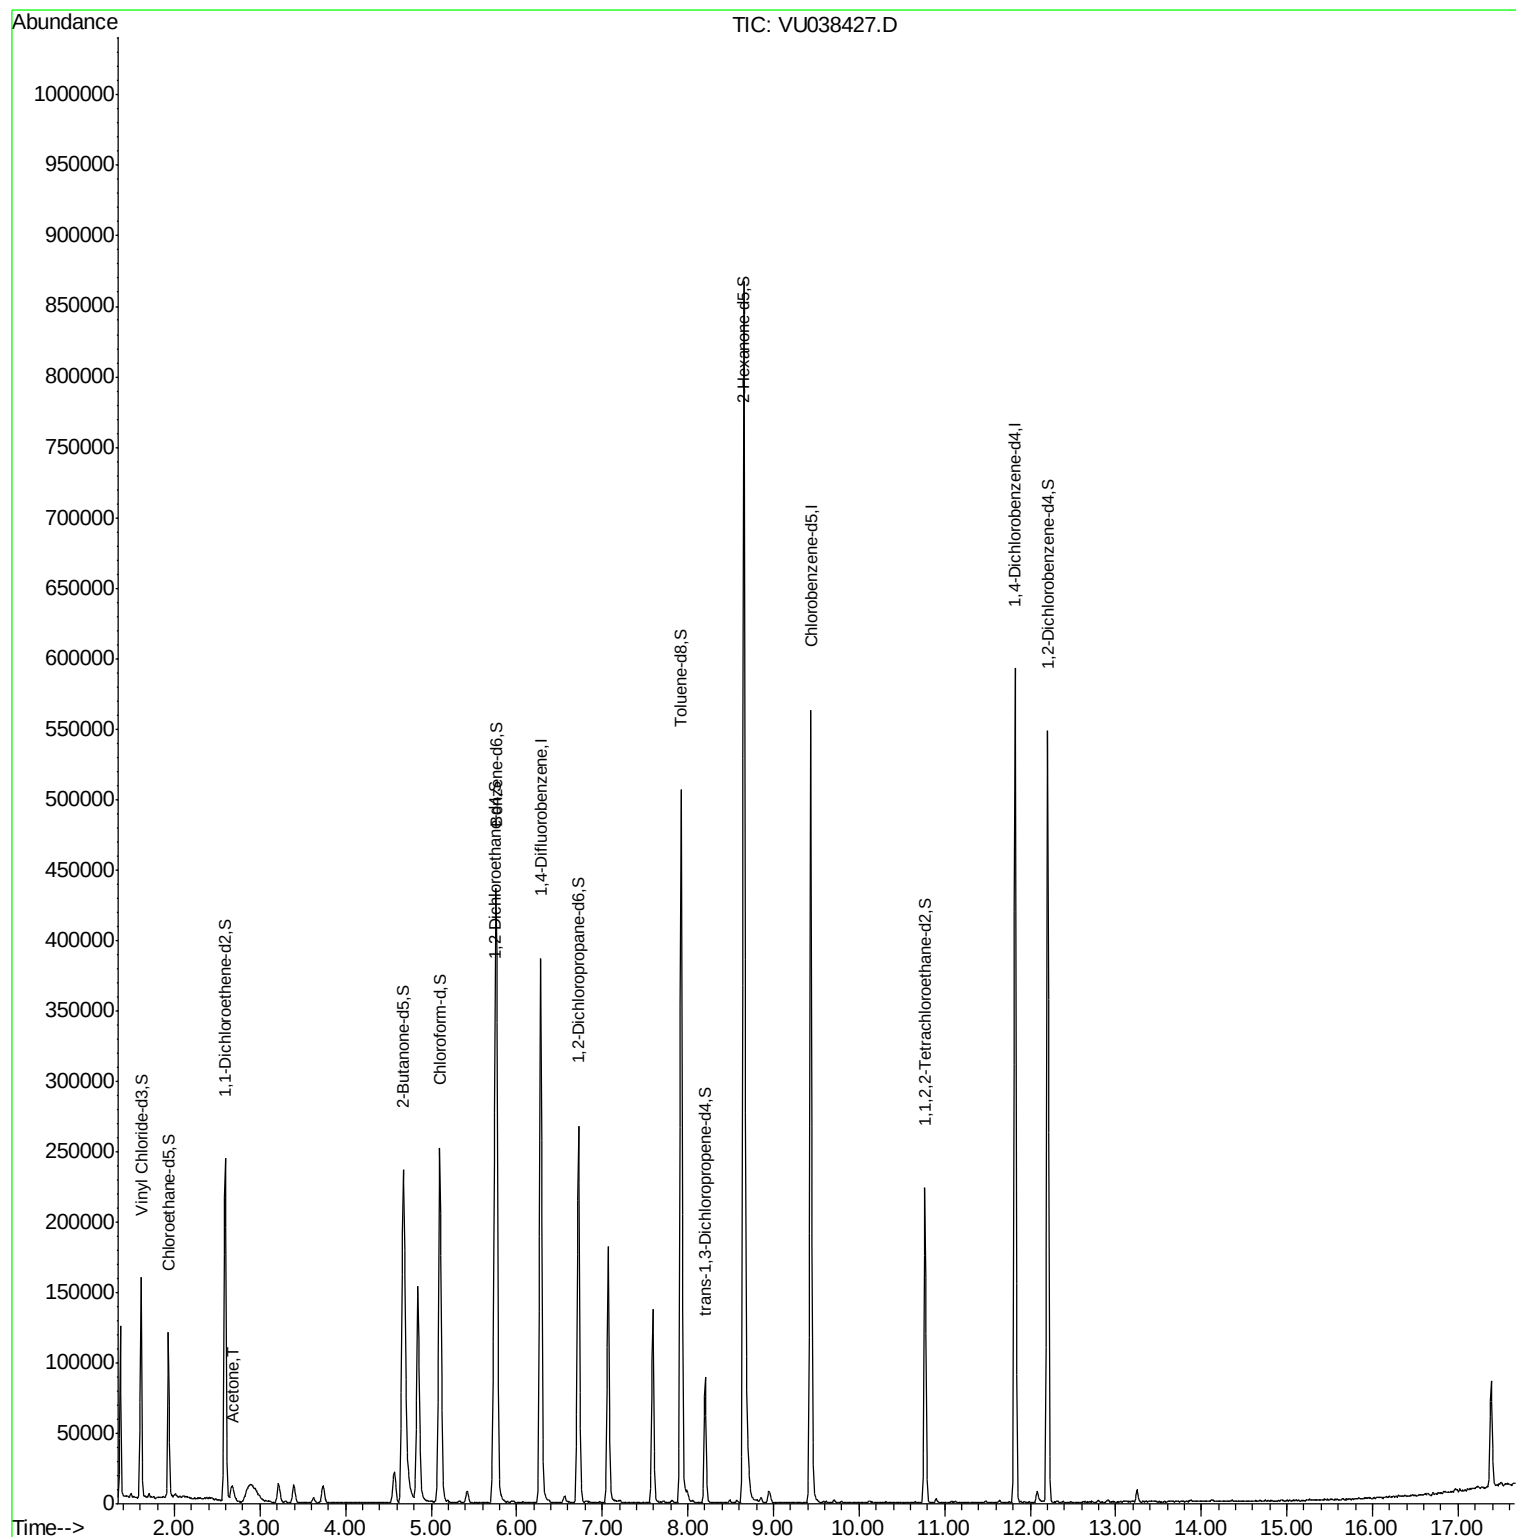

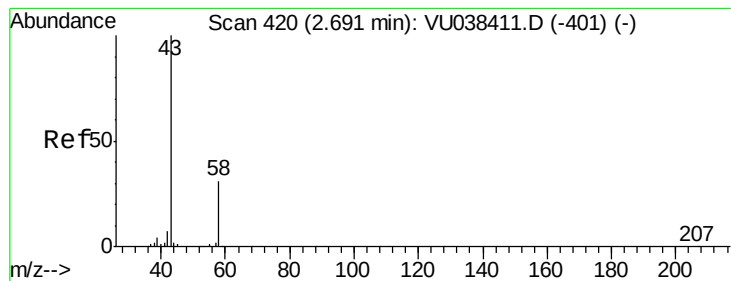

#13

Acetone

Concen: 4.945 ug/L

RT: 2.68 min Scan# 416

Delta R.T. -0.01 min

Lab File: VU038427.D

Acq: 30 May 2020 20:38

Instrument :

MSVOA_U

ClientSampleId :

BFX84

Tot Ion: 43 Resp: 20344

Ion Ratio Lower Upper

43 100

58 17.3 0.0 65.6

