

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU053120\
 Data File : VU038455.D
 Acq On : 31 May 2020 08:09
 Operator : JC/MD
 Sample : L2788-17
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFXC4

Quant Time: Jun 01 08:31:54 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR053120WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Mon Jun 01 06:27:31 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.28	114	298625	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.44	117	298174	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.83	152	142028	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.61	65	89425	4.63	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	92.60%
7) Chloroethane-d5	1.93	69	76650	5.16	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	103.20%
11) 1,1-Dichloroethene-d2	2.59	63	133887	3.52	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	70.40%
20) 2-Butanone-d5	4.68	46	349453	59.52	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	119.04%
24) Chloroform-d	5.10	84	184379	5.08	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	101.60%
26) 1,2-Dichloroethane-d4	5.74	65	112498	5.46	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	109.20%
32) Benzene-d6	5.76	84	372365	5.00	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	100.00%
36) 1,2-Dichloropropane-d6	6.72	67	116488	5.09	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	101.80%
41) Toluene-d8	7.92	98	311978	4.67	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	93.40%
43) trans-1,3-Dichloropropene-	8.20	79	45504	4.62	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	92.40%
46) 2-Hexanone-d5	8.65	63	301132	61.94	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	123.88%
57) 1,1,2,2-Tetrachloroethane-	10.77	84	105791	5.44	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	108.80%
64) 1,2-Dichlorobenzene-d4	12.20	152	128982	5.27	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	105.40%


Target Compounds					Ovalue
13) Acetone	2.68	43	8648	2.251 ug/L	78


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU053120\
Data File : VU038455.D
Acq On : 31 May 2020 08:09
Operator : JC/MD
Sample : L2788-17
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFXC4

Quant Time: Jun 01 08:31:54 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR053120WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Mon Jun 01 06:27:31 2020
Response via : Initial Calibration

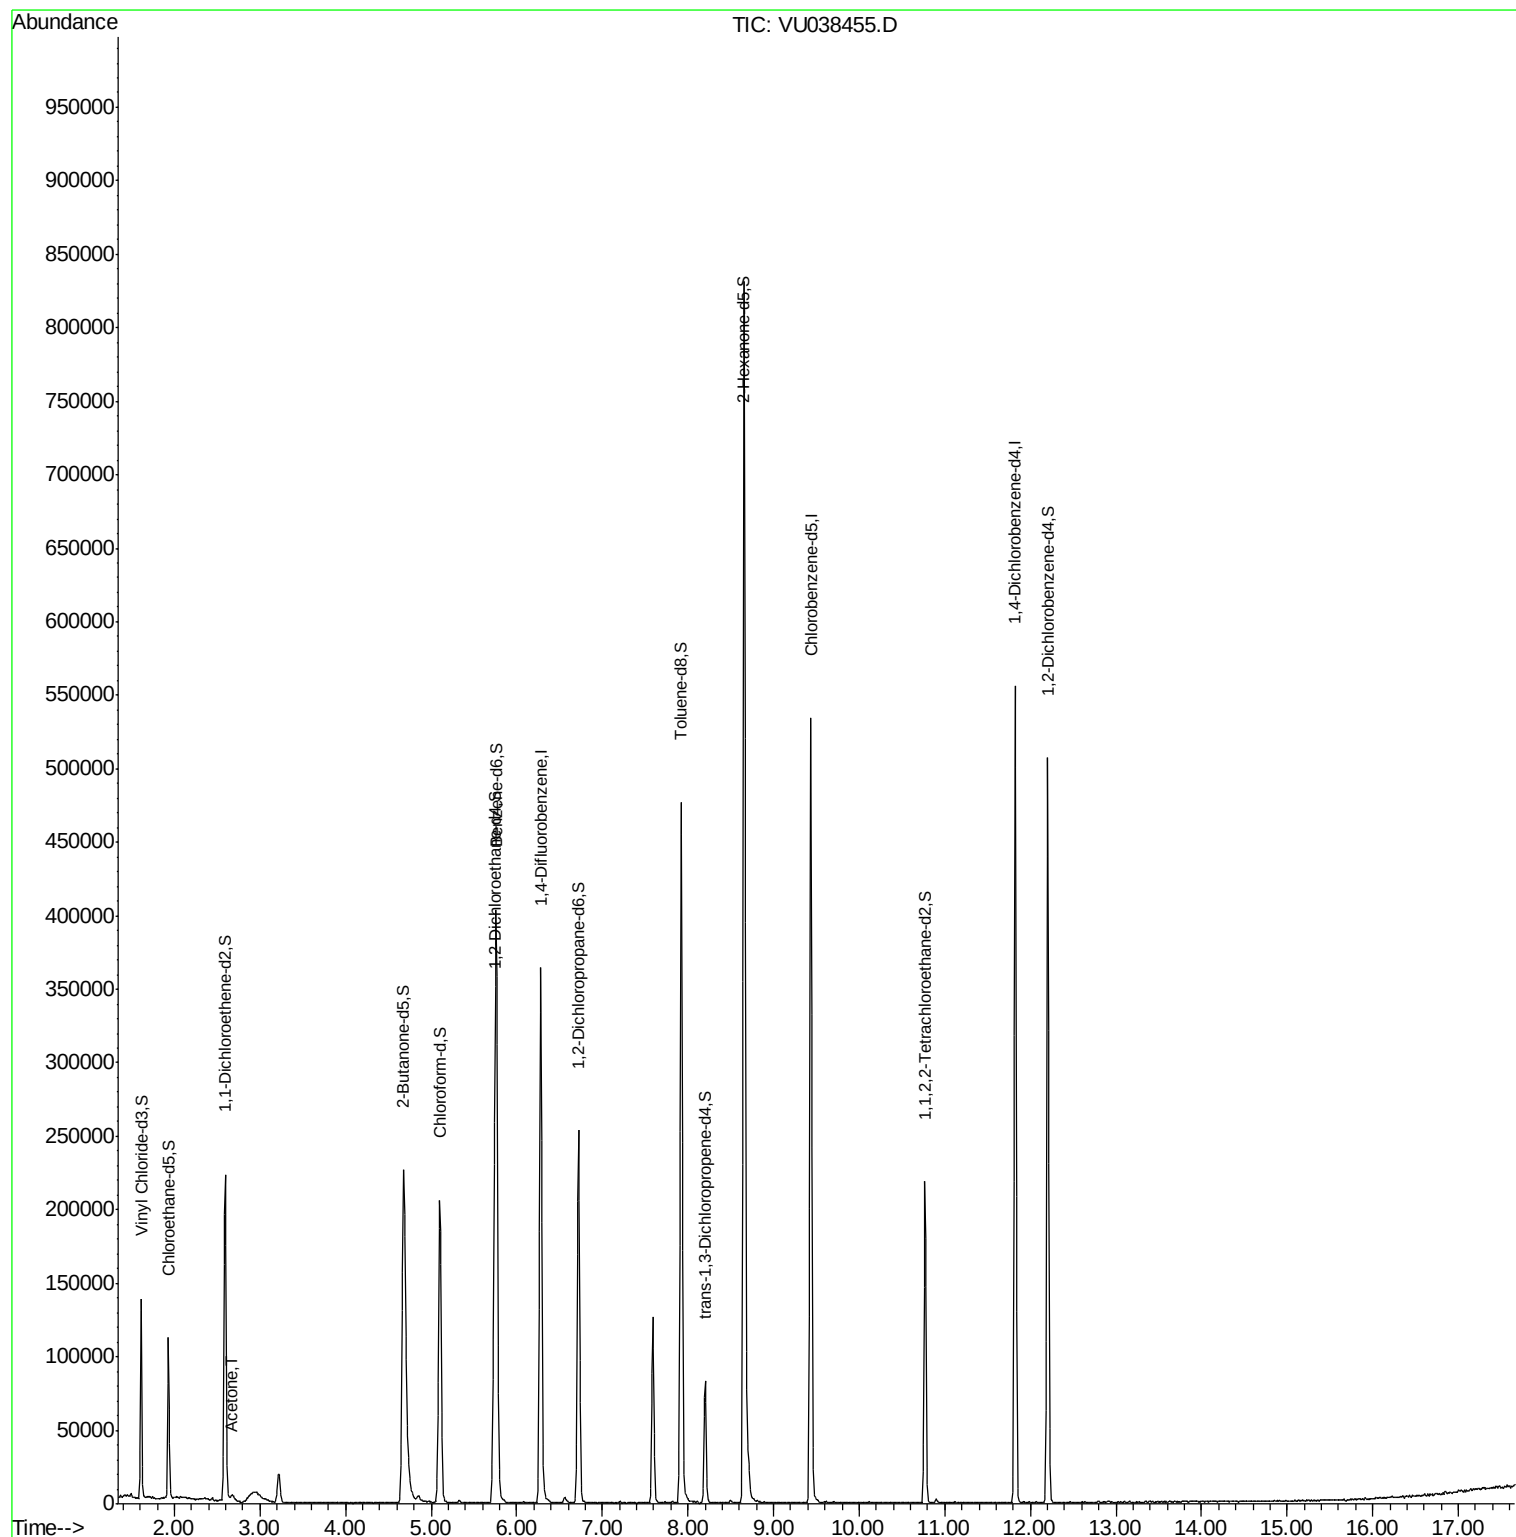

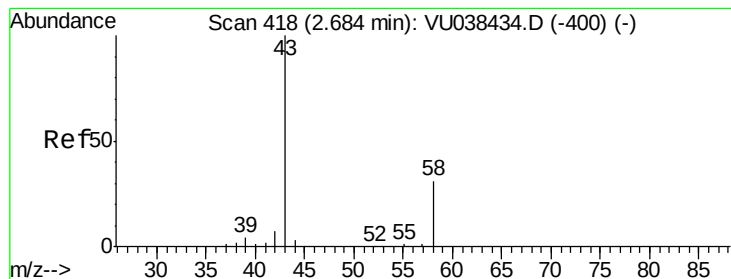

#13

Acetone

Concen: 2.251 ug/L

RT: 2.68 min Scan# 416

Delta R.T. -0.01 min

Lab File: VU038455.D

Acq: 31 May 2020 08:09

Instrument :
MSVOA_U
ClientSampleId :
BFXC4

Tot Ion: 43 Resp: 8648

Ion Ratio Lower Upper

43 100

58 20.3 0.0 65.6

