


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU053120\
 Data File : VU038403.D
 Acq On : 30 May 2020 08:27
 Operator : JC/MD
 Sample : BFB03
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB03

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR053020WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Sat May 30 11:02:05 2020

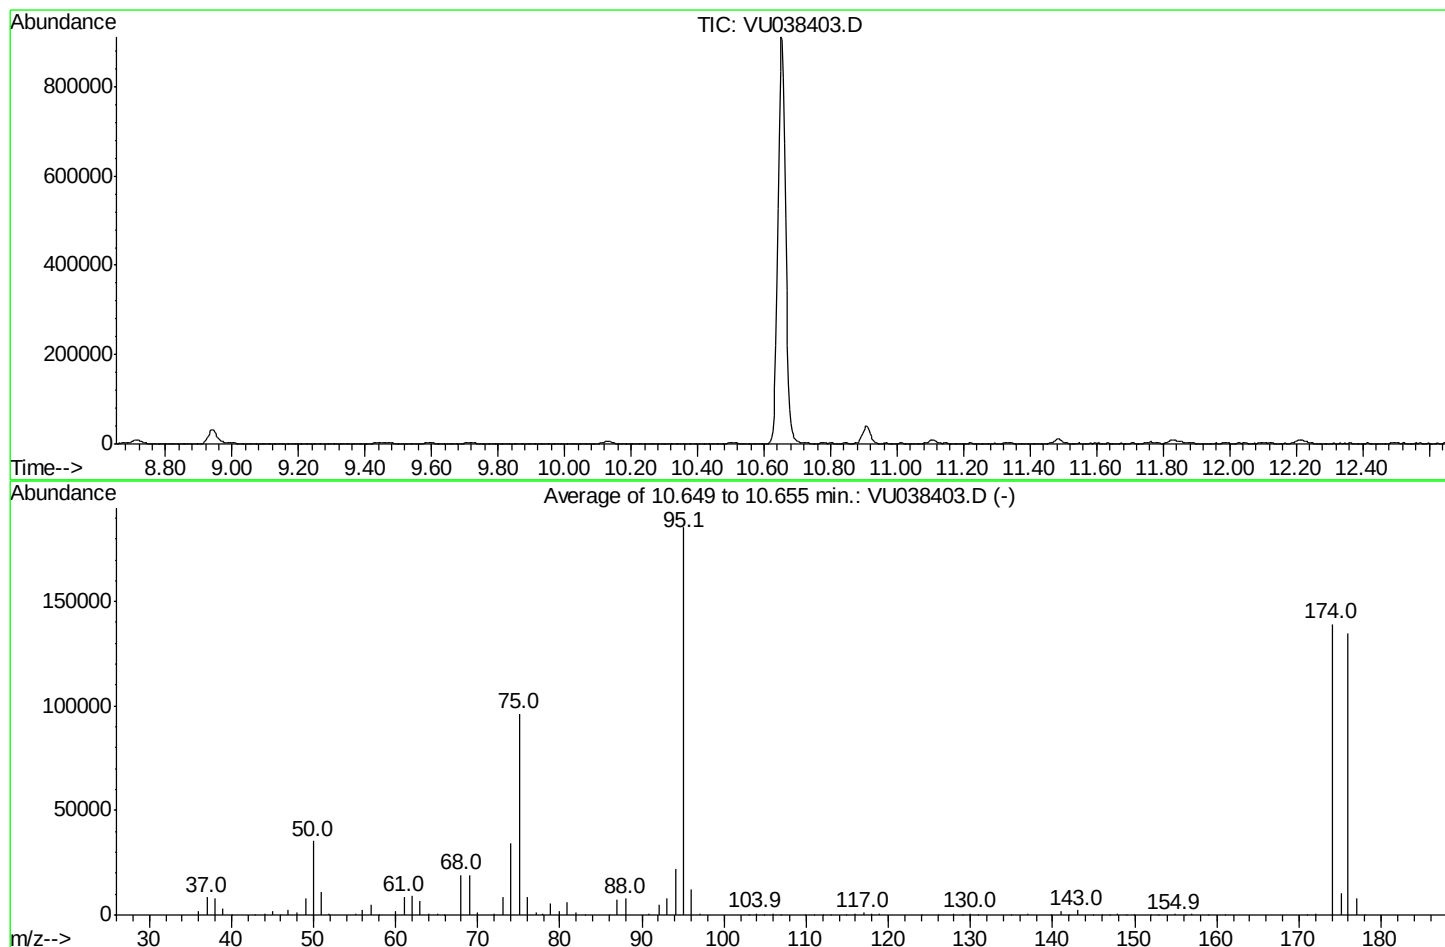

AutoFind: Scans 2895, 2896, 2897; Background Corrected with Scan 2881

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.1	35464	PASS
75	95	30	80	51.9	96229	PASS
95	95	100	100	100.0	185536	PASS
96	95	5	9	6.7	12521	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	75.1	139333	PASS
175	174	5	9	7.6	10646	PASS
176	174	95	101	96.6	134541	PASS
177	176	5	9	6.1	8208	PASS

m/z	Abundance
36.00	1836.0
37.00	8240.0
38.00	7374.0
39.00	3211.0
40.00	260.0
42.80	162.0
44.00	1459.0
45.00	1719.0
46.00	239.0
47.00	2280.0
47.90	951.0
49.10	7686.0
50.00	34040.0
51.00	10467.0
51.90	482.0
55.20	603.0
56.00	2493.0
57.00	4738.0
58.00	190.0
60.00	1631.0
61.00	8189.0
62.00	8561.0
63.00	6636.0
64.10	597.0
65.00	709.0
68.00	18184.0
69.00	18456.0
70.00	1476.0
72.00	812.0
73.00	8339.0
74.00	32656.0
75.10	92040.0
76.10	8590.0
77.00	985.0
78.00	651.0
78.90	5324.0
80.00	1515.0
80.90	5889.0
81.90	1166.0
83.00	140.0
87.00	6615.0
88.00	7434.0
90.90	773.0
92.00	4956.0
93.00	7712.0
94.10	21928.0
95.10	176512.0
96.00	12100.0
97.00	257.0
103.90	761.0
104.90	218.0
106.00	744.0
106.90	215.0
109.90	115.0
110.90	138.0
112.90	216.0
114.80	216.0
115.90	528.0
117.00	1051.0
117.90	591.0
118.90	812.0
124.10	102.0
127.90	650.0
129.00	263.0
130.00	747.0
131.00	226.0
134.90	263.0
136.90	314.0
139.90	128.0
141.00	1753.0
142.00	240.0
143.00	2109.0
144.90	332.0
146.00	295.0
147.90	448.0
150.00	106.0
151.90	131.0
152.80	127.0
154.90	390.0
156.90	300.0
158.80	174.0
161.00	195.0
172.00	763.0
174.00	128528.0
175.10	10439.0
176.00	123432.0
177.00	7740.0
177.90	182.0

Instrument :
MSVOA_U
ClientSampleId :
BFB03

m/z	Abundance
36.00	1880.0
37.00	8834.0
38.00	7981.0
39.00	3420.0
40.00	317.0
42.80	161.0
44.00	1502.0
45.10	1596.0
46.00	214.0
46.90	2405.0
47.90	1103.0
49.10	8191.0
50.00	36504.0
51.00	11131.0
51.90	546.0
55.10	590.0
56.00	2636.0
57.00	4950.0
58.00	247.0
60.00	1814.0
61.00	8747.0
62.00	9500.0
63.00	7310.0
64.10	620.0
65.10	747.0
65.90	163.0
68.00	19792.0
69.00	19296.0
70.00	1541.0
71.90	950.0
73.00	9004.0
74.00	35432.0
75.10	99312.0
76.10	9006.0
77.10	1069.0
77.90	747.0
78.90	5651.0
80.00	1651.0
80.90	6293.0
81.90	1312.0
83.00	119.0
86.00	299.0
87.00	7485.0
88.00	8088.0
90.90	802.0
92.00	5279.0
93.00	8542.0
94.10	22968.0
95.10	191296.0
96.00	12906.0
97.00	356.0
103.00	117.0
103.90	951.0
104.90	248.0
106.00	879.0
107.00	203.0
109.80	127.0
110.90	127.0
113.00	221.0
114.80	188.0
116.00	654.0
117.00	1183.0
117.90	627.0
118.90	826.0
126.00	144.0
127.90	786.0
129.00	262.0
130.00	866.0
130.90	336.0
135.00	217.0
136.90	346.0
139.80	124.0
141.00	1824.0
142.00	234.0
143.00	2290.0
144.90	331.0
145.90	316.0
147.90	519.0
149.00	100.0
149.90	110.0
151.90	120.0
152.80	146.0
154.90	454.0
156.90	365.0
158.90	151.0
161.00	216.0
172.00	955.0
174.00	143104.0
175.10	11013.0
176.00	138944.0
177.00	8277.0
177.90	202.0

Instrument :
MSVOA_U
ClientSampleId :
BFB03

m/z	Abundance
36.00	1705.0
37.00	8248.0
38.00	7855.0
39.00	3143.0
40.00	356.0
42.80	103.0
44.00	1374.0
45.00	1421.0
45.90	174.0
46.90	2231.0
47.90	1095.0
49.10	7933.0
50.00	35848.0
51.00	10805.0
51.90	654.0
55.00	529.0
56.00	2692.0
57.00	4940.0
57.90	252.0
60.00	1694.0
61.00	8876.0
62.00	9333.0
63.00	7176.0
64.10	670.0
65.10	695.0
65.90	184.0
68.00	19616.0
69.00	18640.0
70.00	1544.0
71.90	959.0
73.00	8841.0
74.00	34592.0
75.00	97336.0
76.00	8643.0
77.10	1044.0
77.90	796.0
78.90	5737.0
80.00	1595.0
80.90	5967.0
81.90	1381.0
85.90	280.0
87.00	7662.0
88.00	8083.0
90.90	658.0
92.10	5433.0
93.00	8622.0
94.10	22008.0
95.10	188800.0
96.10	12557.0
97.00	404.0
103.00	148.0
103.90	1015.0
104.90	245.0
106.00	915.0
107.00	165.0
109.80	116.0
112.10	128.0
113.00	219.0
114.80	178.0
116.00	745.0
117.00	1248.0
117.90	711.0
118.80	866.0
126.00	184.0
127.90	794.0
128.90	256.0
130.00	873.0
130.90	404.0
134.80	176.0
136.90	342.0
139.70	131.0
141.00	1702.0
142.00	226.0
143.00	2191.0
144.90	291.0
146.00	302.0
147.00	107.0
147.90	420.0
149.00	147.0
149.90	135.0
152.90	154.0
154.90	419.0
156.10	118.0
156.90	388.0
159.00	164.0
161.00	193.0
171.00	117.0
172.00	1102.0
174.00	146368.0
175.10	10488.0
176.00	141248.0
177.00	8609.0

Instrument :
MSVOA_U
ClientSampleId :
BFB03

178.00

238.0

Instrument :
MSVOA_U
ClientSampleId :
BFB03

Scan 2881 (10.604 min): VU038403.D
BFB03

m/z	Abundance
39.90	275.0
44.00	832.0

Instrument :
MSVOA_U
ClientSampleId :
BFB03