

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU053122\
 Data File : VU048763.D
 Acq On : 01 Jun 2022 01:49
 Operator : SY/MD
 Sample : N3099-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 20220426-SPLP-AMENDED-COMPOSITE-F

Quant Time: Jun 01 05:45:11 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U052622W.M
 Quant Title : SW846 8260
 QLast Update : Fri May 27 06:42:31 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.375	168	196206	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.250	114	349185	50.000	ug/l	0.00
63) Chlorobenzene-d5	9.417	117	324236	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	11.812	152	154441	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.703	65	171254	58.118	ug/l	0.00
Spiked Amount 50.000	Range 78 - 117		Recovery = 116.240%			
35) Dibromofluoromethane	5.292	113	819	0.329	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery = 0.660%#			
50) Toluene-d8	7.899	98	400436	44.842	ug/l	0.00
Spiked Amount 50.000	Range 92 - 112		Recovery = 89.680%#			
62) 4-Bromofluorobenzene	10.632	95	145174	42.986	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery = 85.980%			
Target Compounds						Qvalue
4) Vinyl Chloride	1.604	62	6364	2.376	ug/l #	72
5) Bromomethane	1.858	94	49	Below Cal	#	29
6) Chloroethane	1.932	64	1891	Below Cal	#	88
11) Tert butyl alcohol	3.192	59	11023	14.755	ug/l #	28
12) 1,1-Dichloroethene	2.581	96	1377	0.690	ug/l #	93
13) Acrolein	2.485	56	504	Below Cal	#	62
16) Acetone	2.623	43	58675	39.073	ug/l	100
17) Carbon Disulfide	2.797	76	2137	0.367	ug/l #	86
18) Methyl Acetate	2.961	43	1125	0.298	ug/l #	65
20) Methylene Chloride	3.044	84	5622	2.202	ug/l	89
24) 1,1-Dichloroethane	3.874	63	19818	4.423	ug/l	99
25) 2-Butanone	4.710	43	10415	4.828	ug/l	95
27) cis-1,2-Dichloroethene	4.665	96	16500	6.240	ug/l	87
29) Tetrahydrofuran	5.060	42	1142	0.840	ug/l #	70
31) Cyclohexane	5.372	56	4953	1.334	ug/l #	7
36) 1,1-Dichloropropene	5.372	75	16064	4.418	ug/l #	50
37) Ethyl Acetate	4.710	43	10415	2.266	ug/l #	68
38) Carbon Tetrachloride	5.375	117	19637	4.708	ug/l #	19
41) Methacrylonitrile	5.060	41	771	0.332	ug/l #	40
42) 1,2-Dichloroethane	5.806	62	1475	0.351	ug/l #	76
44) Trichloroethene	6.542	130	1395	0.504	ug/l	85
49) 1,4-Dioxane	6.967	88	231	3.450	ug/l #	30
51) 4-Methyl-2-Pentanone	7.793	43	3792	0.875	ug/l #	84
59) 2-Hexanone	8.687	43	3043	0.856	ug/l	82
64) Tetrachloroethene	8.558	164	87	Below Cal	#	63
65) Chlorobenzene	9.452	112	2536	0.370	ug/l	89
74) N-amyl acetate	10.327	43	360	2.535	ug/l #	41
76) 1,2,3-Trichloropropane	10.632	75	73569	14.774	ug/l #	47
81) trans-1,4-Dichloro-2-b...	10.632	75	73569	53.643	ug/l #	13
84) 1,2,4-Trimethylbenzene	11.475	105	1547	1.349	ug/l #	48
89) n-Butylbenzene	12.208	91	1098	2.303	ug/l #	90
92) 1,2-Dibromo-3-Chloropr...	13.153	75	496	0.423	ug/l #	4
93) 1,2,4-Trichlorobenzene	13.848	180	911	0.262	ug/l #	57
95) Naphthalene	14.092	128	5893	2.993	ug/l	97
96) 1,2,3-Trichlorobenzene	14.333	180	759	0.220	ug/l	87

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU053122\
Data File : VU048763.D
Acq On : 01 Jun 2022 01:49
Operator : SY/MD
Sample : N3099-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 39 Sample Multiplier: 1


Instrument :
MSVOA_U
ClientSampleId :
20220426-SPLP-AMENDED-COMPOSITE-F


Quant Time: Jun 01 05:45:11 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U052622W.M
Quant Title : SW846 8260
QLast Update : Fri May 27 06:42:31 2022
Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
----------	------	------	----------	------	-------	----------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quant Time: Jun 01 05:45:11 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U052622W.M
Quant Title : SW846 8260
QLast Update : Fri May 27 06:42:31 2022
Response via : Initial Calibration









#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.375 min Scan# 11
Delta R.T. 0.000 min
Lab File: VU048763.D
Acq: 01 Jun 2022 01:49




Instrument :
MSVOA_U
ClientSampleId :
20220426-SPLP-AMENDED-COMPOSITE-F


Tgt Ion:168 Resp: 196206
Ion Ratio Lower Upper
168 100
99 59.6 49.3 73.9

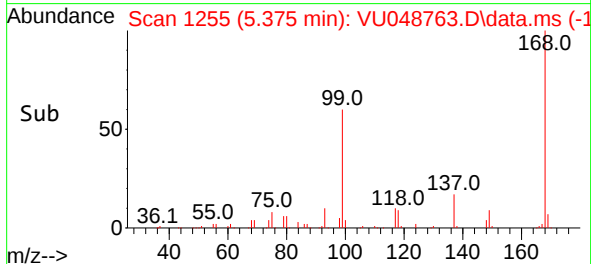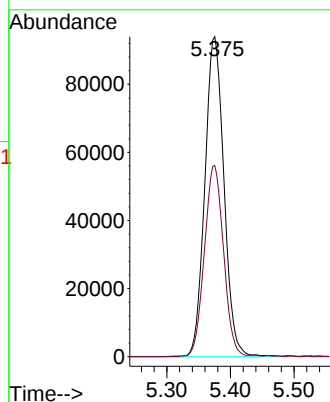

#4
Vinyl Chloride
Concen: 2.376 ug/l
RT: 1.604 min Scan# 82
Delta R.T. -0.000 min
Lab File: VU048763.D
Acq: 01 Jun 2022 01:49

Tgt Ion: 62 Resp: 6364
Ion Ratio Lower Upper
62 100
64 47.2 25.2 37.8#


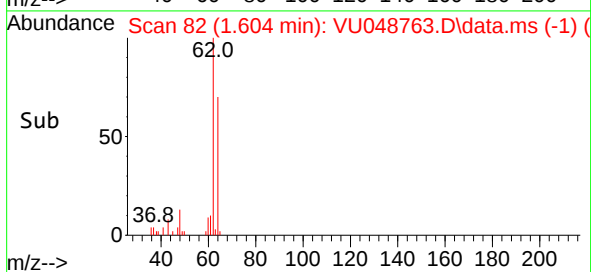
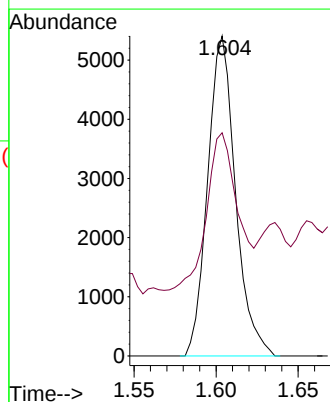





#5
Bromomethane
Concen: Below Cal
RT: 1.858 min Scan# 1
Delta R.T. 0.007 min
Lab File: VU048763.D
Acq: 01 Jun 2022 01:49




Instrument :
MSVOA_U
ClientSampleId :
20220426-SPLP-AMENDED-COMPOSITE-F


Tgt Ion: 94 Resp: 49
Ion Ratio Lower Upper
94 100
96 161.9 75.1 112.7#

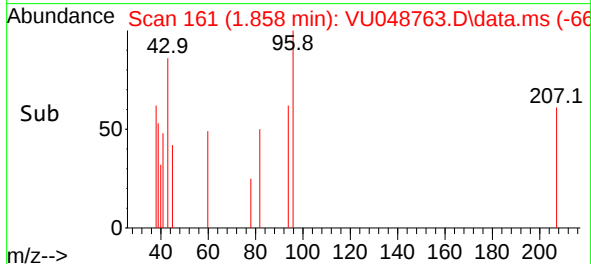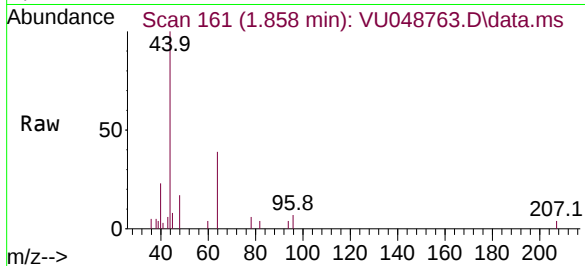

#6
Chloroethane
Concen: Below Cal
RT: 1.932 min Scan# 184
Delta R.T. -0.000 min
Lab File: VU048763.D
Acq: 01 Jun 2022 01:49

Tgt Ion: 64 Resp: 1891
Ion Ratio Lower Upper
64 100
66 38.1 25.2 37.8#


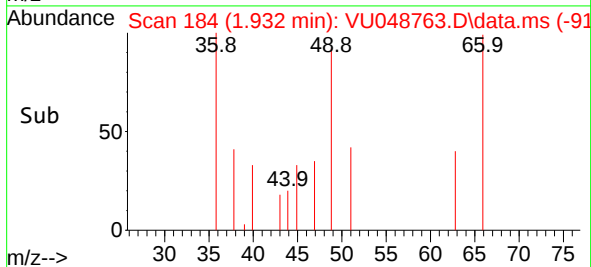

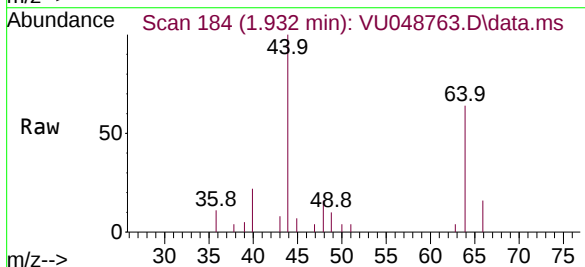




#11
Tert butyl alcohol
Concen: 14.755 ug/l
RT: 3.192 min Scan# 51
Delta R.T. 0.003 min
Lab File: VU048763.D
Acq: 01 Jun 2022 01:49




Instrument :
MSVOA_U
ClientSampleId :
20220426-SPLP-AMENDED-COMPOSITE-F


Tgt Ion: 59 Resp: 11023
Ion Ratio Lower Upper
59 100
57 0.0 39.7 59.5#

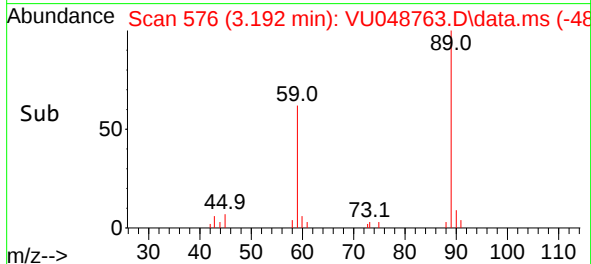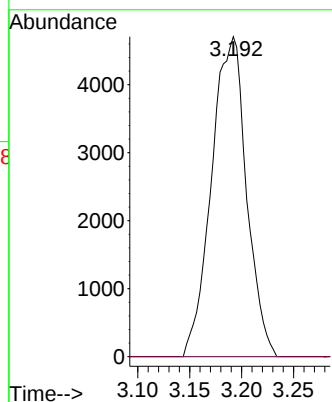

#12
1,1-Dichloroethene
Concen: 0.690 ug/l
RT: 2.581 min Scan# 386
Delta R.T. -0.000 min
Lab File: VU048763.D
Acq: 01 Jun 2022 01:49

Tgt Ion: 96 Resp: 1377
Ion Ratio Lower Upper
96 100
61 160.6 131.1 196.7
98 50.0 51.8 77.8#

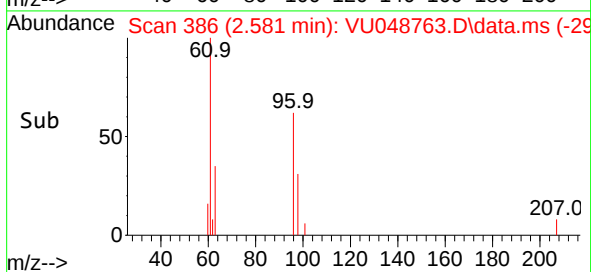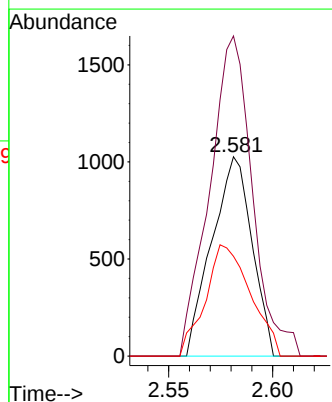



#13

Acrolein

Concen: Below Cal

RT: 2.485 min Scan# 31

Delta R.T. -0.003 min

Lab File: VU048763.D

Acq: 01 Jun 2022 01:49

Instrument :

MSVOA_U

ClientSampleId :





20220426-SPLP-AMENDED-COMPOSITE-F

Tgt Ion: 56 Resp: 504

Ion Ratio Lower Upper

56 100

55 40.1 57.7 86.5#

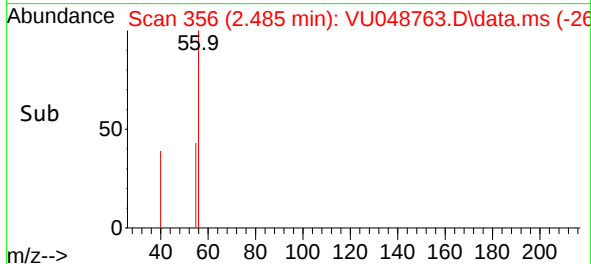

#16

Acetone

Concen: 39.073 ug/l

RT: 2.623 min Scan# 399

Delta R.T. -0.003 min

Lab File: VU048763.D




Acq: 01 Jun 2022 01:49


Tgt Ion: 43 Resp: 58675

Ion Ratio Lower Upper

43 100

58 33.2 26.3 39.5


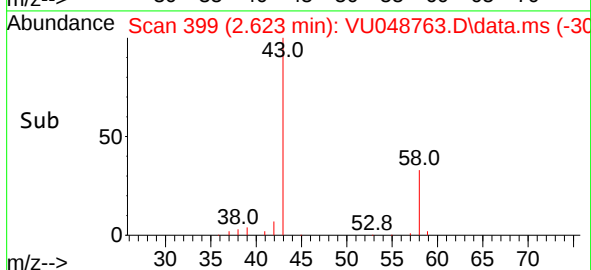






#17
Carbon Disulfide
Concen: 0.367 ug/l
RT: 2.797 min Scan# 411
Delta R.T. 0.003 min
Lab File: VU048763.D
Acq: 01 Jun 2022 01:49




Instrument : MSVOA_U
ClientSampleId : 20220426-SPLP-AMENDED-COMPOSITE-F


Tgt Ion: 76 Resp: 2137
Ion Ratio Lower Upper
76 100
78 14.3 7.3 10.9#

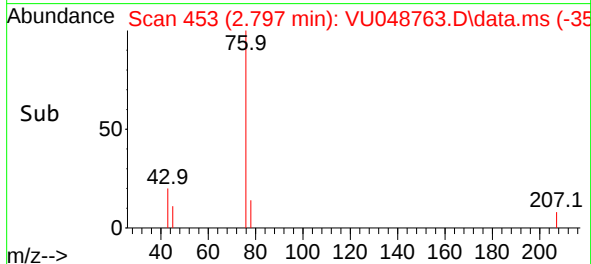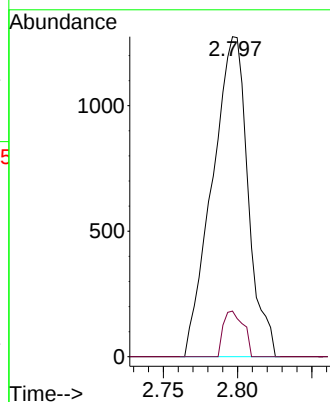

#18
Methyl Acetate
Concen: 0.298 ug/l
RT: 2.961 min Scan# 504
Delta R.T. 0.013 min
Lab File: VU048763.D
Acq: 01 Jun 2022 01:49

Tgt Ion: 43 Resp: 1125
Ion Ratio Lower Upper
43 100
74 6.7 19.2 28.8#


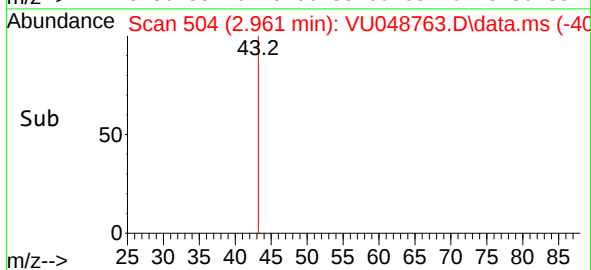
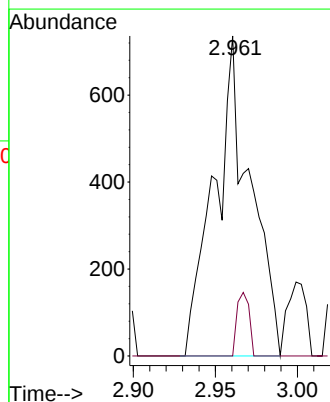
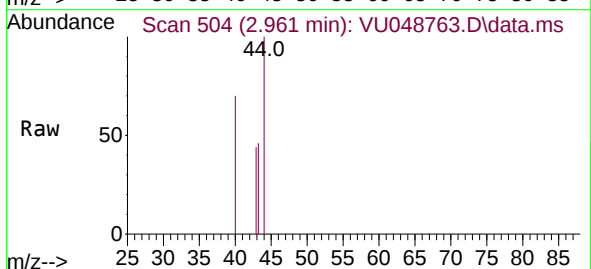




#20
Methylene Chloride
Concen: 2.202 ug/l
RT: 3.044 min Scan# 511
Delta R.T. -0.003 min
Lab File: VU048763.D
Acq: 01 Jun 2022 01:49




Instrument :
MSVOA_U
ClientSampleId :
20220426-SPLP-AMENDED-COMPOSITE-F


Tgt Ion:	84	Resp:	5622
Ion	Ratio	Lower	Upper
84	100		
49	106.7	97.0	145.4
51	33.2	29.8	44.8
86	55.2	50.9	76.3

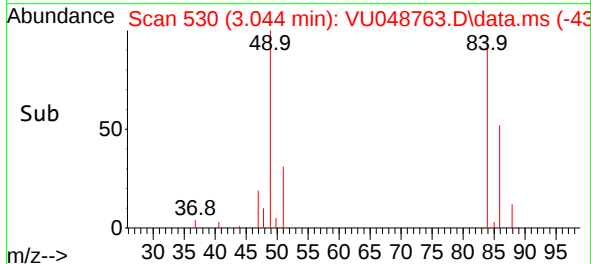

#24
1,1-Dichloroethane
Concen: 4.423 ug/l
RT: 3.874 min Scan# 788
Delta R.T. 0.003 min
Lab File: VU048763.D
Acq: 01 Jun 2022 01:49

Tgt Ion:	63	Resp:	19818
Ion	Ratio	Lower	Upper
63	100		
98	6.4	3.1	9.3
100	4.6	2.0	5.8

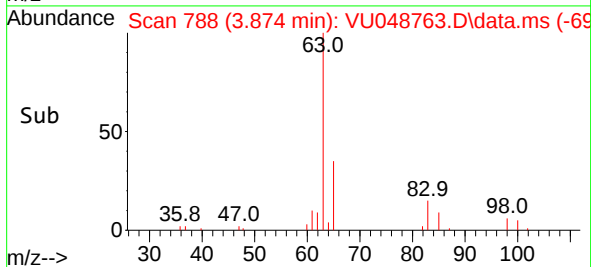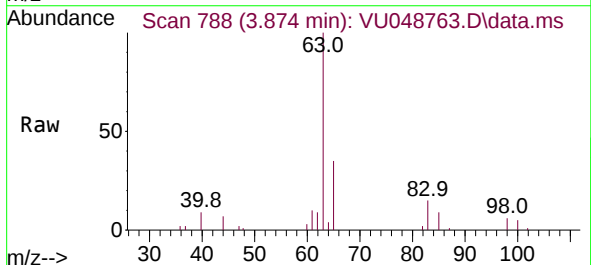

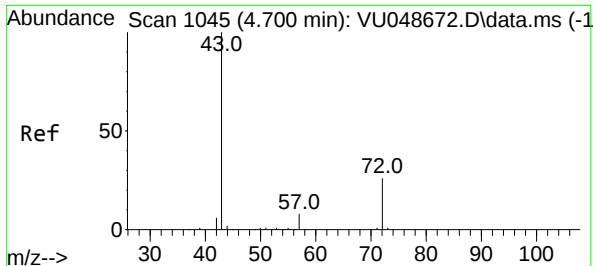

#25

2-Butanone

Concen: 4.828 ug/l

RT: 4.710 min Scan# 1045

Delta R.T. 0.010 min

Lab File: VU048763.D

Acq: 01 Jun 2022 01:49

Instrument :

MSVOA_U

ClientSampleId :





20220426-SPLP-AMENDED-COMPOSITE-F

Tgt Ion: 43 Resp: 10415

Ion Ratio Lower Upper

43 100

72 23.8 21.1 31.7

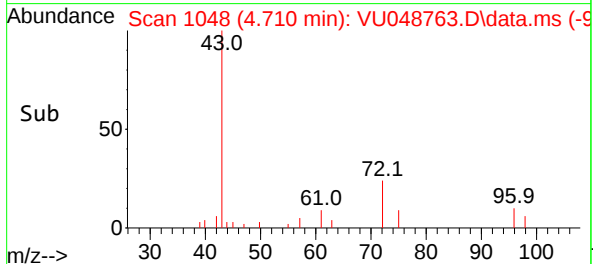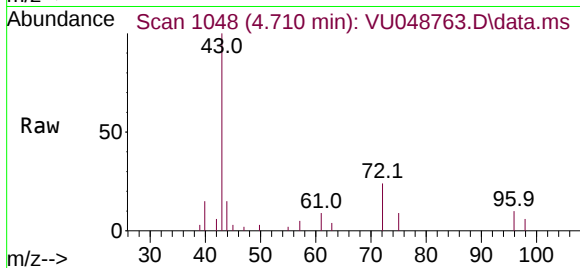

#27

cis-1,2-Dichloroethene

Concen: 6.240 ug/l

RT: 4.665 min Scan# 1034

Delta R.T. -0.003 min

Lab File: VU048763.D

Acq: 01 Jun 2022 01:49




Tgt Ion: 96 Resp: 16500


Ion Ratio Lower Upper

96 100

61 130.2 0.0 306.2

98 62.9 0.0 130.4

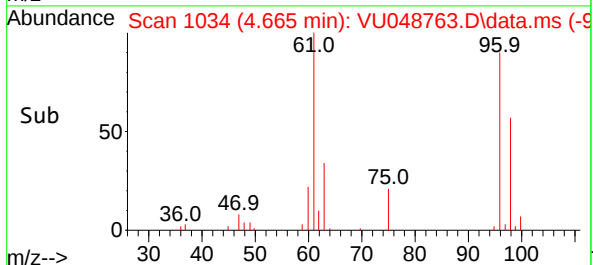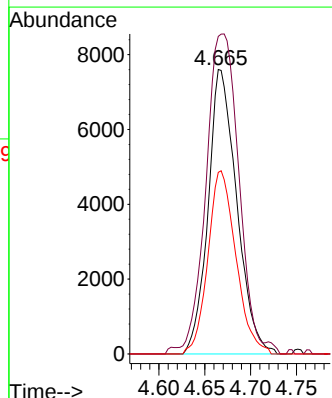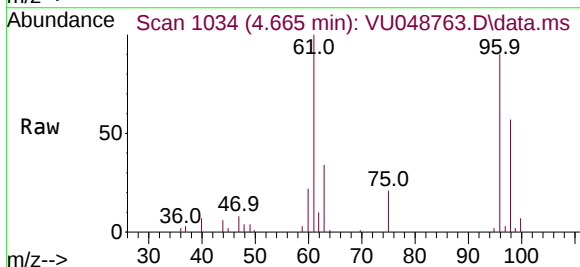

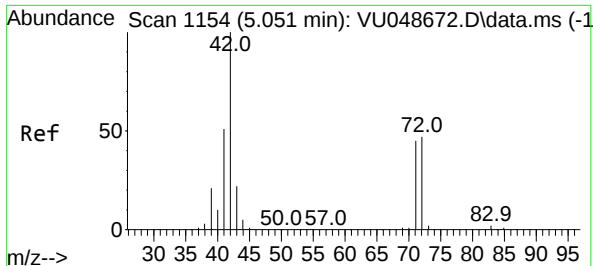

#29

Tetrahydrofuran

Concen: 0.840 ug/l

RT: 5.060 min Scan# 1154

Delta R.T. 0.010 min

Lab File: VU048763.D

Acq: 01 Jun 2022 01:49

Instrument :

MSVOA_U

ClientSampleId :

20220426-SPLP-AMENDED-COMPOSITE-F





Tgt Ion: 42 Resp: 1142

Ion Ratio Lower Upper

42 100

72 18.2 37.6 56.4#

71 33.1 35.0 52.4#

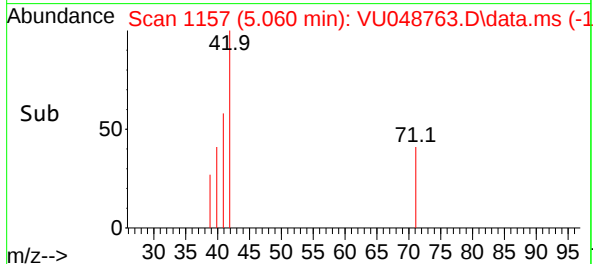

#31

Cyclohexane

Concen: 1.334 ug/l

RT: 5.372 min Scan# 1254

Delta R.T. -0.019 min

Lab File: VU048763.D

Acq: 01 Jun 2022 01:49




Tgt Ion: 56 Resp: 4953


Ion Ratio Lower Upper

56 100

69 160.3 25.6 38.4#

84 118.1 66.2 99.4#

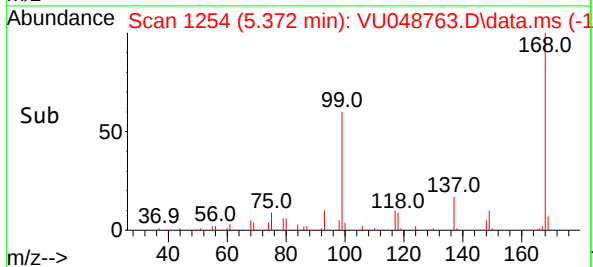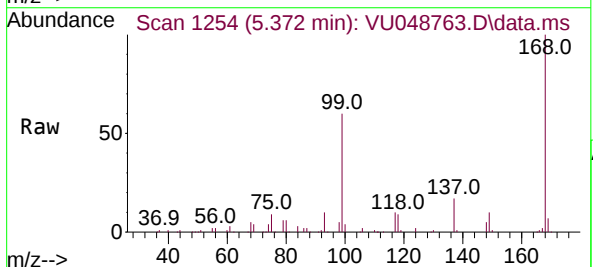

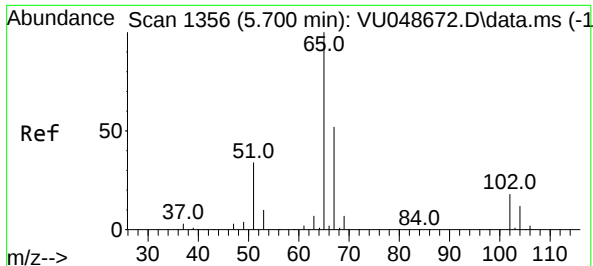

#33

1,2-Dichloroethane-d4

Concen: 58.118 ug/l

RT: 5.703 min Scan# 11

Delta R.T. 0.003 min

Lab File: VU048763.D

Acq: 01 Jun 2022 01:49

Instrument :

MSVOA_U

ClientSampleId :





20220426-SPLP-AMENDED-COMPOSITE-F

Tgt Ion: 65 Resp: 171254

Ion Ratio Lower Upper

65 100

67 52.7 0.0 103.0

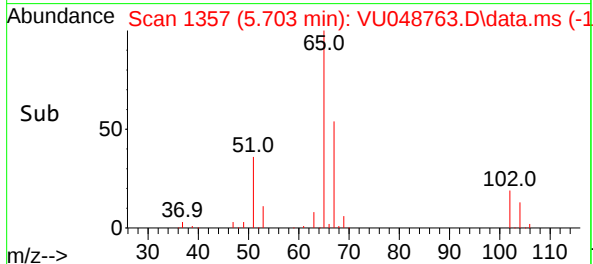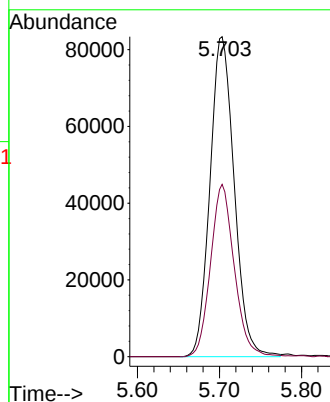

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.250 min Scan# 1527

Delta R.T. -0.000 min

Lab File: VU048763.D

Acq: 01 Jun 2022 01:49




Tgt Ion: 114 Resp: 349185


Ion Ratio Lower Upper

114 100

63 21.4 0.0 42.6

88 16.2 0.0 32.2


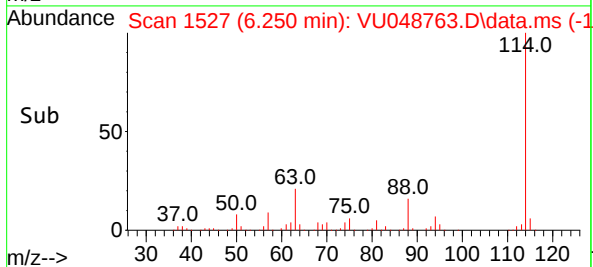

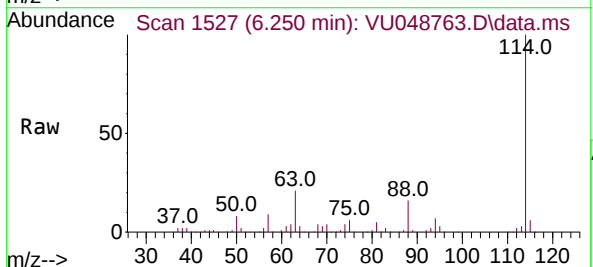


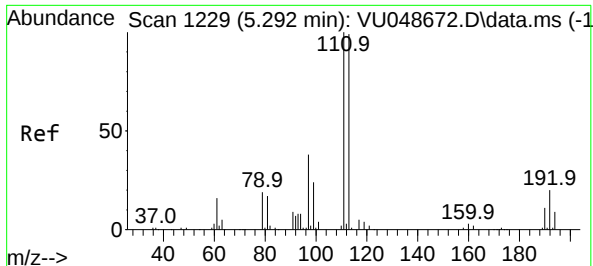

#35
Dibromofluoromethane
Concen: 0.329 ug/l
RT: 5.292 min Scan# 11
Delta R.T. -0.000 min
Lab File: VU048763.D
Acq: 01 Jun 2022 01:49




Instrument : MSVOA_U
ClientSampleId : 20220426-SPLP-AMENDED-COMPOSITE-F


Tgt Ion:113 Resp: 819
Ion Ratio Lower Upper
113 100
111 74.7 80.7 121.1#
192 0.0 15.9 23.9#

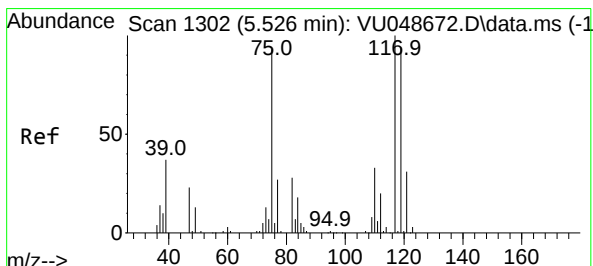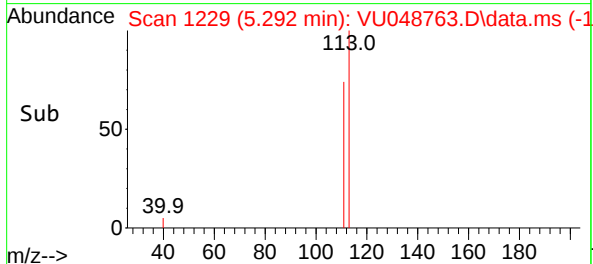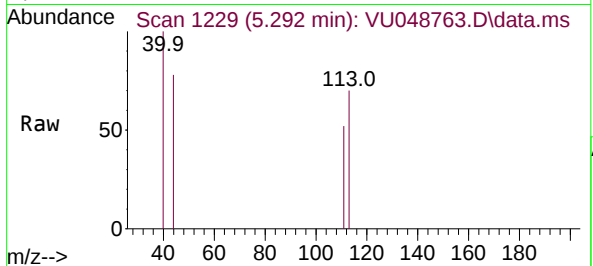

#36
1,1-Dichloropropene
Concen: 4.418 ug/l
RT: 5.372 min Scan# 1254
Delta R.T. -0.154 min
Lab File: VU048763.D
Acq: 01 Jun 2022 01:49

Tgt Ion: 75 Resp: 16064
Ion Ratio Lower Upper
75 100
110 9.6 17.4 52.3#
77 0.0 24.8 37.2#

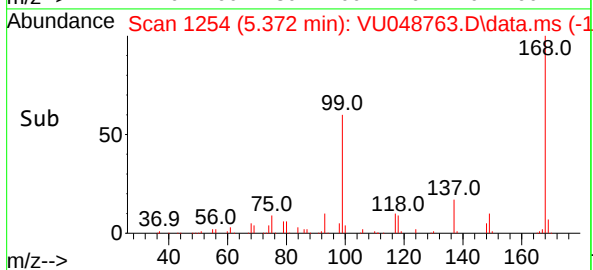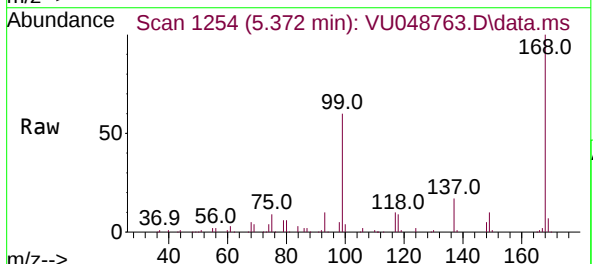



#37

Ethyl Acetate

Concen: 2.266 ug/l

RT: 4.710 min Scan# 1048

Delta R.T. -0.090 min

Lab File: VU048763.D

Acq: 01 Jun 2022 01:49





Instrument :

MSVOA_U

ClientSampleId :

20220426-SPLP-AMENDED-COMPOSITE-F

Tgt Ion: 43	Resp: 10415
Ion Ratio	Lower Upper
43	100
61	0.0 11.7 17.5#
70	0.0 8.4 12.6#

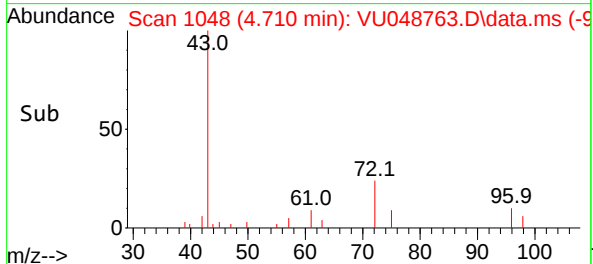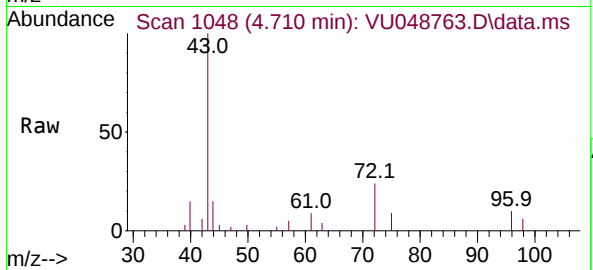

#38

Carbon Tetrachloride

Concen: 4.708 ug/l




RT: 5.375 min Scan# 1255


Delta R.T. -0.151 min

Lab File: VU048763.D

Acq: 01 Jun 2022 01:49

Tgt Ion: 117	Resp: 19637
Ion Ratio	Lower Upper
117	100
119	8.3 75.4 113.2#
121	0.0 24.6 36.8#



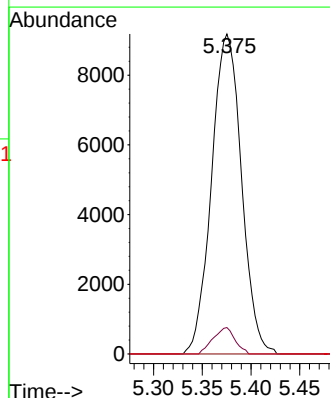
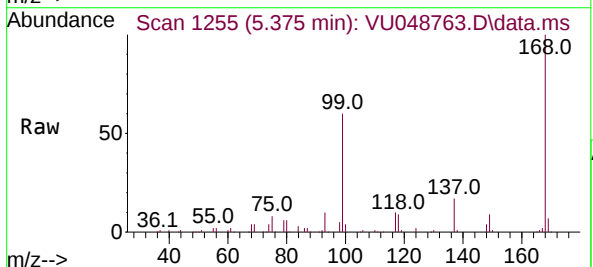


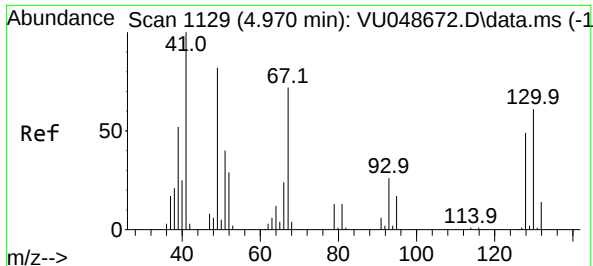

#41
Methacrylonitrile
Concen: 0.332 ug/l
RT: 5.060 min Scan# 1129
Delta R.T. 0.090 min
Lab File: VU048763.D
Acq: 01 Jun 2022 01:49




Instrument : MSVOA_U
ClientSampleId : 20220426-SPLP-AMENDED-COMPOSITE-F


Tgt Ion: 41	Resp: 771		
Ion	Ratio	Lower	Upper
41	100		
39	37.1	42.6	64.0#
67	0.0	61.0	91.4#
52	0.0	24.2	36.4#

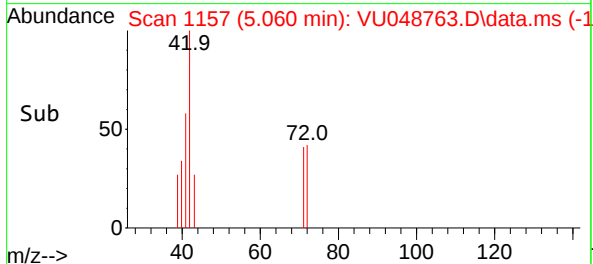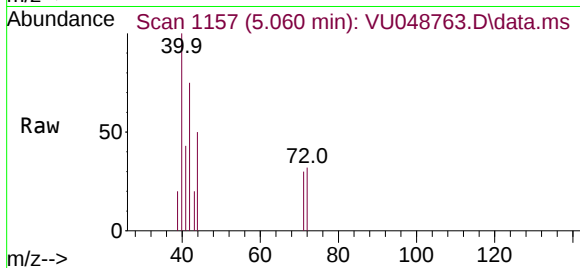

#42
1,2-Dichloroethane
Concen: 0.351 ug/l
RT: 5.806 min Scan# 1389
Delta R.T. 0.013 min
Lab File: VU048763.D
Acq: 01 Jun 2022 01:49

Tgt Ion: 62	Resp: 1475
Ion Ratio	Lower Upper
62 100	
98 0.0	0.0 17.0


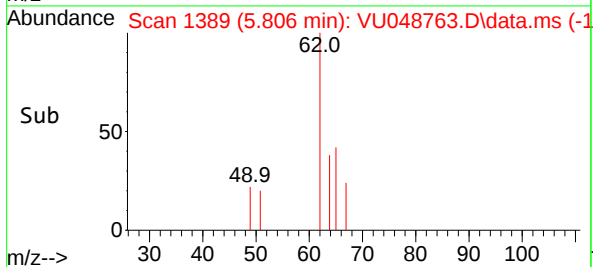

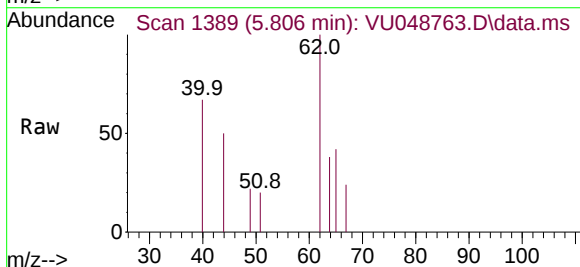




#44
Trichloroethene
Concen: 0.504 ug/l
RT: 6.542 min Scan# 1
Delta R.T. -0.000 min
Lab File: VU048763.D
Acq: 01 Jun 2022 01:49




Instrument :
MSVOA_U
ClientSampleId :
20220426-SPLP-AMENDED-COMPOSITE-F


Tgt Ion:130 Resp: 1395
Ion Ratio Lower Upper
130 100
95 87.2 0.0 204.8

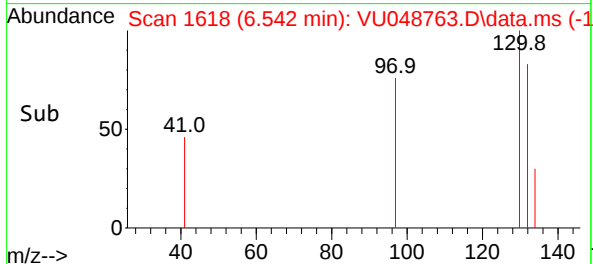

#49
1,4-Dioxane
Concen: 3.450 ug/l
RT: 6.967 min Scan# 1750
Delta R.T. -0.007 min
Lab File: VU048763.D
Acq: 01 Jun 2022 01:49

Tgt Ion: 88 Resp: 231
Ion Ratio Lower Upper
88 100
43 115.2 24.6 36.8#
58 94.4 54.7 82.1#


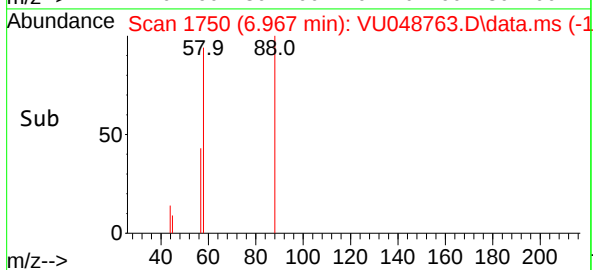

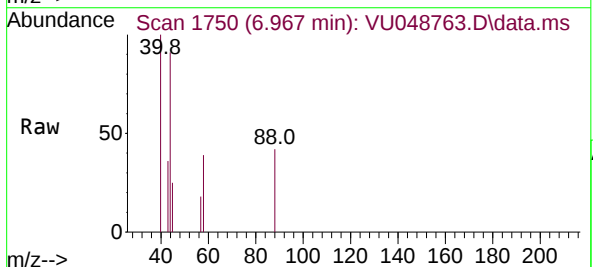


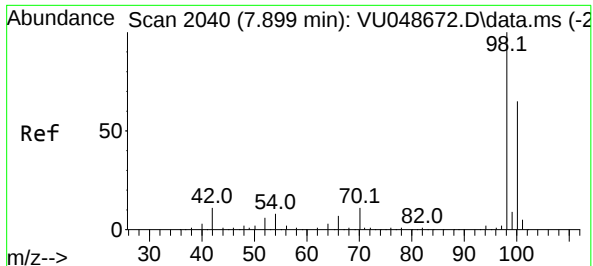

#50
Toluene-d8
Concen: 44.842 ug/l
RT: 7.899 min Scan# 2040
Delta R.T. -0.000 min
Lab File: VU048763.D
Acq: 01 Jun 2022 01:49




Instrument : MSVOA_U
ClientSampleId : 20220426-SPLP-AMENDED-COMPOSITE-F


Tgt Ion: 98 Resp: 400436
Ion Ratio Lower Upper
98 100
100 65.0 52.2 78.4

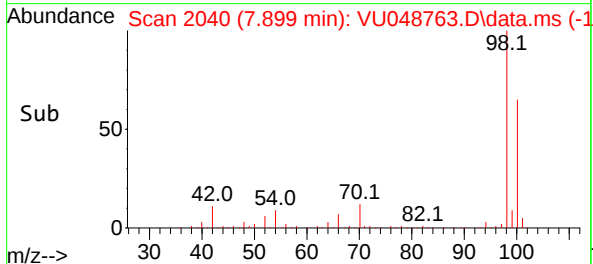

#51
4-Methyl-2-Pentanone
Concen: 0.875 ug/l
RT: 7.793 min Scan# 2007
Delta R.T. 0.003 min
Lab File: VU048763.D
Acq: 01 Jun 2022 01:49

Tgt Ion: 43 Resp: 3792
Ion Ratio Lower Upper
43 100
58 30.6 32.7 49.1#


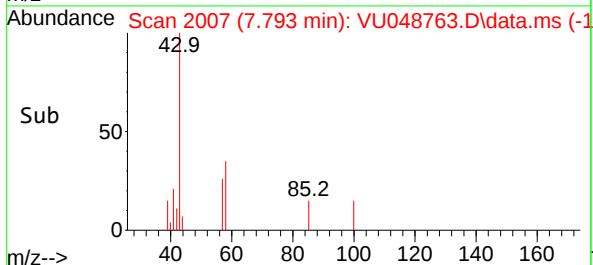

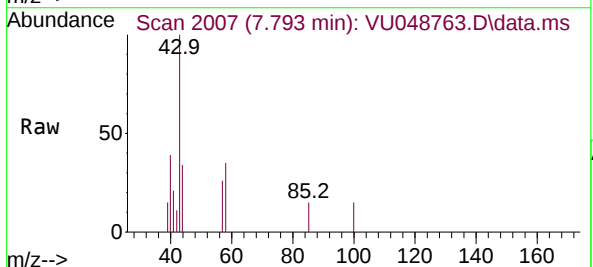




#59
2-Hexanone
Concen: 0.856 ug/l
RT: 8.687 min Scan# 21
Delta R.T. 0.003 min
Lab File: VU048763.D
Acq: 01 Jun 2022 01:49




Instrument :
MSVOA_U
ClientSampleId :
20220426-SPLP-AMENDED-COMPOSITE-F


Tgt Ion: 43 Resp: 3043
Ion Ratio Lower Upper
43 100
58 43.1 28.2 84.6

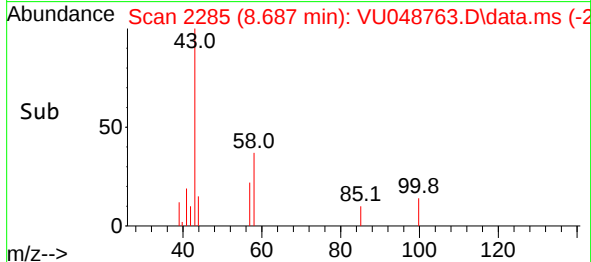

#62
4-Bromofluorobenzene
Concen: 42.986 ug/l
RT: 10.632 min Scan# 2890
Delta R.T. -0.000 min
Lab File: VU048763.D
Acq: 01 Jun 2022 01:49

Tgt Ion: 95 Resp: 145174
Ion Ratio Lower Upper
95 100
174 78.6 0.0 159.4
176 76.9 0.0 152.4


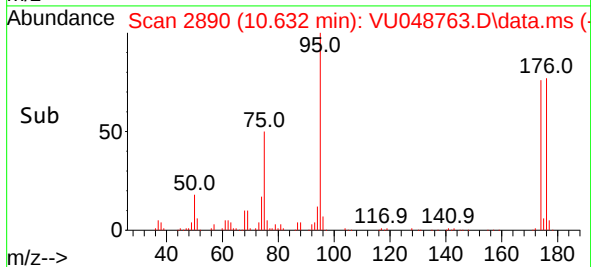

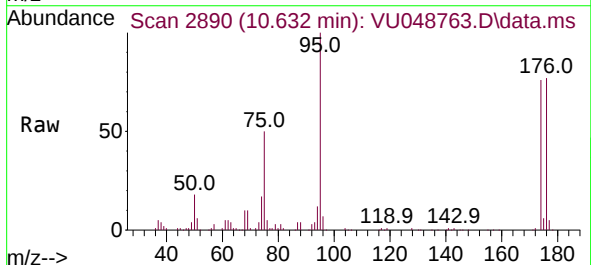




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 9.417 min Scan# 21
Delta R.T. -0.000 min
Lab File: VU048763.D
Acq: 01 Jun 2022 01:49




Instrument : MSVOA_U
ClientSampleId : 20220426-SPLP-AMENDED-COMPOSITE-F


Tgt Ion:117 Resp: 324236
Ion Ratio Lower Upper
117 100
82 57.3 45.3 67.9
119 31.4 25.4 38.2

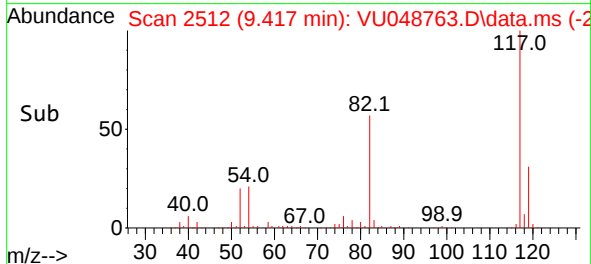

#64
Tetrachloroethene
Concen: Below Cal
RT: 8.558 min Scan# 2245
Delta R.T. 0.003 min
Lab File: VU048763.D
Acq: 01 Jun 2022 01:49

Tgt Ion:164 Resp: 87
Ion Ratio Lower Upper
164 100
166 158.5 105.0 157.4#
129 29.8 76.5 114.7#
131 67.3 73.8 110.6#


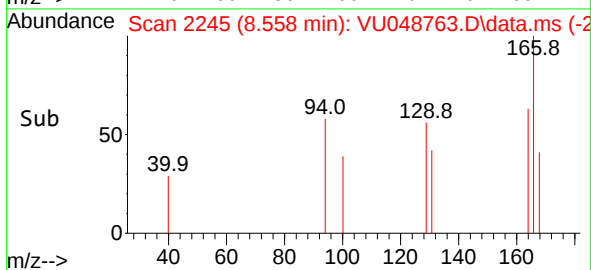

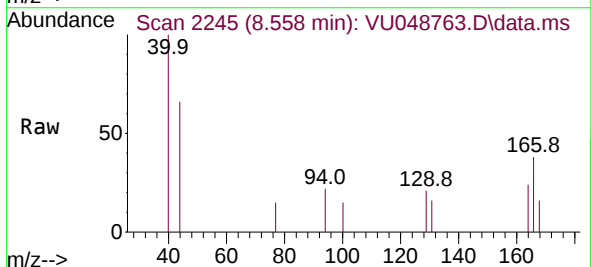




#65
Chlorobenzene
Concen: 0.370 ug/l
RT: 9.452 min Scan# 21
Delta R.T. 0.006 min
Lab File: VU048763.D
Acq: 01 Jun 2022 01:49




Instrument :
MSVOA_U
ClientSampleId :
20220426-SPLP-AMENDED-COMPOSITE-F


Tgt Ion:112 Resp: 2536
Ion Ratio Lower Upper
112 100
114 26.5 26.3 39.5

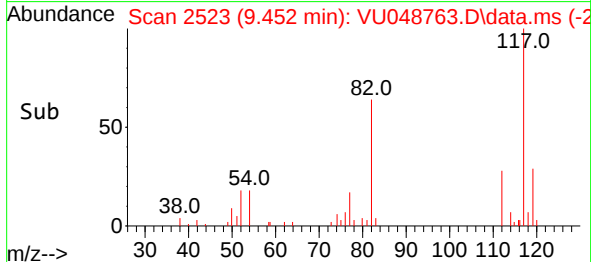

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 11.812 min Scan# 3257
Delta R.T. 0.003 min
Lab File: VU048763.D
Acq: 01 Jun 2022 01:49

Tgt Ion:152 Resp: 154441
Ion Ratio Lower Upper
152 100
115 60.3 41.8 125.4
150 157.8 0.0 341.0


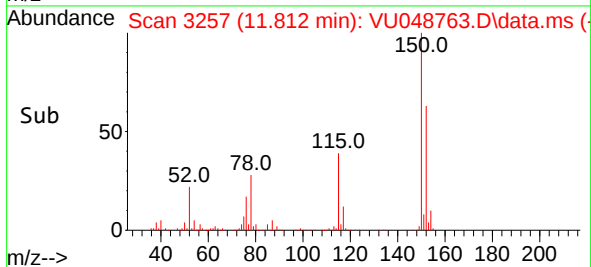

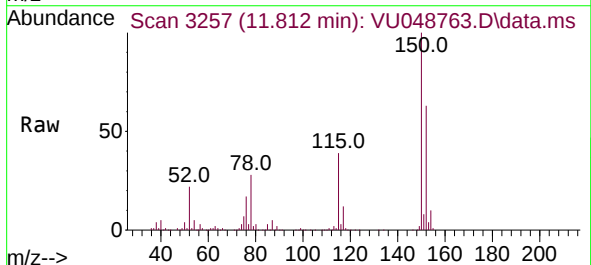


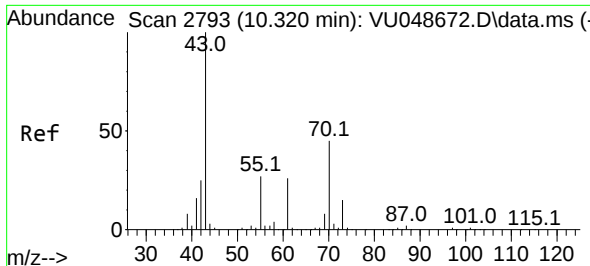

#74
N-amy1 acetate
Concen: 2.535 ug/l
RT: 10.327 min Scan# 21
Delta R.T. 0.007 min
Lab File: VU048763.D
Acq: 01 Jun 2022 01:49




Instrument : MSVOA_U
ClientSampleId : 20220426-SPLP-AMENDED-COMPOSITE-F


Tgt Ion: 43	Resp: 360
Ion Ratio	Lower Upper
43 100	
70 0.0	35.8 53.6#
55 0.0	21.1 31.7#
61 0.0	20.2 30.4#

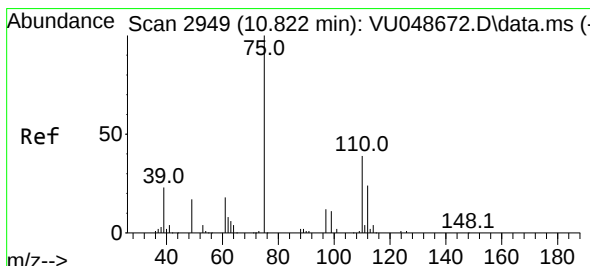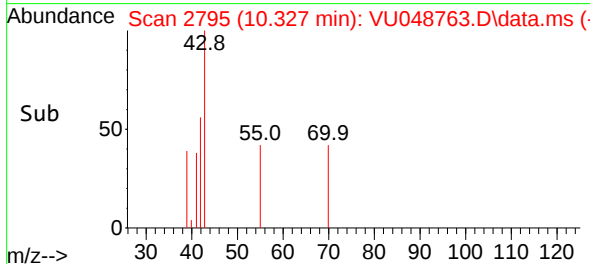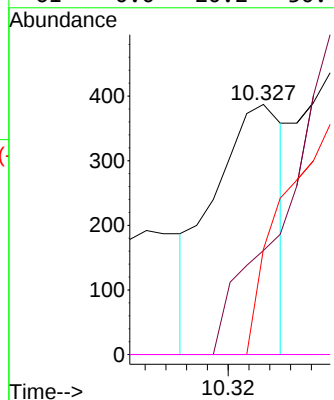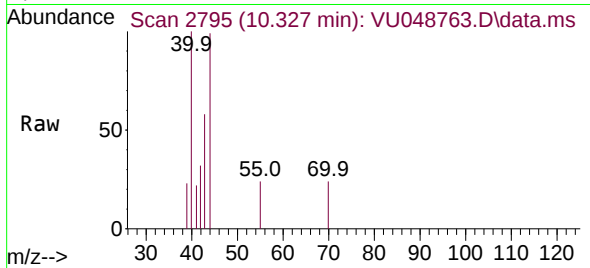

#76
1,2,3-Trichloropropane
Concen: 14.774 ug/l
RT: 10.632 min Scan# 2890
Delta R.T. -0.190 min
Lab File: VU048763.D
Acq: 01 Jun 2022 01:49

Tgt Ion: 75	Resp: 73569
Ion Ratio	Lower Upper
75 100	
77 1.2	14.8 44.3#


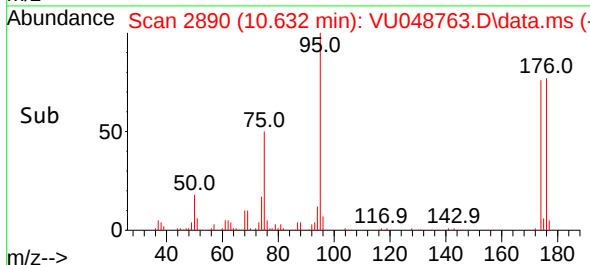
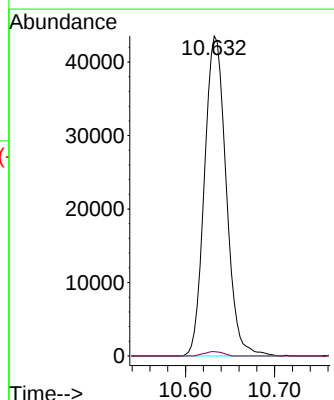
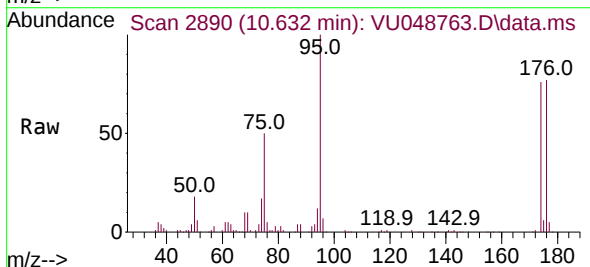


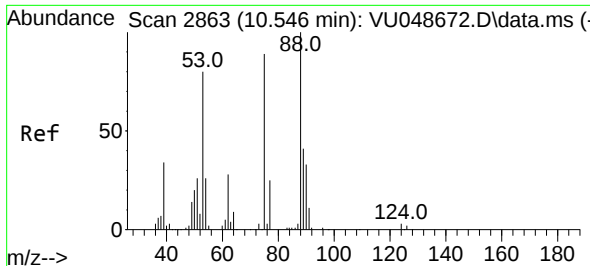

#81
trans-1,4-Dichloro-2-butene
Concen: 53.643 ug/l
RT: 10.632 min Scan# 21
Delta R.T. 0.087 min
Lab File: VU048763.D
Acq: 01 Jun 2022 01:49




Instrument : MSVOA_U
ClientSampleId : 20220426-SPLP-AMENDED-COMPOSITE-F


Tgt Ion: 75 Resp: 73569
Ion Ratio Lower Upper
75 100
53 0.1 72.5 108.7#
89 0.1 37.0 55.4#

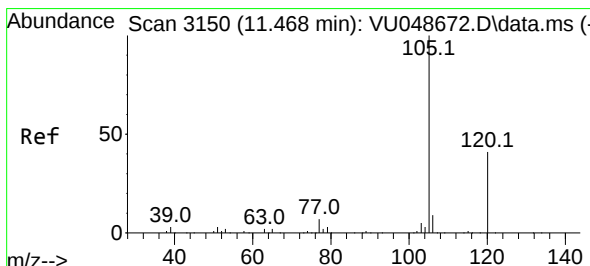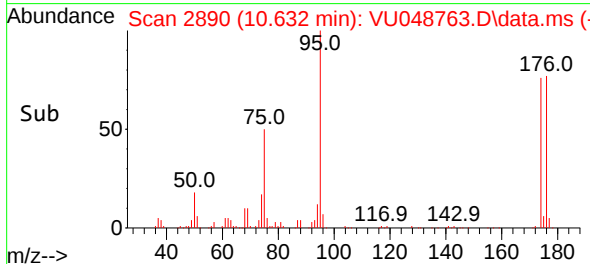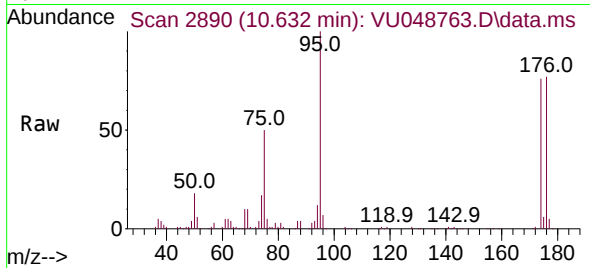

#84
1,2,4-Trimethylbenzene
Concen: 1.349 ug/l
RT: 11.475 min Scan# 3152
Delta R.T. 0.007 min
Lab File: VU048763.D
Acq: 01 Jun 2022 01:49

Tgt Ion: 105 Resp: 1547
Ion Ratio Lower Upper
105 100
120 10.8 22.5 67.5#

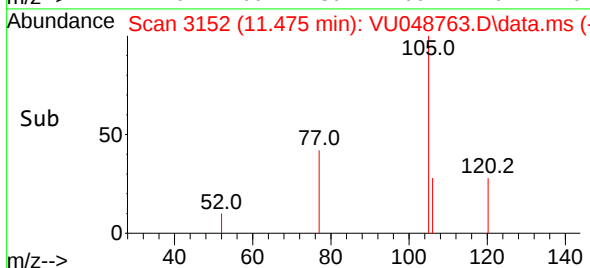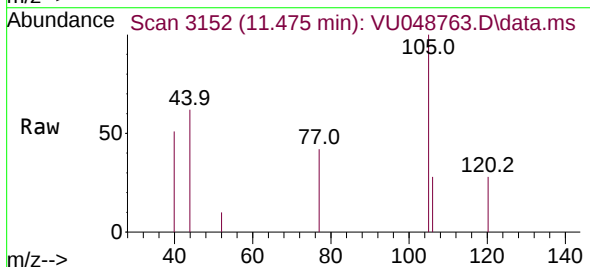



#89

n-Butylbenzene

Concen: 2.303 ug/l

RT: 12.208 min Scan# 31

Delta R.T. -0.000 min

Lab File: VU048763.D

Acq: 01 Jun 2022 01:49





Instrument :

MSVOA_U

ClientSampleId :

20220426-SPLP-AMENDED-COMPOSITE-F

Tgt Ion: 91	Resp:	1098
Ion	Ratio	Lower Upper
91	100	
92	52.3	25.9 77.8
134	10.6	12.5 37.5#

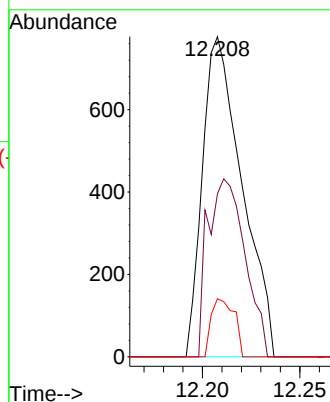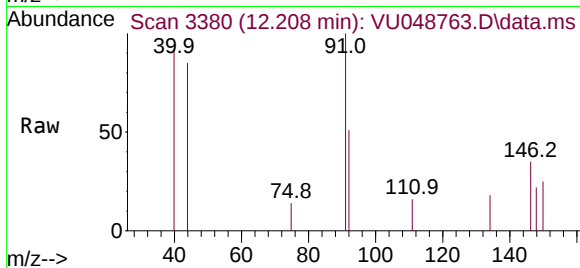

#92

1,2-Dibromo-3-Chloropropane

Concen: 0.423 ug/l




RT: 13.153 min Scan# 3674


Delta R.T. 0.157 min

Lab File: VU048763.D

Acq: 01 Jun 2022 01:49

Tgt Ion: 75	Resp:	496
Ion	Ratio	Lower Upper
75	100	
155	0.0	40.3 120.8#
157	0.0	50.0 150.0#


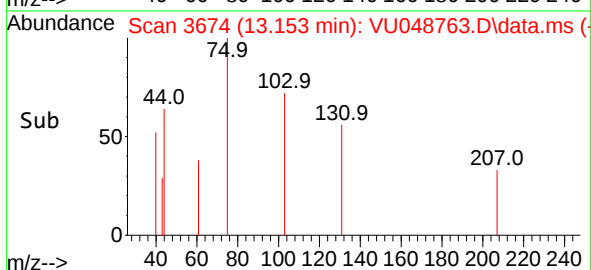

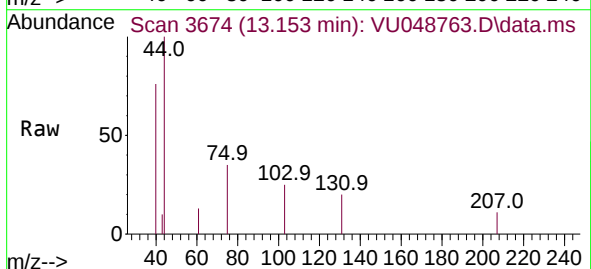




#93
1,2,4-Trichlorobenzene
Concen: 0.262 ug/l
RT: 13.848 min Scan# 3887
Delta R.T. 0.010 min
Lab File: VU048763.D
Acq: 01 Jun 2022 01:49




Instrument : MSVOA_U
ClientSampleId : 20220426-SPLP-AMENDED-COMPOSITE-F


Tgt Ion:180 Resp: 911
Ion Ratio Lower Upper
180 100
182 45.9 48.3 144.9#
145 22.8 15.6 46.7

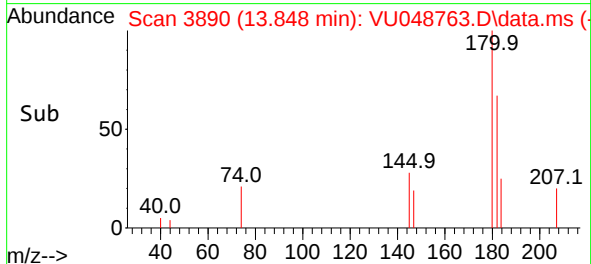

#95
Naphthalene
Concen: 2.993 ug/l
RT: 14.092 min Scan# 3966
Delta R.T. 0.006 min
Lab File: VU048763.D
Acq: 01 Jun 2022 01:49


Tgt Ion:128 Resp: 5893
Ion Ratio Lower Upper
128 100
127 13.6 10.2 15.4
129 9.2 8.7 13.1

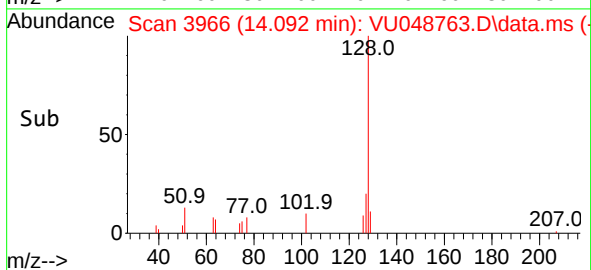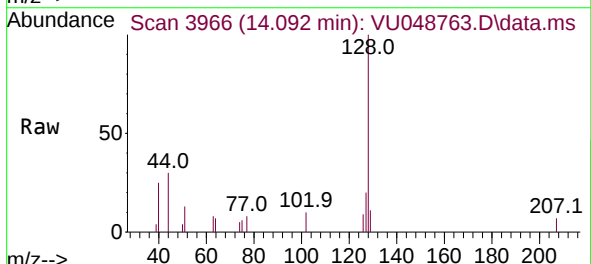



#96
 1,2,3-Trichlorobenzene
 Concen: 0.220 ug/l
 RT: 14.333 min Scan# 40
 Delta R.T. 0.006 min
 Lab File: VU048763.D
 Acq: 01 Jun 2022 01:49

Instrument :
 MSVOA_U
 ClientSampleId :
 20220426-SPLP-AMENDED-COMPOSITE-F



Tgt Ion:	180	Resp:	759
Ion	Ratio	Lower	Upper
180	100		
182	108.3	47.4	142.2
145	27.4	16.6	49.8

