


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU053123\
Data File : VU054329.D
Acq On : 31 May 2023 09:30
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U052523W.M
Title : SW846 8260
Last Update : Fri May 26 06:40:51 2023

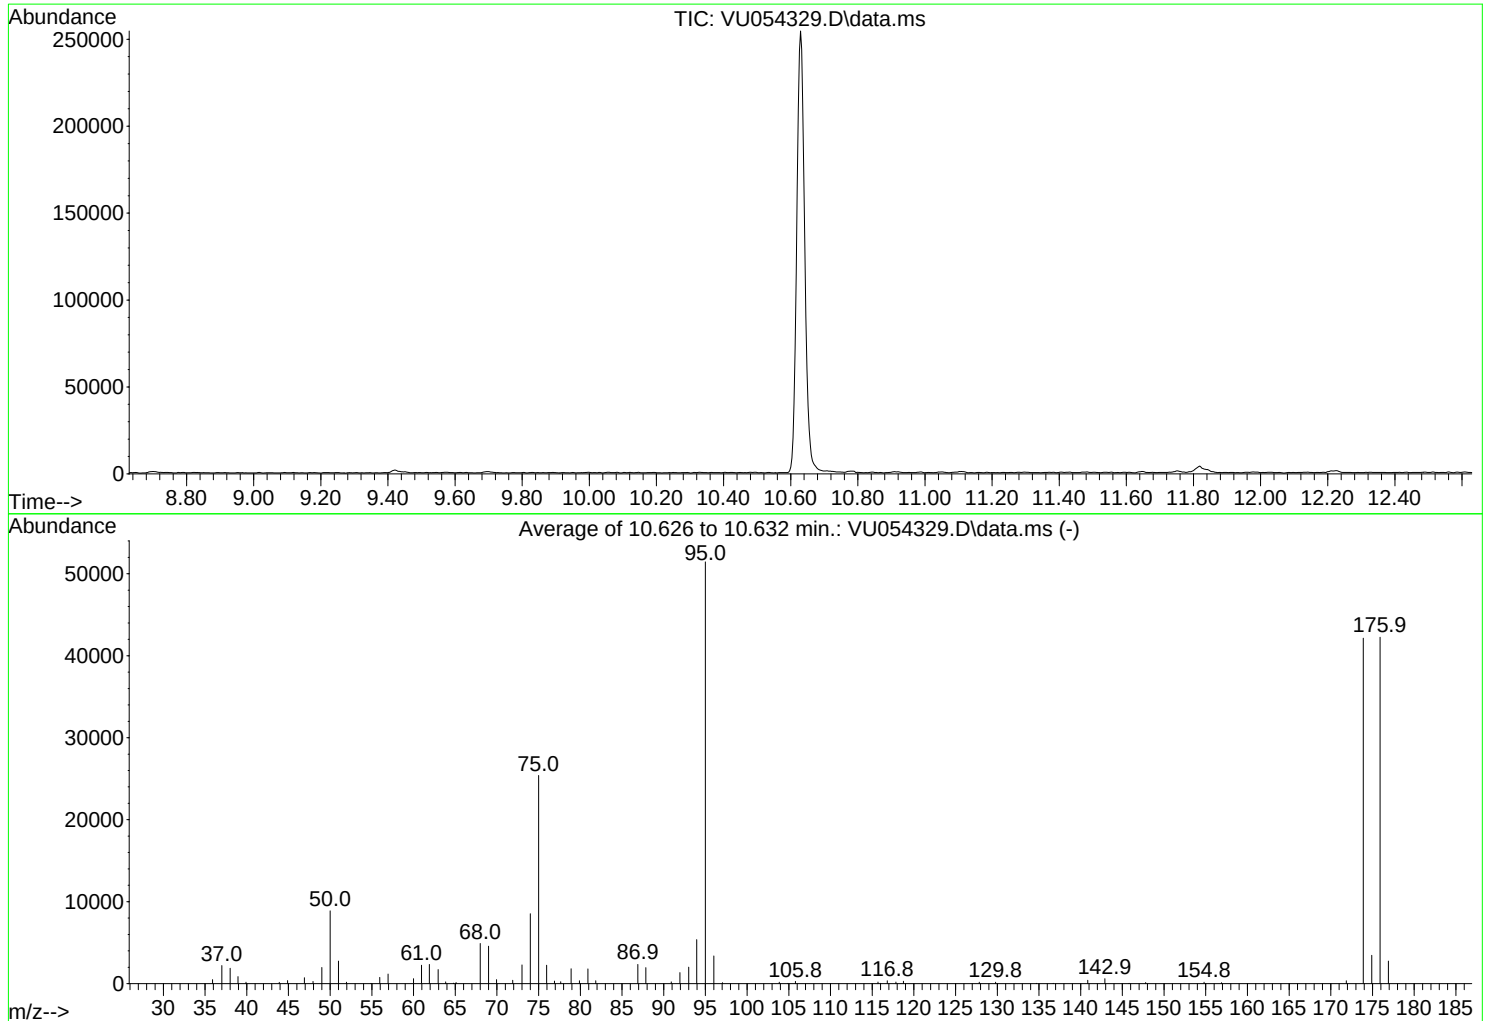

AutoFind: Scans 2888, 2889, 2890; Background Corrected with Scan 2875

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.3	8882	PASS
75	95	30	60	49.4	25403	PASS
95	95	100	100	100.0	51456	PASS
96	95	5	9	6.6	3378	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	81.9	42139	PASS
175	174	5	9	8.2	3451	PASS
176	174	95	101	100.3	42267	PASS
177	176	5	9	6.5	2755	PASS