
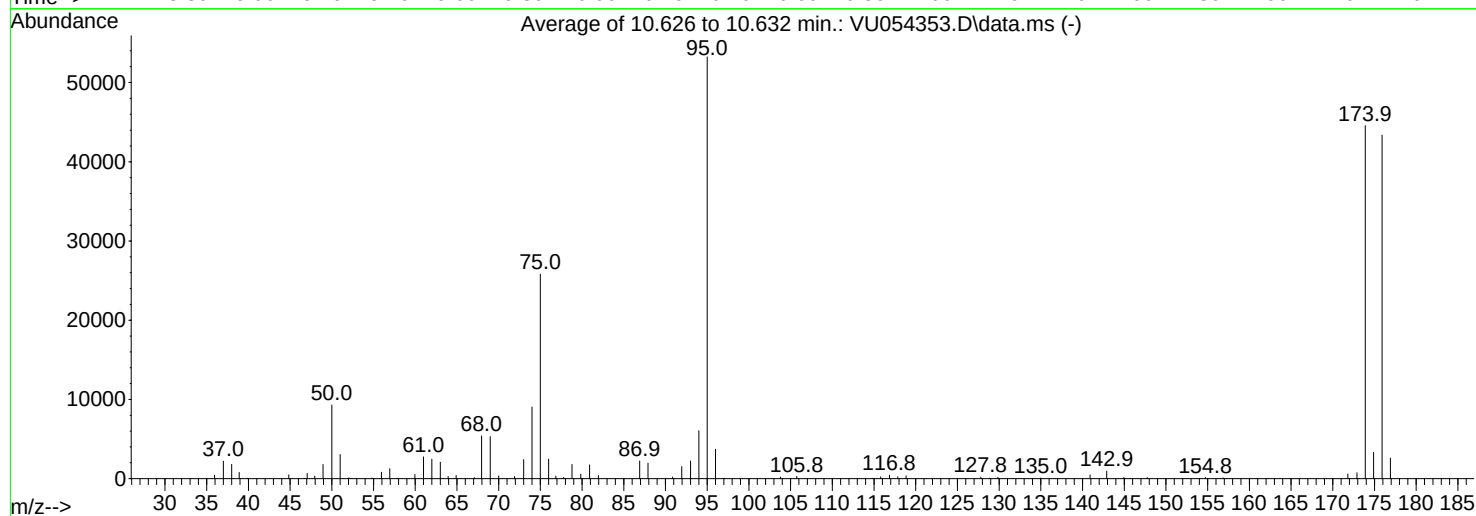


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU053123\
Data File : VU054353.D
Acq On : 31 May 2023 21:45
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM060123WMA.M
Title : VOC Analysis
Last Update : Fri Jun 02 01:40:39 2023

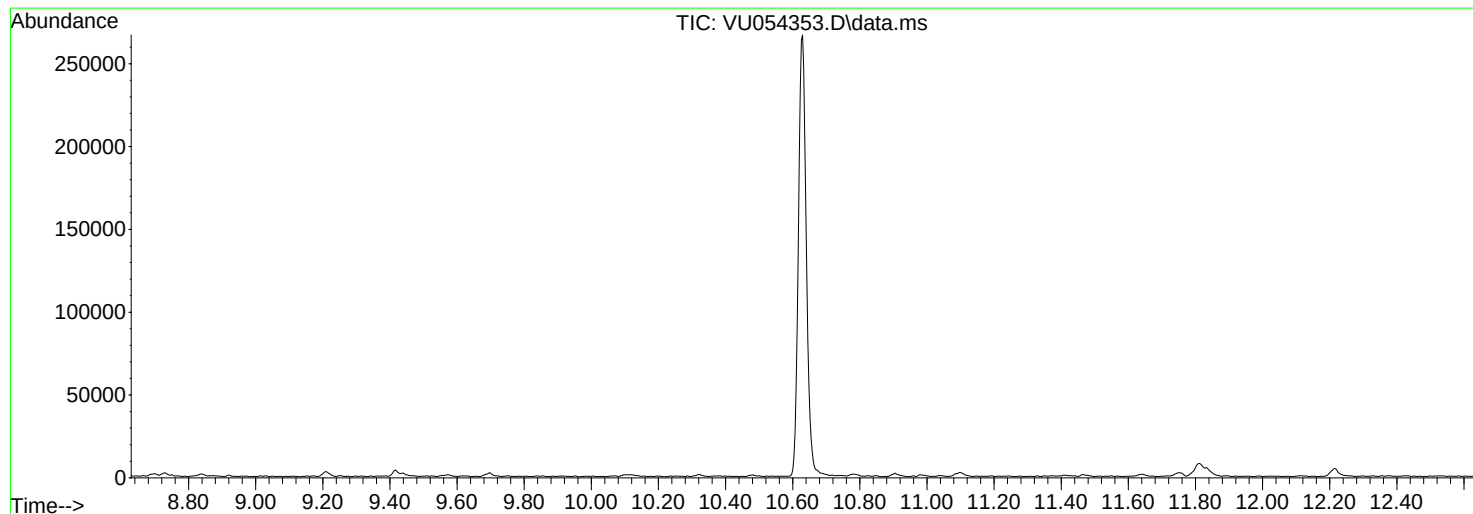

AutoFind: Scans 2888, 2889, 2890; Background Corrected with Scan 2876

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.4	9285	PASS
75	95	30	80	48.5	25821	PASS
95	95	100	100	100.0	53245	PASS
96	95	5	9	7.0	3722	PASS
173	174	0.00	2	1.7	740	PASS
174	95	50	120	83.7	44584	PASS
175	174	5	9	7.4	3316	PASS
176	174	95	101	97.3	43365	PASS
177	176	5	9	6.0	2588	PASS