


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU060120\
 Data File : VU038458.D
 Acq On : 01 Jun 2020 08:52
 Operator : JC/MD
 Sample : BFB04
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB04

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR053120WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Tue Jun 02 05:25:28 2020

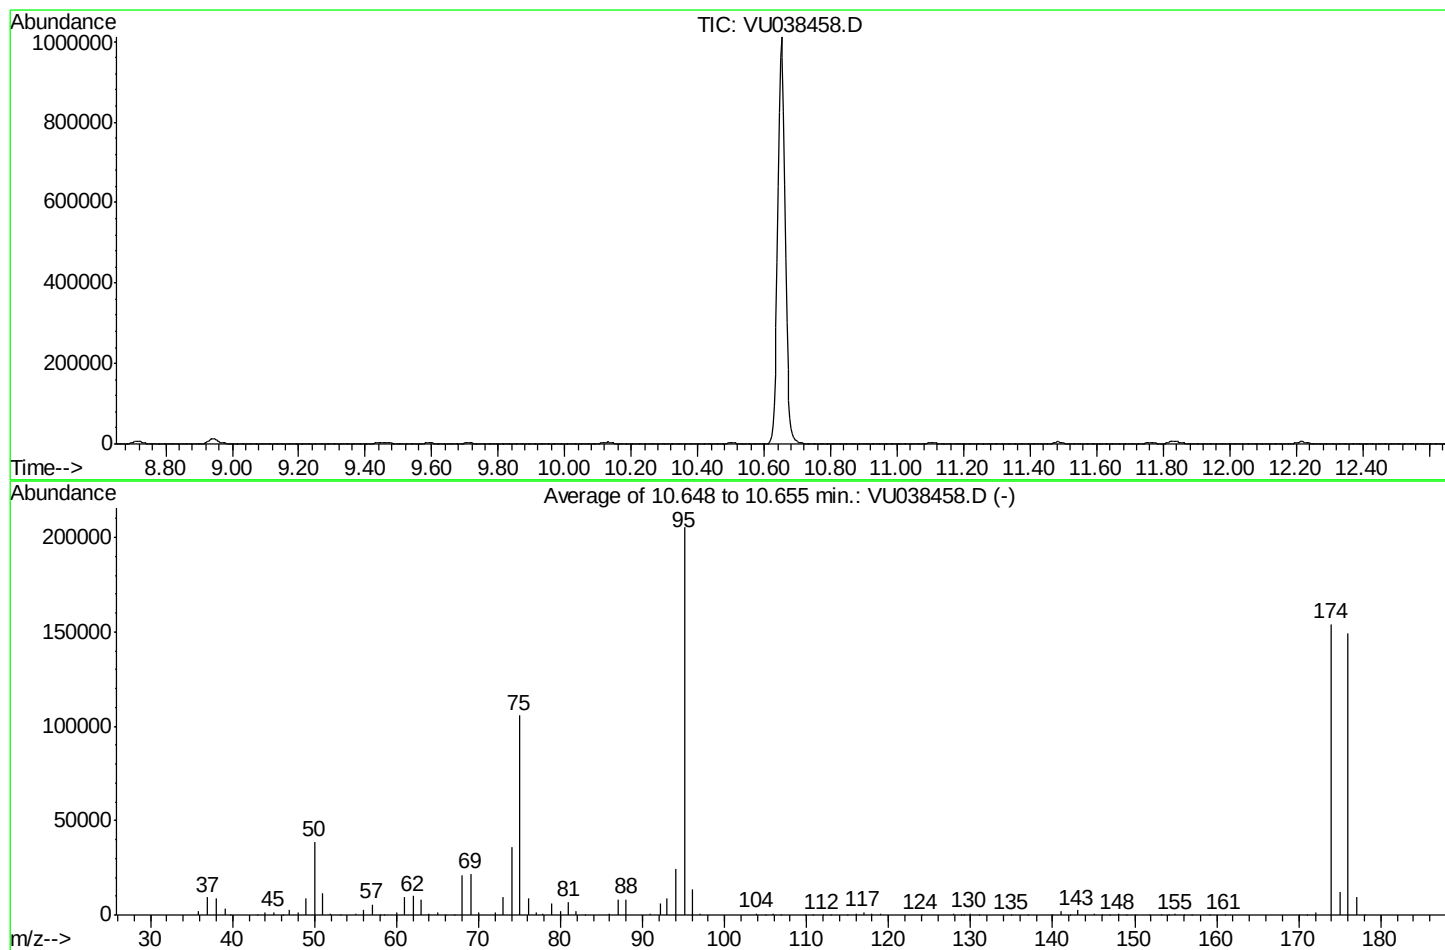

AutoFind: Scans 2895, 2896, 2897; Background Corrected with Scan 2881

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.0	38984	PASS
75	95	30	80	51.5	105781	PASS
95	95	100	100	100.0	205397	PASS
96	95	5	9	6.7	13737	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	75.0	154112	PASS
175	174	5	9	7.8	11986	PASS
176	174	95	101	96.8	149248	PASS
177	176	5	9	6.4	9557	PASS

m/z	Abundance
35.90	1870.0
37.00	9186.0
38.00	8848.0
39.00	3254.0
39.80	419.0
42.90	106.0
44.00	1767.0
45.00	1534.0
46.10	276.0
46.90	2632.0
48.00	1430.0
49.00	8698.0
50.00	39040.0
51.00	11760.0
52.00	682.0
53.10	155.0
55.20	507.0
56.00	2852.0
57.00	5719.0
57.90	245.0
58.50	131.0
60.00	1706.0
61.00	9655.0
62.00	9763.0
63.00	7799.0
64.00	799.0
65.00	1437.0
67.00	778.0
68.00	20584.0
69.00	21952.0
70.00	1757.0
72.00	1093.0
73.00	9331.0
74.00	35576.0
75.00	104792.0
76.00	8751.0
77.10	1159.0
77.80	725.0
78.90	6037.0
80.00	1898.0
80.90	6726.0
81.90	1809.0
82.90	190.0
86.00	474.0
87.00	8125.0
88.00	8338.0
90.90	815.0
92.10	6181.0
93.00	9057.0
94.10	23704.0
95.10	202304.0
96.10	14448.0
97.10	388.0
103.90	940.0
104.90	333.0
105.90	877.0
106.90	221.0
109.80	191.0
110.80	189.0
112.00	173.0
112.90	151.0
114.90	247.0
116.00	749.0
116.90	1353.0
117.90	786.0
119.00	969.0
124.10	148.0
127.90	651.0
128.90	381.0
129.90	916.0
131.00	301.0
135.00	248.0
136.90	296.0
141.00	1866.0
142.10	291.0
143.00	2472.0
145.00	371.0
145.90	390.0
146.90	184.0
148.00	512.0
148.90	123.0
150.00	163.0
153.20	122.0
154.10	122.0
155.00	498.0
156.00	126.0
156.90	344.0
159.00	222.0
161.00	270.0
171.00	207.0
172.00	1360.0
174.00	148224.0

Instrument :
MSVOA_U
ClientSampleId :
BFB04

175.10	11817.0
176.00	142592.0
177.00	9482.0
178.00	248.0

Instrument :
MSVOA_U
ClientSampleId :
BFB04

m/z	Abundance
35.90	1831.0
37.00	9629.0
38.00	8894.0
39.10	3315.0
39.90	333.0
42.90	137.0
44.00	1773.0
45.00	1424.0
46.10	261.0
46.90	2633.0
48.00	1320.0
49.00	9063.0
50.00	40440.0
51.00	12074.0
52.00	609.0
53.10	157.0
55.00	551.0
56.00	3112.0
57.00	5842.0
58.00	215.0
60.00	1724.0
61.00	9817.0
62.00	10265.0
63.00	8184.0
64.00	933.0
65.00	1495.0
68.00	21560.0
69.00	22440.0
70.00	1723.0
72.00	1095.0
73.10	9731.0
74.00	37216.0
75.00	109528.0
76.00	9137.0
77.10	1264.0
77.80	722.0
78.90	6219.0
80.00	2133.0
80.90	7082.0
81.90	1831.0
82.90	208.0
85.90	452.0
87.00	8486.0
88.00	8517.0
90.90	917.0
92.10	6614.0
93.00	9406.0
94.10	24944.0
95.10	212544.0
96.10	14089.0
97.10	405.0
103.90	1005.0
104.90	347.0
105.90	784.0
106.90	259.0
109.80	144.0
110.80	149.0
111.90	222.0
112.90	138.0
114.90	251.0
116.00	839.0
116.90	1495.0
117.90	851.0
118.90	1025.0
123.90	119.0
127.90	753.0
129.10	371.0
129.90	938.0
131.10	301.0
135.00	346.0
136.90	285.0
140.00	110.0
141.00	2070.0
142.00	279.0
143.00	2686.0
145.00	399.0
145.90	342.0
146.90	163.0
148.00	509.0
149.00	206.0
150.00	185.0
153.10	125.0
155.00	482.0
156.00	145.0
157.00	327.0
159.00	245.0
160.90	227.0
171.00	216.0
172.00	1495.0
174.00	159168.0
175.10	12441.0
176.00	154560.0

Instrument :
MSVOA_U
ClientSampleId :
BFB04

177.009952.0

178.00308.0

Instrument :
MSVOA_U

ClientSampleId :
BFB04

m/z	Abundance
35.90	1496.0
37.00	9183.0
38.00	7920.0
39.10	3217.0
39.90	212.0
43.00	169.0
44.00	1577.0
45.00	1329.0
46.10	209.0
47.00	2360.0
47.90	1129.0
49.00	8471.0
50.00	37472.0
51.00	11383.0
51.90	492.0
53.10	113.0
54.90	540.0
56.00	3070.0
57.00	5173.0
58.00	166.0
60.10	1687.0
61.00	9166.0
62.00	9745.0
63.00	7738.0
64.00	933.0
65.00	1266.0
65.90	106.0
68.00	20680.0
69.00	21040.0
70.10	1560.0
72.00	960.0
73.10	9089.0
74.00	35048.0
75.00	103024.0
76.10	8945.0
77.00	1250.0
77.80	637.0
79.00	6037.0
80.00	2158.0
81.00	6682.0
81.90	1629.0
83.00	191.0
85.90	332.0
87.00	8013.0
88.00	7815.0
90.90	858.0
92.10	6197.0
93.00	8520.0
94.10	23856.0
95.10	201344.0
96.00	12674.0
97.00	342.0
103.90	900.0
104.90	287.0
105.90	679.0
106.80	254.0
109.80	131.0
110.90	109.0
112.00	193.0
112.90	154.0
114.90	186.0
116.00	834.0
117.00	1415.0
117.90	787.0
118.90	1008.0
123.90	105.0
128.00	856.0
128.90	366.0
129.90	894.0
131.10	261.0
135.00	427.0
136.90	262.0
139.90	117.0
141.00	2109.0
142.00	273.0
143.00	2580.0
145.00	371.0
146.00	278.0
146.90	139.0
148.00	390.0
149.10	242.0
150.00	186.0
151.80	108.0
153.10	142.0
154.90	434.0
156.00	149.0
157.00	326.0
159.10	253.0
160.90	185.0
170.10	102.0
171.10	186.0
172.00	1419.0

Instrument :
MSVOA_U
ClientSampleId :
BFB04

174.00	154944.0
175.10	11701.0
176.00	150592.0
177.00	9238.0
178.00	294.0

Instrument :
MSVOA_U
ClientSampleId :
BFB04

Scan 2881 (10.603 min): VU038458.D
BFB04

m/z	Abundance
39.80	191.0
43.90	622.0

Instrument :
MSVOA_U
ClientSampleId :
BFB04