

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060122\
 Data File : VU048779.D
 Acq On : 01 Jun 2022 14:10
 Operator : SY/MD
 Sample : N3030-08DL 4X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 HW-1DL

Quant Time: Jun 02 05:03:09 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U052622W.M
 Quant Title : SW846 8260
 QLast Update : Fri May 27 06:42:31 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.375	168	265640	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.250	114	445880	50.000	ug/l	0.00
63) Chlorobenzene-d5	9.420	117	423711	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	11.812	152	218268	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.703	65	190420	47.731	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	95.460%
35) Dibromofluoromethane	5.292	113	150314	47.254	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	94.500%
50) Toluene-d8	7.899	98	538418	47.218	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	94.440%
62) 4-Bromofluorobenzene	10.632	95	204910	47.516	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	95.040%


Target Compounds			Qvalue			
3) Chloromethane	1.469	50	6930	1.770	ug/l #	43
5) Bromomethane	1.861	94	43	Below Cal	#	3
6) Chloroethane	2.089	64	1202	Below Cal	#	46
10) Methyl Iodide	2.449	142	22	3.009	ug/l #	37
11) Tert butyl alcohol	3.176	59	59746	59.071	ug/l #	41
13) Acrolein	2.475	56	46	Below Cal	#	1
14) Allyl chloride	3.176	41	11943	2.281	ug/l #	65
15) Acrylonitrile	3.362	53	4278	1.950	ug/l #	28
16) Acetone	2.633	43	3595	1.768	ug/l	92
17) Carbon Disulfide	2.793	76	2241	0.284	ug/l	96
19) Methyl tert-butyl Ether	3.362	73	376851	36.735	ug/l	96
20) Methylene Chloride	3.047	84	1272	0.368	ug/l #	92
29) Tetrahydrofuran	5.067	42	599	0.326	ug/l #	62
31) Cyclohexane	5.375	56	5792	1.152	ug/l #	1
36) 1,1-Dichloropropene	5.372	75	21793	4.694	ug/l #	49
38) Carbon Tetrachloride	5.375	117	27413	5.147	ug/l #	18
43) Isopropyl Acetate	5.825	43	16631	1.952	ug/l #	60
49) 1,4-Dioxane	6.983	88	22	0.257	ug/l #	1
51) 4-Methyl-2-Pentanone	7.793	43	2477	0.448	ug/l #	83
56) Ethyl methacrylate	8.330	69	156	2.639	ug/l #	1
59) 2-Hexanone	8.690	43	2770	0.610	ug/l	81
74) N-amyl acetate	10.327	43	592	2.546	ug/l #	76
76) 1,2,3-Trichloropropane	10.632	75	102690	14.592	ug/l #	48
81) trans-1,4-Dichloro-2-b...	10.632	75	102690	52.981	ug/l #	13
84) 1,2,4-Trimethylbenzene	11.472	105	2267	1.355	ug/l	85
89) n-Butylbenzene	12.214	91	1407	2.292	ug/l #	79
90) Hexachloroethane	12.613	117	1215	0.471	ug/l #	10
93) 1,2,4-Trichlorobenzene	13.844	180	1126	0.229	ug/l	81
95) Naphthalene	14.089	128	137184	10.113	ug/l	99
96) 1,2,3-Trichlorobenzene	14.333	180	1046	0.215	ug/l #	85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060122\
Data File : VU048779.D
Acq On : 01 Jun 2022 14:10
Operator : SY/MD
Sample : N3030-08DL 4X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
HW-1DL

Quant Time: Jun 02 05:03:09 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U052622W.M
Quant Title : SW846 8260
QLast Update : Fri May 27 06:42:31 2022
Response via : Initial Calibration




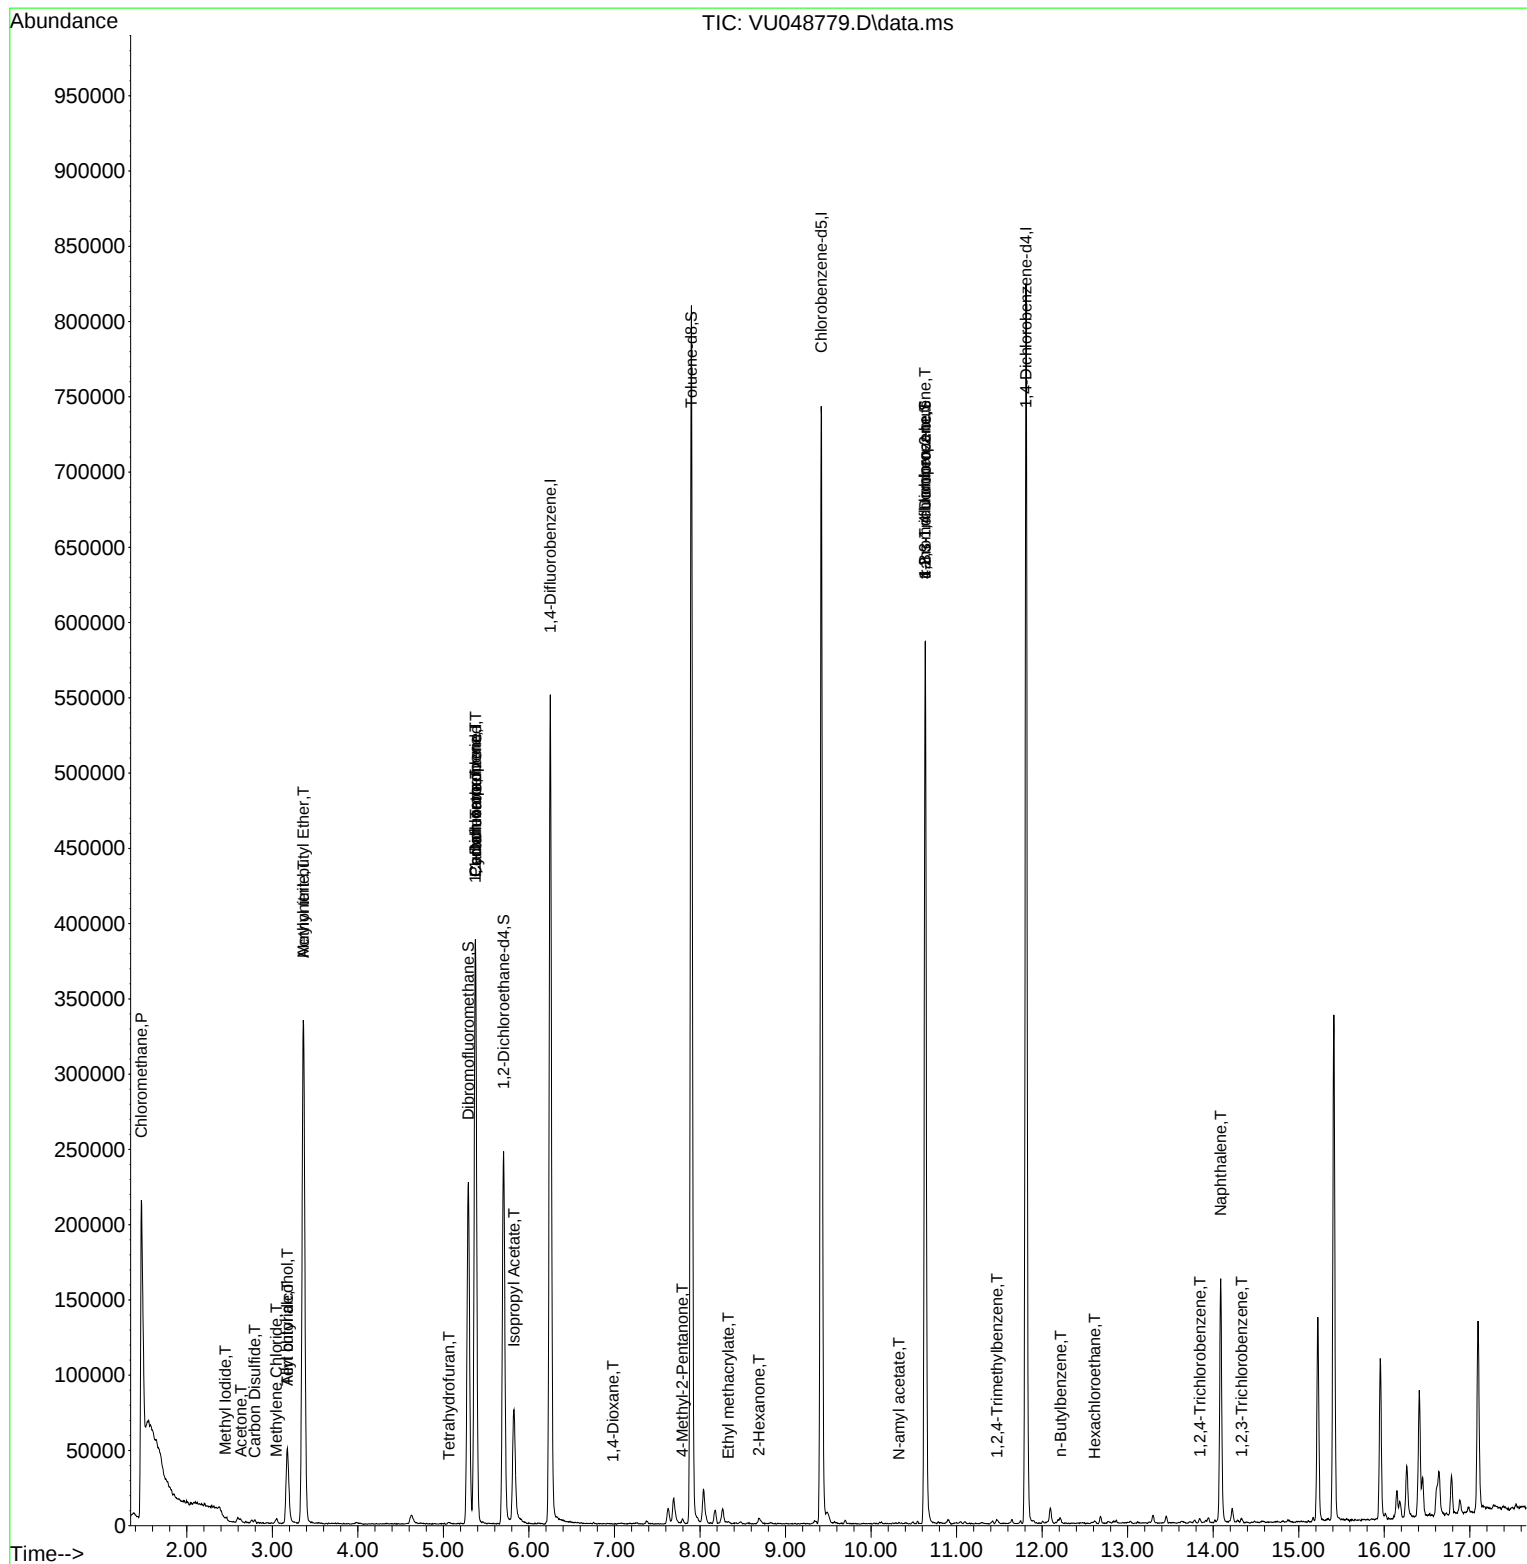




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.375 min Scan# 11
Delta R.T. 0.000 min
Lab File: VU048779.D
Acq: 01 Jun 2022 14:10




Instrument :
MSVOA_U
ClientSampleId :
HW-1DL


Tgt Ion:168 Resp: 265640
Ion Ratio Lower Upper
168 100
99 58.2 49.3 73.9

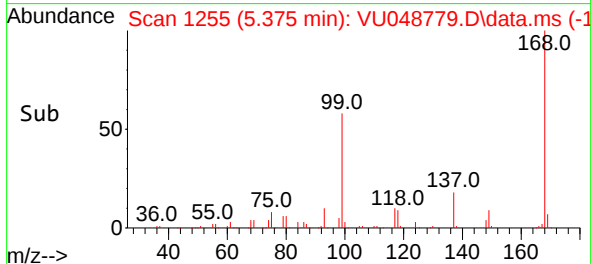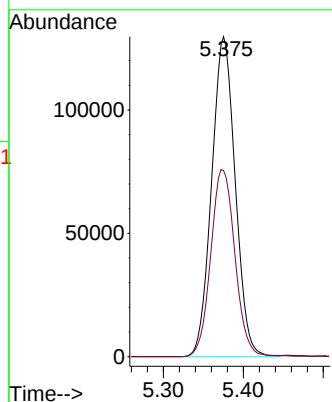

#3
Chloromethane
Concen: 1.770 ug/l
RT: 1.469 min Scan# 40
Delta R.T. -0.055 min
Lab File: VU048779.D
Acq: 01 Jun 2022 14:10

Tgt Ion: 50 Resp: 6930
Ion Ratio Lower Upper
50 100
52 0.0 25.7 38.5#


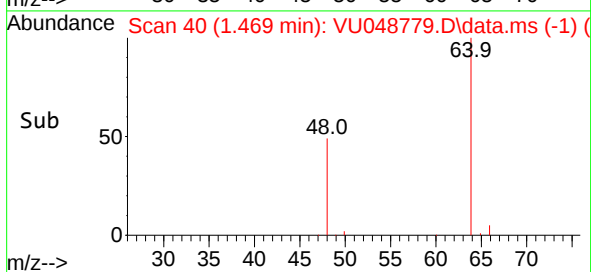
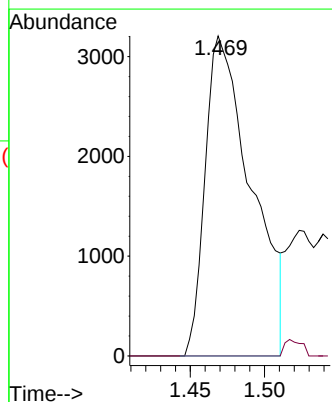





#5
Bromomethane
Concen: Below Cal
RT: 1.861 min Scan# 11
Delta R.T. 0.010 min
Lab File: VU048779.D
Acq: 01 Jun 2022 14:10




Instrument :
MSVOA_U
ClientSampleId :
HW-1DL


Tgt Ion: 94 Resp: 43
Ion Ratio Lower Upper
94 100
96 0.0 75.1 112.7#

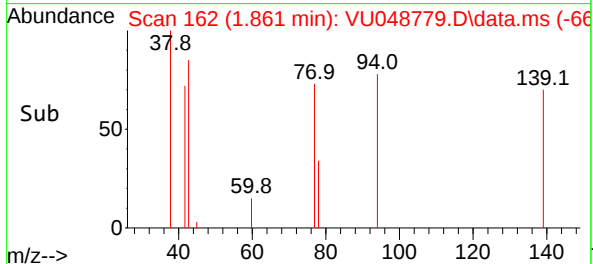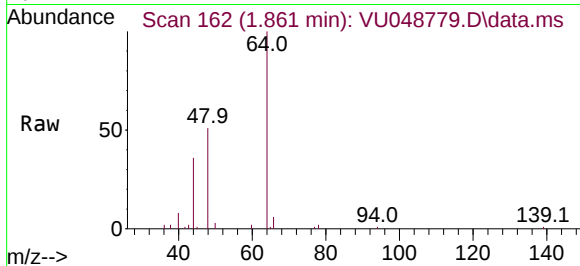

#6
Chloroethane
Concen: Below Cal
RT: 2.089 min Scan# 233
Delta R.T. 0.157 min
Lab File: VU048779.D
Acq: 01 Jun 2022 14:10

Tgt Ion: 64 Resp: 1202
Ion Ratio Lower Upper
64 100
66 1.6 25.2 37.8#


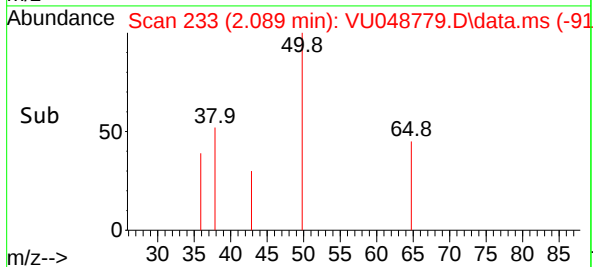

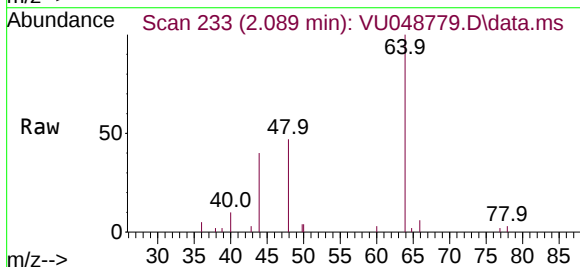




#10
Methyl Iodide
Concen: 3.009 ug/l
RT: 2.449 min Scan# 341
Delta R.T. -0.274 min
Lab File: VU048779.D
Acq: 01 Jun 2022 14:10




Instrument :
MSVOA_U
ClientSampleId :
HW-1DL


Tgt Ion:142 Resp: 22
Ion Ratio Lower Upper
142 100
127 0.0 38.4 57.6#
141 0.0 11.5 17.3#

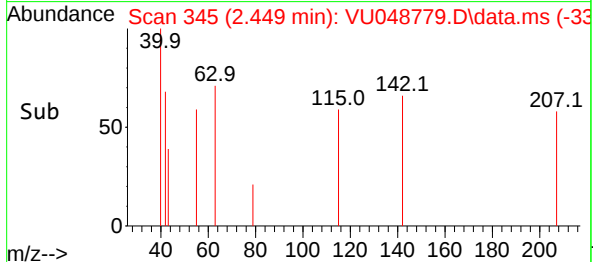

#11
Tert butyl alcohol
Concen: 59.071 ug/l
RT: 3.176 min Scan# 571
Delta R.T. -0.013 min
Lab File: VU048779.D
Acq: 01 Jun 2022 14:10

Tgt Ion: 59 Resp: 59746
Ion Ratio Lower Upper
59 100
57 8.8 39.7 59.5#


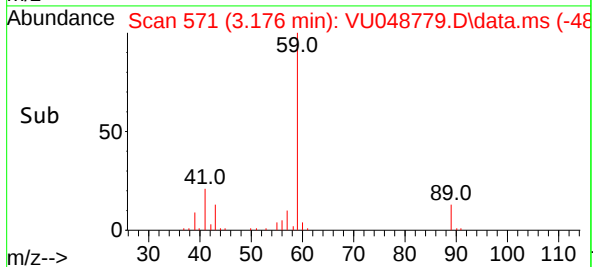

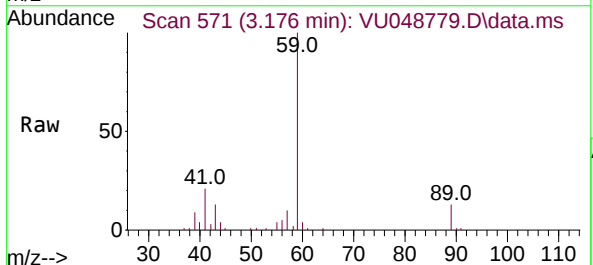




#13
Acrolein
Concen: Below Cal
RT: 2.475 min Scan# 31
Delta R.T. -0.013 min
Lab File: VU048779.D
Acq: 01 Jun 2022 14:10




Instrument :
MSVOA_U
ClientSampleId :
HW-1DL


Tgt Ion: 56 Resp: 46
Ion Ratio Lower Upper
56 100
55 1626.1 57.7 86.5#

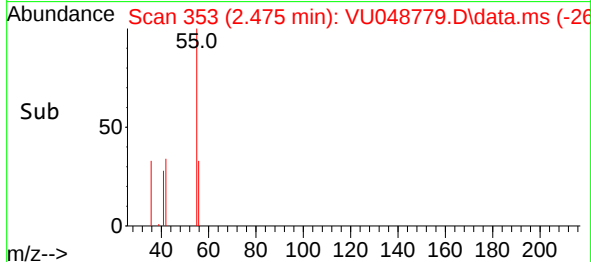

#14
Allyl chloride
Concen: 2.281 ug/l
RT: 3.176 min Scan# 571
Delta R.T. 0.251 min
Lab File: VU048779.D
Acq: 01 Jun 2022 14:10

Tgt Ion: 41 Resp: 11943
Ion Ratio Lower Upper
41 100
39 42.8 48.6 72.8#
76 2.2 27.0 40.4#


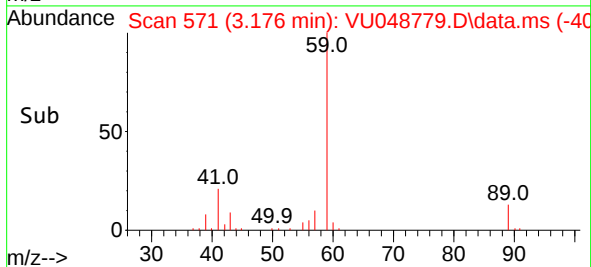

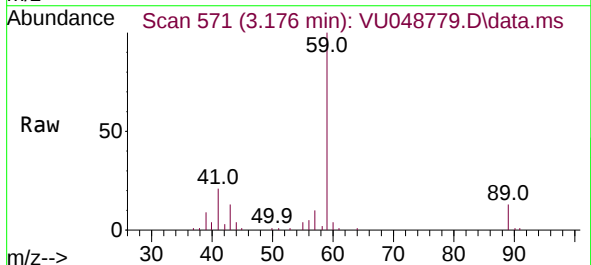




#15
Acrylonitrile
Concen: 1.950 ug/l
RT: 3.362 min Scan# 613
Delta R.T. 0.051 min
Lab File: VU048779.D
Acq: 01 Jun 2022 14:10




Instrument :
MSVOA_U
ClientSampleId :
HW-1DL


Tgt Ion: 53 Resp: 4278
Ion Ratio Lower Upper
53 100
52 16.9 66.3 99.5#
51 75.4 28.6 42.8#

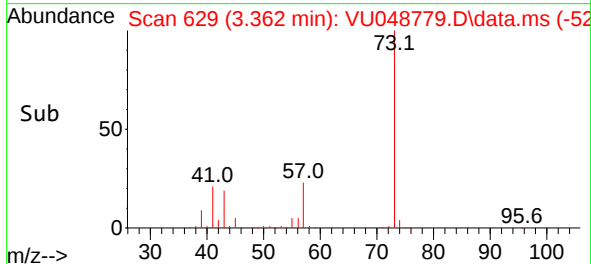

#16
Acetone
Concen: 1.768 ug/l
RT: 2.633 min Scan# 402
Delta R.T. 0.006 min
Lab File: VU048779.D
Acq: 01 Jun 2022 14:10

Tgt Ion: 43 Resp: 3595
Ion Ratio Lower Upper
43 100
58 37.3 26.3 39.5

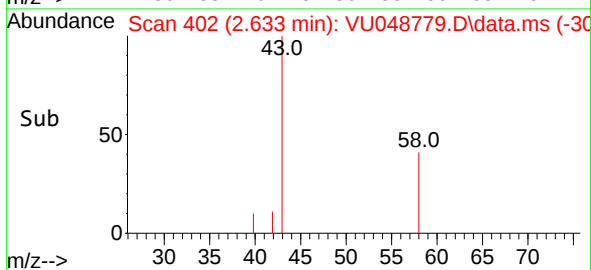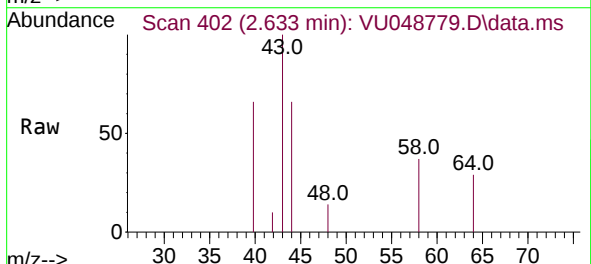



#17

Carbon Disulfide

Concen: 0.284 ug/l

RT: 2.793 min Scan# 4

Delta R.T. 0.000 min

Lab File: VU048779.D

Acq: 01 Jun 2022 14:10

Instrument :

MSVOA_U

ClientSampleId :





HW-1DL

Tgt Ion: 76 Resp: 2241

Ion Ratio Lower Upper

76 100

78 10.5 7.3 10.9

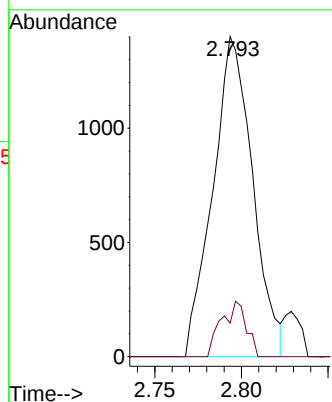

#19

Methyl tert-butyl Ether

Concen: 36.735 ug/l

RT: 3.362 min Scan# 629

Delta R.T. -0.000 min

Lab File: VU048779.D




Acq: 01 Jun 2022 14:10


Tgt Ion: 73 Resp: 376851

Ion Ratio Lower Upper

73 100

57 23.1 17.1 25.7


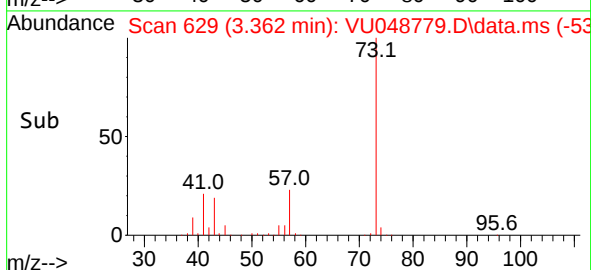






#20
Methylene Chloride
Concen: 0.368 ug/l
RT: 3.047 min Scan# 511
Delta R.T. -0.000 min
Lab File: VU048779.D
Acq: 01 Jun 2022 14:10




Instrument :
MSVOA_U
ClientSampleId :
HW-1DL


Tgt Ion: 84	Resp: 1272
Ion Ratio	Lower Upper
84 100	
49 115.6	97.0 145.4
51 39.4	29.8 44.8
86 77.4	50.9 76.3#

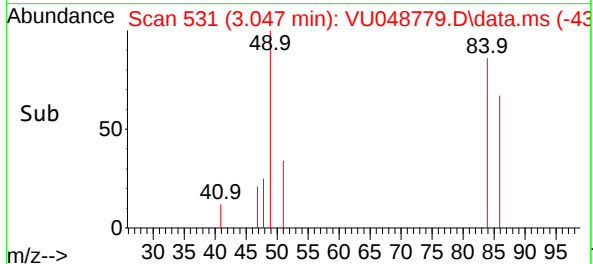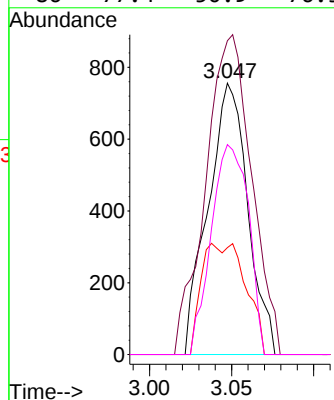

#29
Tetrahydrofuran
Concen: 0.326 ug/l
RT: 5.067 min Scan# 1159
Delta R.T. 0.016 min
Lab File: VU048779.D
Acq: 01 Jun 2022 14:10

Tgt Ion: 42	Resp: 599
Ion Ratio	Lower Upper
42 100	
72 29.0	37.6 56.4#
71 11.4	35.0 52.4#

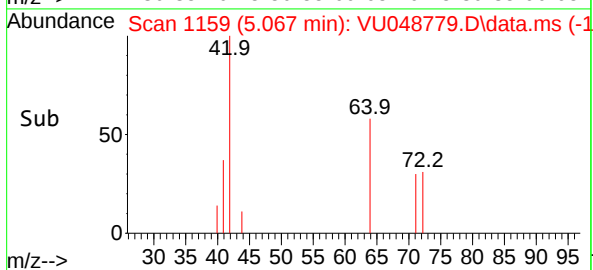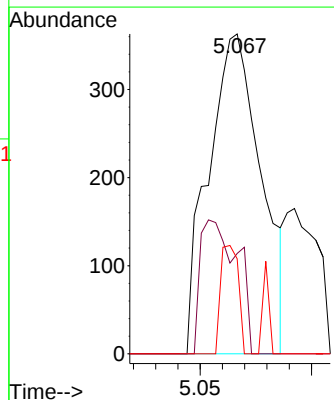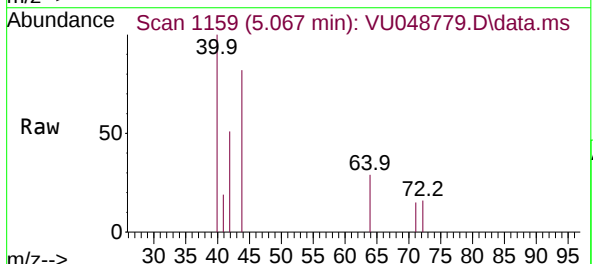



#31

Cyclohexane

Concen: 1.152 ug/l

RT: 5.375 min Scan# 1

Delta R.T. -0.016 min

Lab File: VU048779.D

Acq: 01 Jun 2022 14:10

Instrument :

MSVOA_U

ClientSampleId :

HW-1DL





Tgt Ion: 56 Resp: 5792

Ion Ratio Lower Upper

56 100

69 181.2 25.6 38.4#

84 130.0 66.2 99.4#

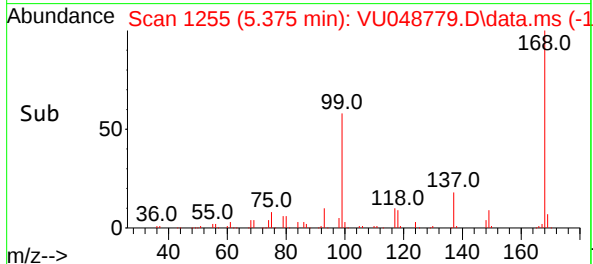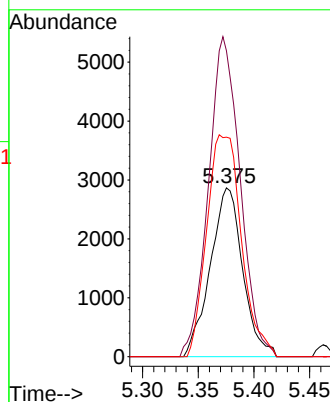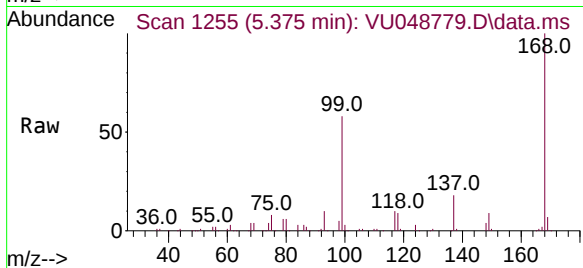

#33

1,2-Dichloroethane-d4

Concen: 47.731 ug/l

RT: 5.703 min Scan# 1357

Delta R.T. 0.003 min

Lab File: VU048779.D




Acq: 01 Jun 2022 14:10


Tgt Ion: 65 Resp: 190420

Ion Ratio Lower Upper

65 100

67 52.9 0.0 103.0

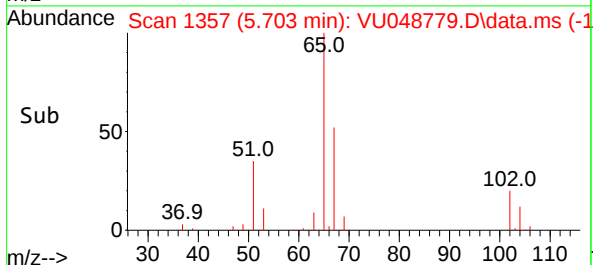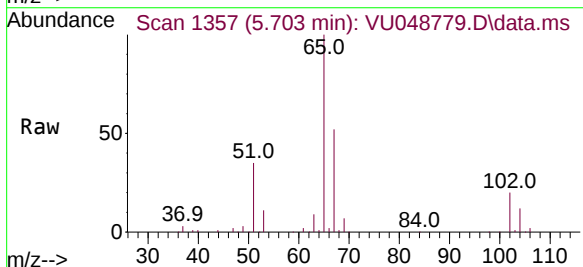



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.250 min Scan# 11

Delta R.T. -0.000 min

Lab File: VU048779.D

Acq: 01 Jun 2022 14:10

Instrument :

MSVOA_U

ClientSampleId :

HW-1DL





Tgt Ion:114 Resp: 445880

Ion Ratio Lower Upper

114 100

63 21.3 0.0 42.6

88 16.1 0.0 32.2

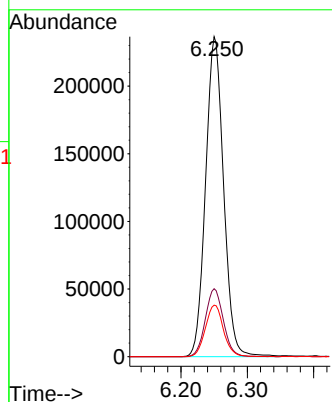

#35

Dibromofluoromethane

Concen: 47.254 ug/l

RT: 5.292 min Scan# 1229

Delta R.T. -0.000 min

Lab File: VU048779.D

Acq: 01 Jun 2022 14:10




Tgt Ion:113 Resp: 150314


Ion Ratio Lower Upper

113 100

111 102.7 80.7 121.1

192 18.6 15.9 23.9

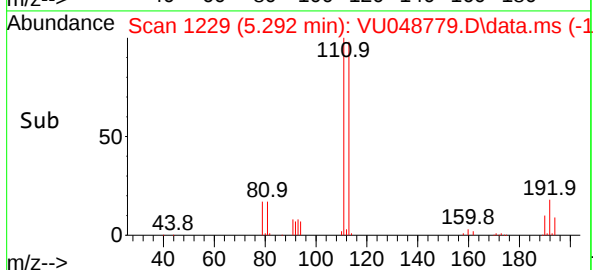



#36

1,1-Dichloropropene

Concen: 4.694 ug/l

RT: 5.372 min Scan# 11

Delta R.T. -0.154 min

Lab File: VU048779.D

Acq: 01 Jun 2022 14:10

Instrument :

MSVOA_U

ClientSampleId :

HW-1DL





Tgt Ion: 75 Resp: 21793

Ion Ratio Lower Upper

75 100

110 7.9 17.4 52.3#

77 0.0 24.8 37.2#

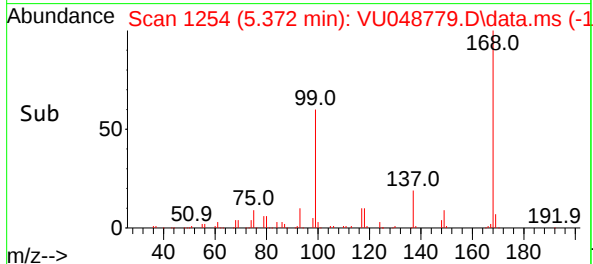

#38

Carbon Tetrachloride

Concen: 5.147 ug/l

RT: 5.375 min Scan# 1255

Delta R.T. -0.151 min

Lab File: VU048779.D

Acq: 01 Jun 2022 14:10




Tgt Ion: 117 Resp: 27413


Ion Ratio Lower Upper

117 100

119 6.4 75.4 113.2#

121 0.0 24.6 36.8#

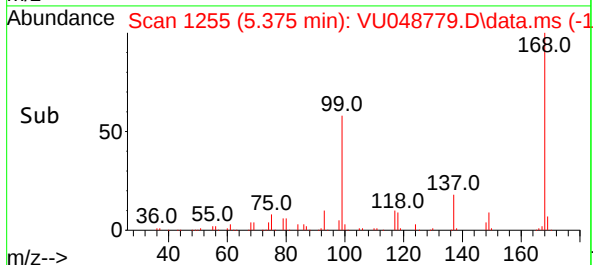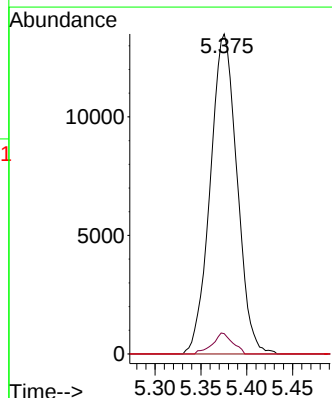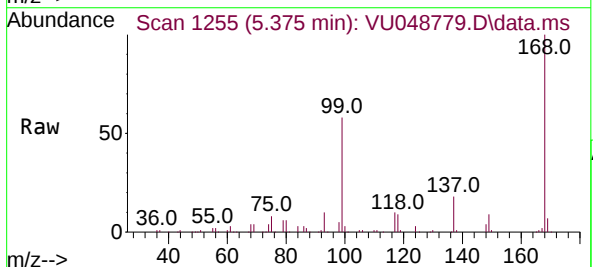



#43

Isopropyl Acetate

Concen: 1.952 ug/l

RT: 5.825 min Scan# 1

Delta R.T. -0.084 min

Lab File: VU048779.D

Acq: 01 Jun 2022 14:10

Instrument :

MSVOA_U

ClientSampleId :

HW-1DL





Tgt Ion: 43 Resp: 16631

Ion Ratio Lower Upper

43 100

61 0.0 16.7 25.1#

87 0.0 10.9 16.3#

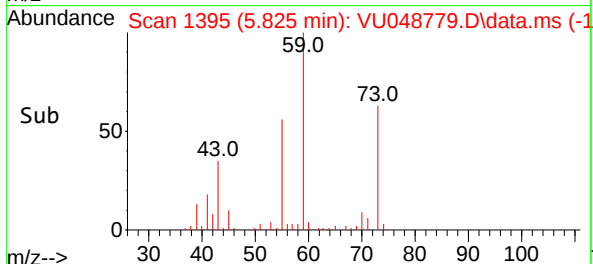

#49

1,4-Dioxane

Concen: 0.257 ug/l

RT: 6.983 min Scan# 1755

Delta R.T. 0.010 min

Lab File: VU048779.D

Acq: 01 Jun 2022 14:10




Tgt Ion: 88 Resp: 22


Ion Ratio Lower Upper

88 100

43 200.0 24.6 36.8#

58 0.0 54.7 82.1#

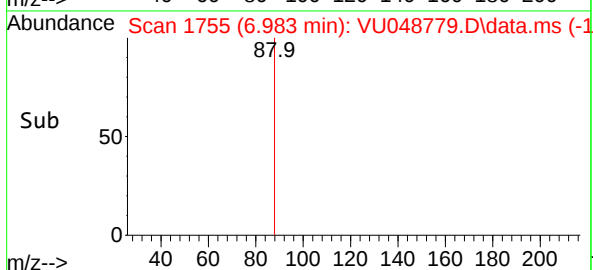



#50

Toluene-d8

Concen: 47.218 ug/l

RT: 7.899 min Scan# 2040

Delta R.T. -0.000 min

Lab File: VU048779.D

Acq: 01 Jun 2022 14:10

Instrument :

MSVOA_U

ClientSampleId :





HW-1DL

Tgt Ion: 98 Resp: 538418

Ion Ratio Lower Upper

98 100

100 64.9 52.2 78.4

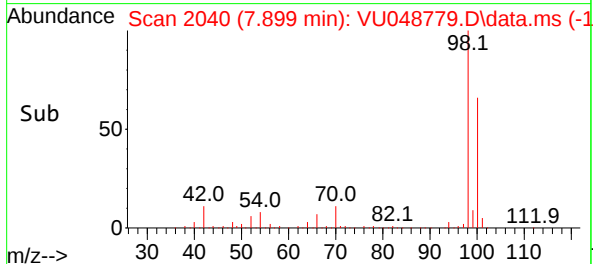

#51

4-Methyl-2-Pentanone

Concen: 0.448 ug/l

RT: 7.793 min Scan# 2007

Delta R.T. 0.003 min

Lab File: VU048779.D




Acq: 01 Jun 2022 14:10


Tgt Ion: 43 Resp: 2477

Ion Ratio Lower Upper

43 100

58 30.1 32.7 49.1#


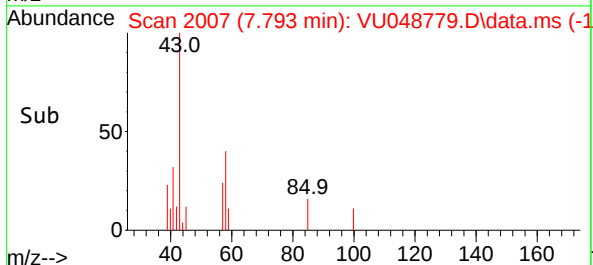
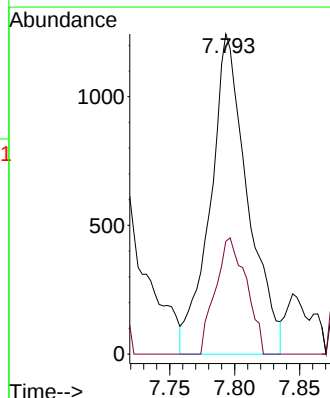
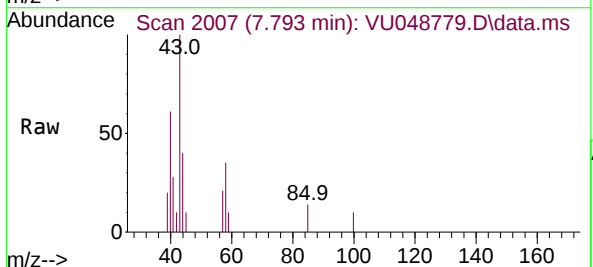




#56
Ethyl methacrylate
Concen: 2.639 ug/l
RT: 8.330 min Scan# 2175
Delta R.T. -0.003 min
Lab File: VU048779.D
Acq: 01 Jun 2022 14:10




Instrument :
MSVOA_U
ClientSampleId :
HW-1DL


Tgt Ion: 69 Resp: 156
Ion Ratio Lower Upper
69 100
41 235.3 50.6 76.0#
39 0.0 26.6 40.0#

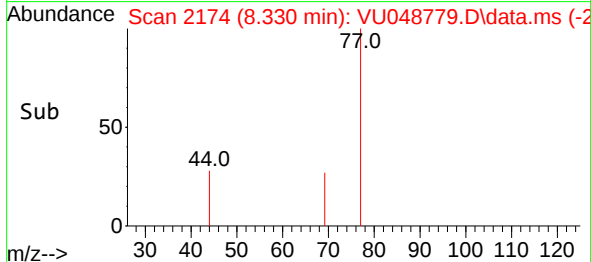

#59
2-Hexanone
Concen: 0.610 ug/l
RT: 8.690 min Scan# 2286
Delta R.T. 0.006 min
Lab File: VU048779.D
Acq: 01 Jun 2022 14:10

Tgt Ion: 43 Resp: 2770
Ion Ratio Lower Upper
43 100
58 42.7 28.2 84.6


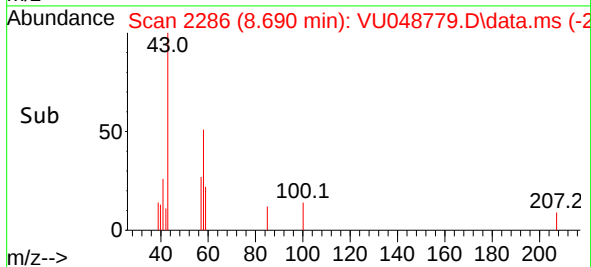

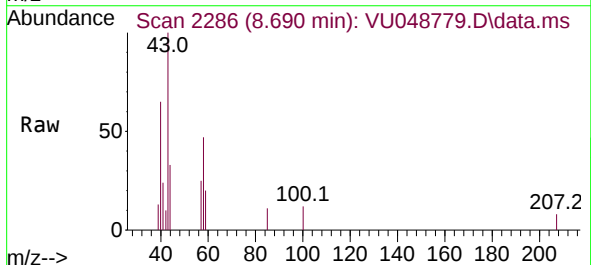




#62
4-Bromofluorobenzene
Concen: 47.516 ug/l
RT: 10.632 min Scan# 21
Delta R.T. 0.000 min
Lab File: VU048779.D
Acq: 01 Jun 2022 14:10




Instrument :
MSVOA_U
ClientSampleId :
HW-1DL


Tgt Ion: 95 Resp: 204910
Ion Ratio Lower Upper
95 100
174 77.8 0.0 159.4
176 75.8 0.0 152.4

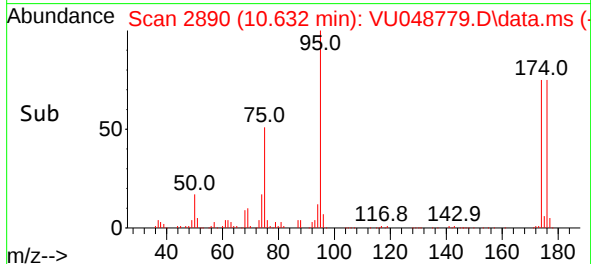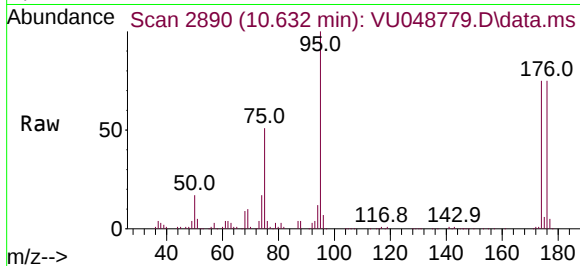

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 9.420 min Scan# 2513
Delta R.T. 0.003 min
Lab File: VU048779.D
Acq: 01 Jun 2022 14:10

Tgt Ion: 117 Resp: 423711
Ion Ratio Lower Upper
117 100
82 55.6 45.3 67.9
119 32.1 25.4 38.2


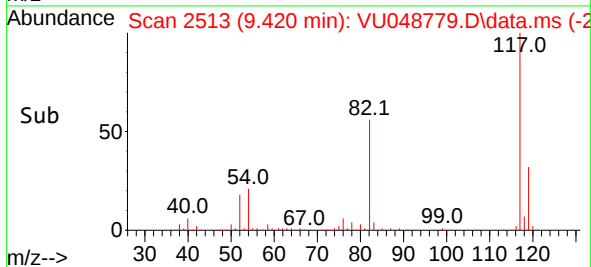

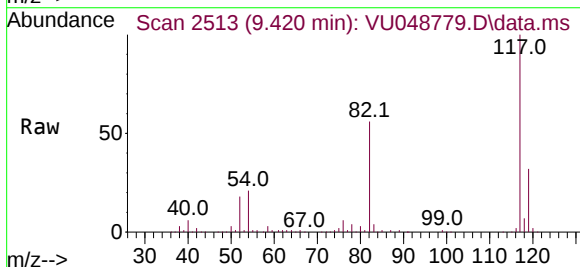


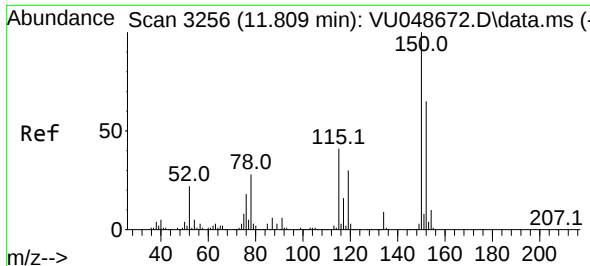

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 11.812 min Scan# 31
Delta R.T. 0.003 min
Lab File: VU048779.D
Acq: 01 Jun 2022 14:10




Instrument :
MSVOA_U
ClientSampleId :
HW-1DL


Tgt Ion:152 Resp: 218268
Ion Ratio Lower Upper
152 100
115 60.5 41.8 125.4
150 157.1 0.0 341.0

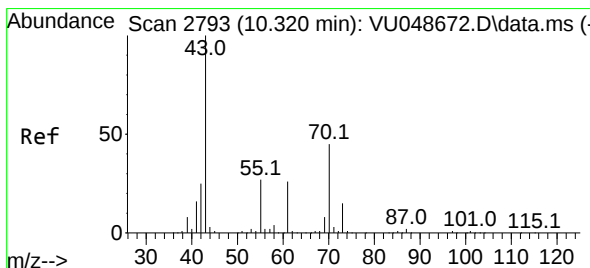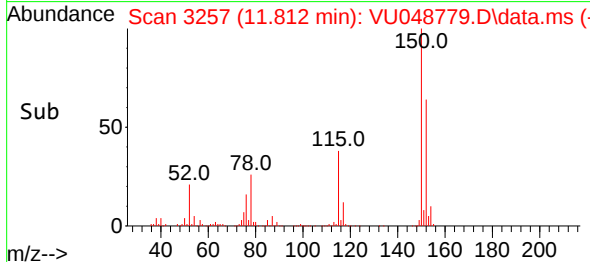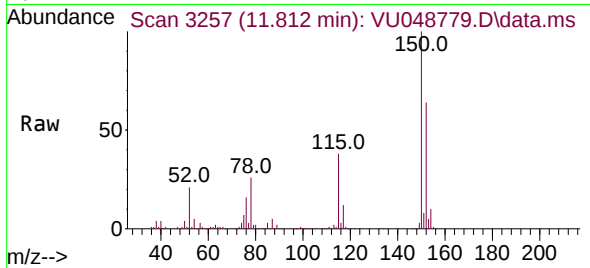

#74
N-amy1 acetate
Concen: 2.546 ug/l
RT: 10.327 min Scan# 2795
Delta R.T. 0.007 min
Lab File: VU048779.D
Acq: 01 Jun 2022 14:10

Tgt Ion: 43 Resp: 592
Ion Ratio Lower Upper
43 100
70 36.1 35.8 53.6
55 16.9 21.1 31.7#
61 0.0 20.2 30.4#


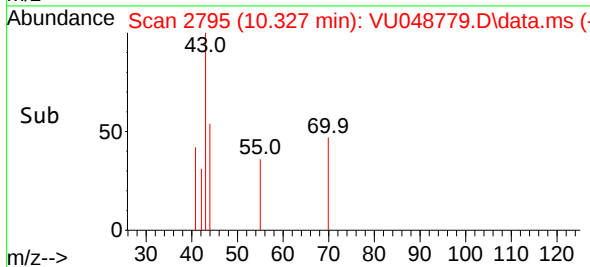

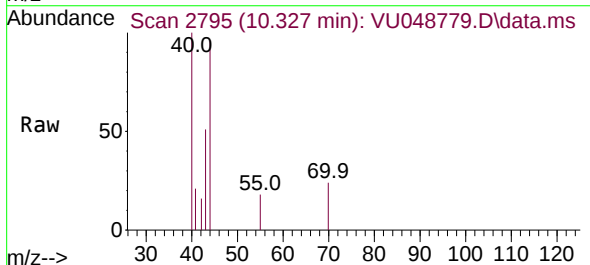




#76
1,2,3-Trichloropropane
Concen: 14.592 ug/l
RT: 10.632 min Scan# 2890
Delta R.T. -0.190 min
Lab File: VU048779.D
Acq: 01 Jun 2022 14:10




Instrument :
MSVOA_U
ClientSampleId :
HW-1DL


Tgt Ion: 75 Resp: 102690
Ion Ratio Lower Upper
75 100
77 1.3 14.8 44.3#

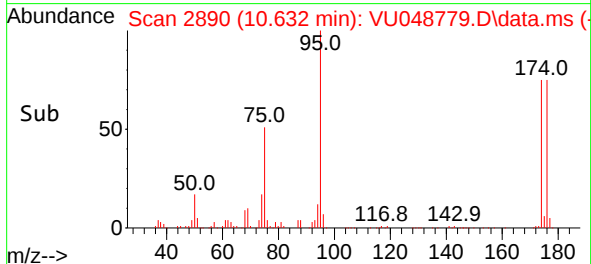

#81
trans-1,4-Dichloro-2-butene
Concen: 52.981 ug/l
RT: 10.632 min Scan# 2890
Delta R.T. 0.087 min
Lab File: VU048779.D
Acq: 01 Jun 2022 14:10

Tgt Ion: 75 Resp: 102690
Ion Ratio Lower Upper
75 100
53 0.1 72.5 108.7#
89 0.0 37.0 55.4#



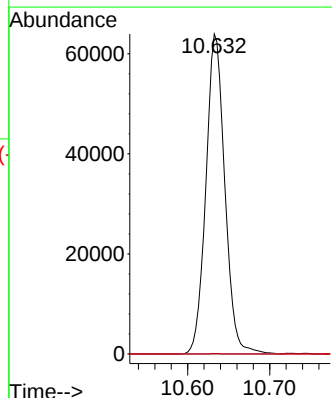
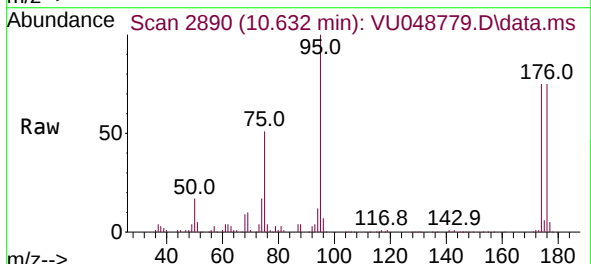


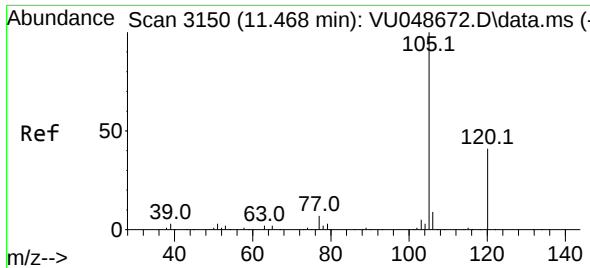

#84
1,2,4-Trimethylbenzene
Concen: 1.355 ug/l
RT: 11.472 min Scan# 3151
Delta R.T. 0.004 min
Lab File: VU048779.D
Acq: 01 Jun 2022 14:10




Instrument :
MSVOA_U
ClientSampleId :
HW-1DL


Tgt Ion:105 Resp: 2267
Ion Ratio Lower Upper
105 100
120 35.5 22.5 67.5

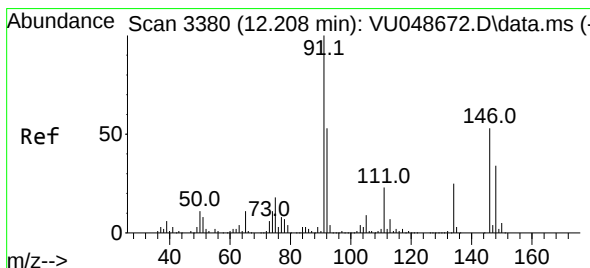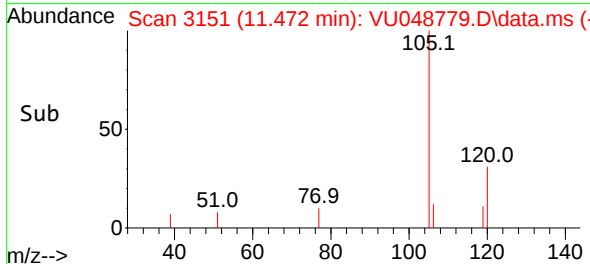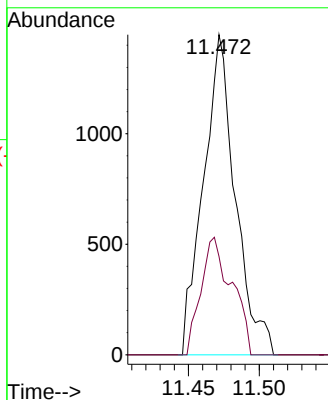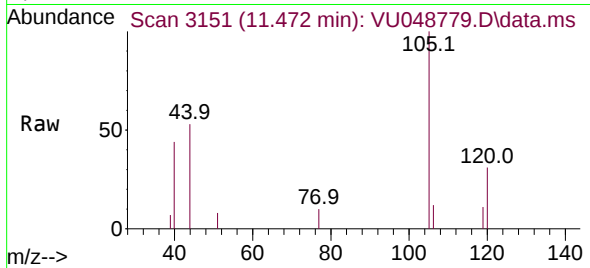

#89
n-Butylbenzene
Concen: 2.292 ug/l
RT: 12.214 min Scan# 3382
Delta R.T. 0.006 min
Lab File: VU048779.D
Acq: 01 Jun 2022 14:10

Tgt Ion: 91 Resp: 1407
Ion Ratio Lower Upper
91 100
92 47.3 25.9 77.8
134 0.0 12.5 37.5#


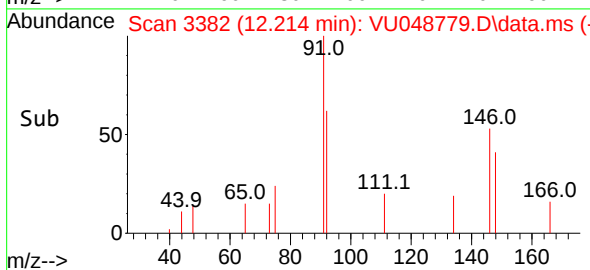
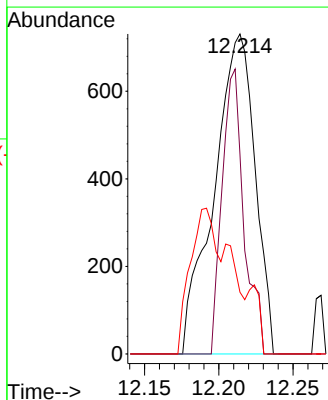
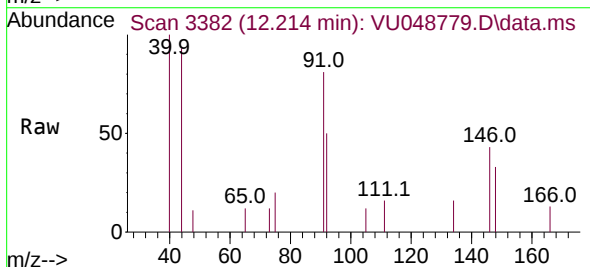




#90
Hexachloroethane
Concen: 0.471 ug/l
RT: 12.613 min Scan# 3506
Delta R.T. 0.138 min
Lab File: VU048779.D
Acq: 01 Jun 2022 14:10




Instrument :
MSVOA_U
ClientSampleId :
HW-1DL


Tgt Ion:117 Resp: 1215
Ion Ratio Lower Upper
117 100
201 0.0 39.6 119.0#

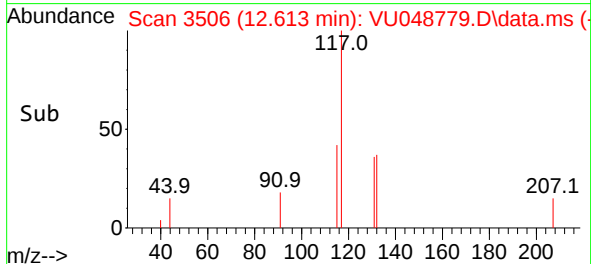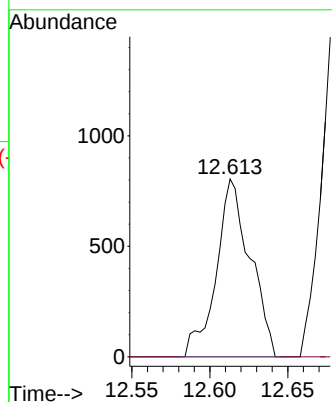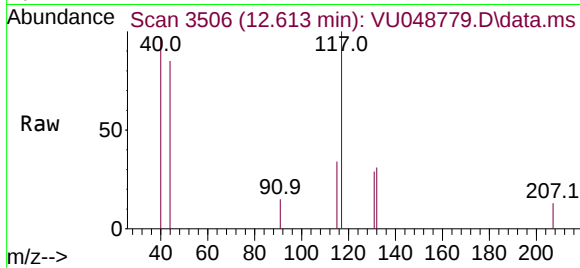

#93
1,2,4-Trichlorobenzene
Concen: 0.229 ug/l
RT: 13.844 min Scan# 3889
Delta R.T. 0.006 min
Lab File: VU048779.D
Acq: 01 Jun 2022 14:10

Tgt Ion:180 Resp: 1126
Ion Ratio Lower Upper
180 100
182 75.0 48.3 144.9
145 35.6 15.6 46.7


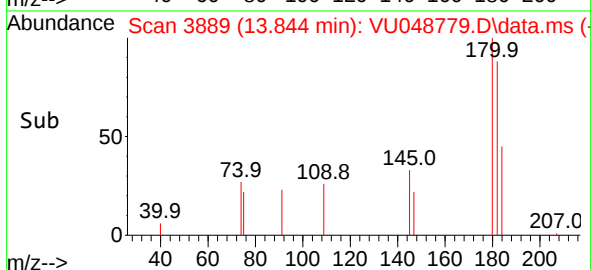

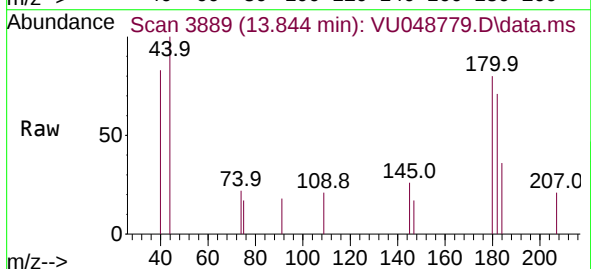


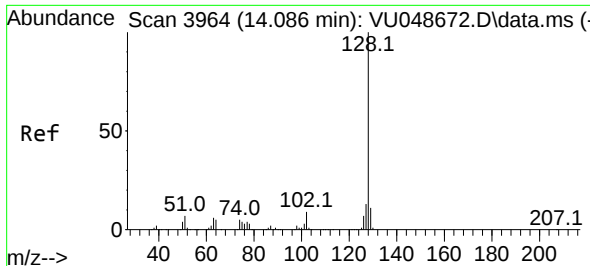

#95
Naphthalene
Concen: 10.113 ug/l
RT: 14.089 min Scan# 3964
Delta R.T. 0.003 min
Lab File: VU048779.D
Acq: 01 Jun 2022 14:10

Instrument :
MSVOA_U
ClientSampleId :
HW-1DL

Tgt Ion:128 Resp: 137184
Ion Ratio Lower Upper
128 100
127 13.6 10.2 15.4
129 10.7 8.7 13.1

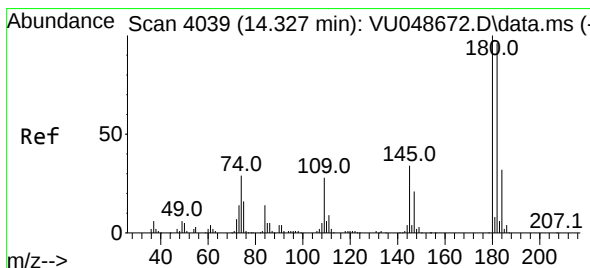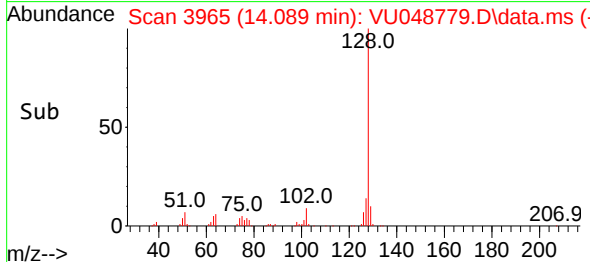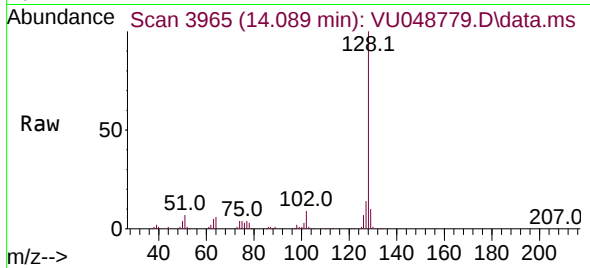

#96
1,2,3-Trichlorobenzene
Concen: 0.215 ug/l
RT: 14.333 min Scan# 4041
Delta R.T. 0.006 min
Lab File: VU048779.D
Acq: 01 Jun 2022 14:10

Tgt Ion:180 Resp: 1046
Ion Ratio Lower Upper
180 100
182 103.0 47.4 142.2
145 51.6 16.6 49.8#

