

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060122\
 Data File : VU048785.D
 Acq On : 01 Jun 2022 17:19
 Operator : SY/MD
 Sample : VIBLK
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U052622W.M
 Title : SW846 8260

Signal : TIC: VU048785.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.485	34	45	56	rBV	23516	63817	4.42%	0.743%
2	2.755	430	440	456	rBV2	13358	26012	1.80%	0.303%
3	5.292	1212	1229	1242	rBV	234413	505206	34.95%	5.878%
4	5.375	1242	1255	1274	rVB	384964	801883	55.48%	9.330%
5	5.703	1338	1357	1378	rBV2	262644	542393	37.53%	6.311%
6	6.250	1513	1527	1547	rBV	552458	1050692	72.70%	12.225%
7	7.899	2025	2040	2055	rBV	831683	1445323	100.00%	16.817%
8	7.970	2057	2062	2074	rVB2	12728	21608	1.50%	0.251%
9	8.472	2205	2218	2232	rBV2	17057	30027	2.08%	0.349%
10	9.417	2495	2512	2535	rBV	752909	1262982	87.38%	14.695%
11	9.693	2585	2598	2607	rBV4	17345	30286	2.10%	0.352%
12	9.745	2607	2614	2623	rVB3	13807	20186	1.40%	0.235%
13	10.632	2875	2890	2916	rBV	628241	1032574	71.44%	12.015%
14	10.896	2960	2972	2985	rBV2	23083	40129	2.78%	0.467%
15	11.115	3026	3040	3054	rVB4	24685	43203	2.99%	0.503%
16	11.472	3143	3151	3168	rVB3	14232	22807	1.58%	0.265%
17	11.812	3243	3257	3273	rBV	826995	1341781	92.84%	15.612%
18	12.327	3406	3417	3428	rVB3	23823	33641	2.33%	0.391%
19	13.436	3750	3762	3775	rBV4	17315	33670	2.33%	0.392%
20	14.089	3956	3965	3977	rBV	38222	63178	4.37%	0.735%
21	15.224	4307	4318	4334	rBV	81352	138798	9.60%	1.615%
22	15.410	4366	4376	4389	rBV2	25706	44194	3.06%	0.514%




Sum of corrected areas: 8594390

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060122\
Data File : VU048785.D
Acq On : 01 Jun 2022 17:19
Operator : SY/MD
Sample : VIBLK
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U052622W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

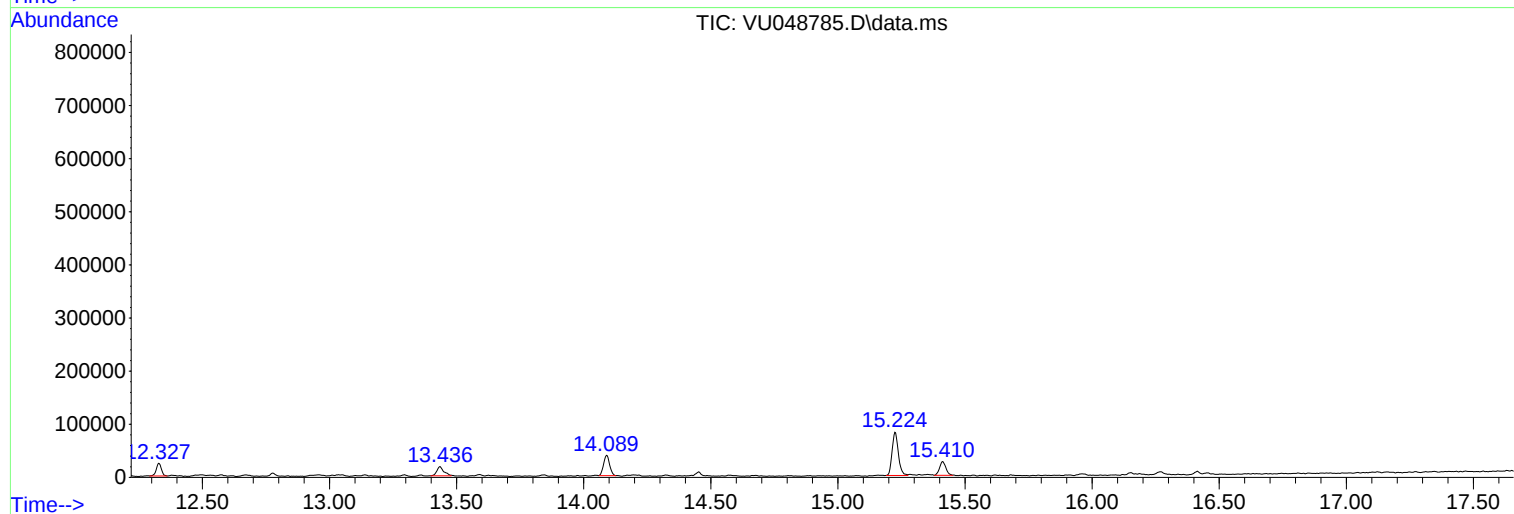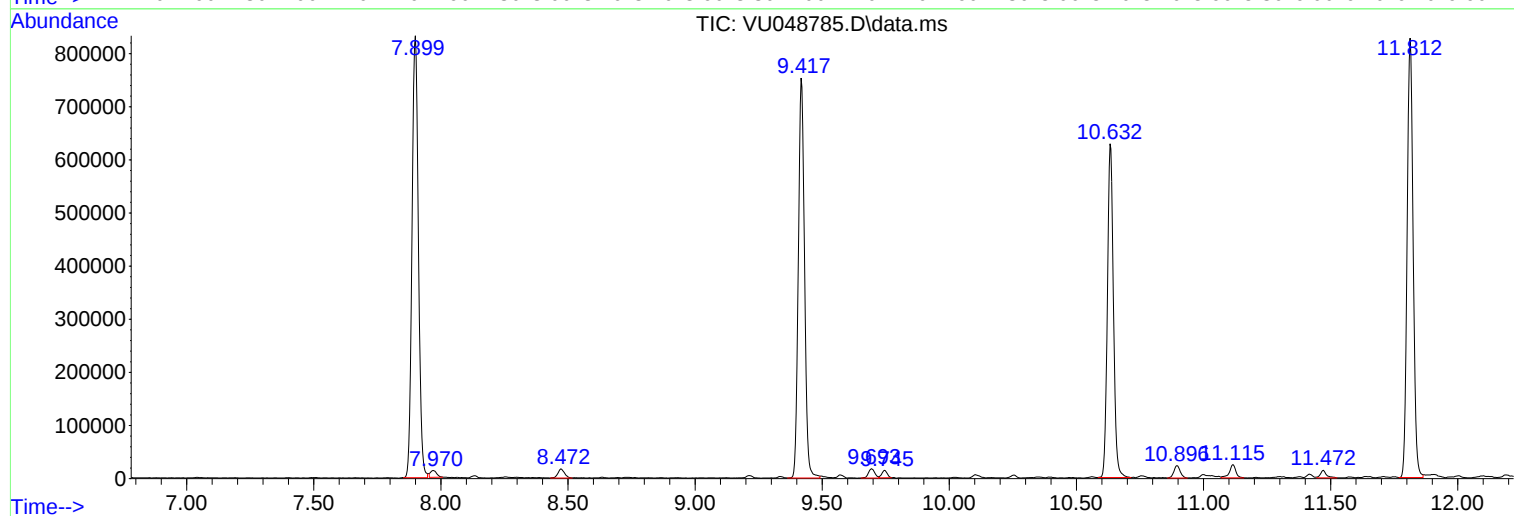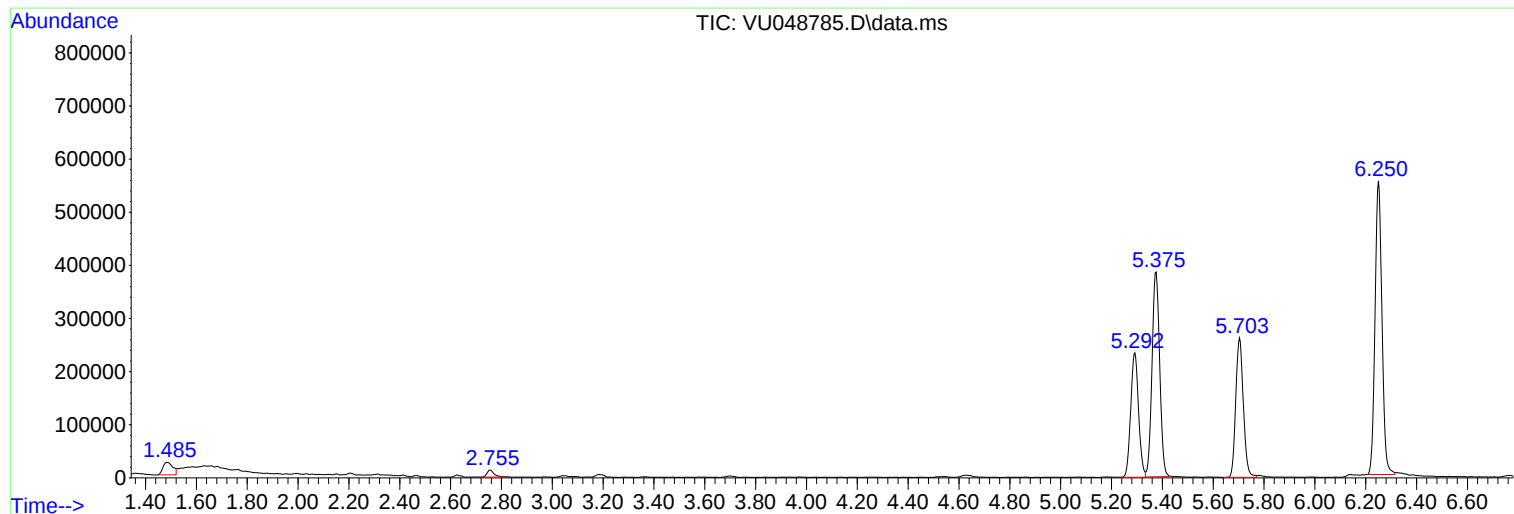

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060122\
Data File : VU048785.D
Acq On : 01 Jun 2022 17:19
Operator : SY/MD
Sample : VIBLK
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U052622W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 1H-Indene, 1-ethylidene- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
15.224	5.17 ug/l	138798	1,4-Dichlorobenzene-d4	11.812

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Naphthalene, 2-methyl-	142	C11H10	000091-57-6	97
2			Naphthalene, 1-methyl-	142	C11H10	000090-12-0	96
3			1H-Indene, 1-ethylidene-	142	C11H10	002471-83-2	91
4			1,4-Methanonaphthalene, 1,4-dihy...	142	C11H10	004453-90-1	91
5			Bicyclo[4.4.1]undeca-1,3,5,7,9-p...	142	C11H10	002443-46-1	91

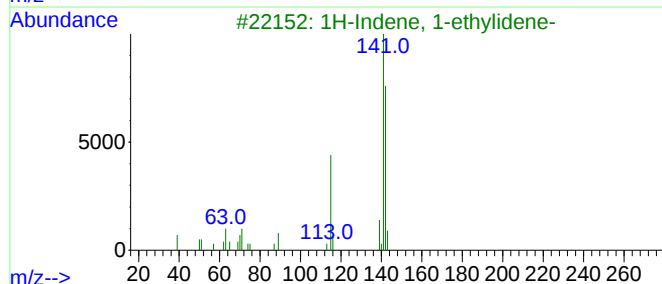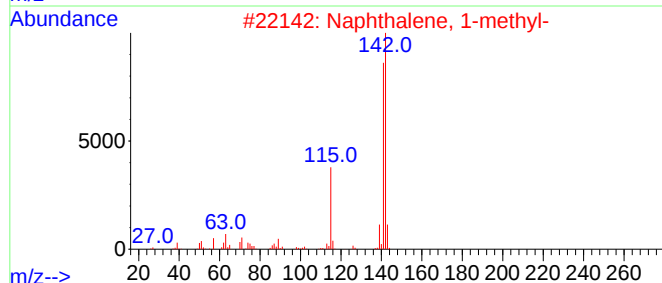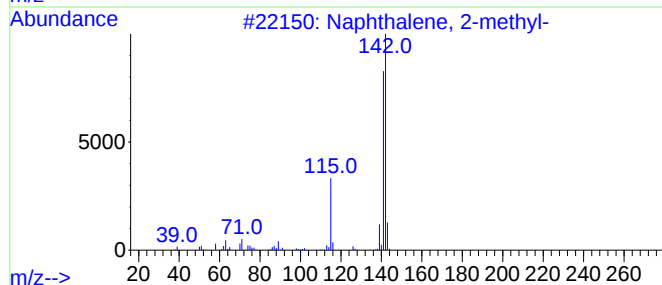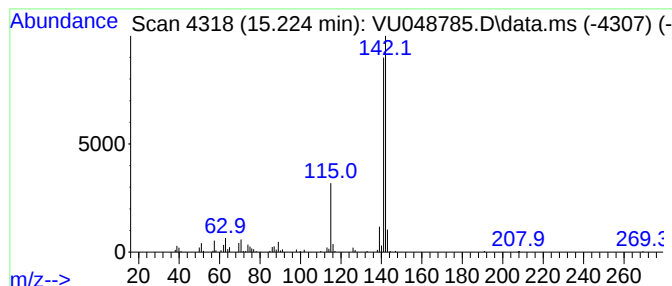

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060122\
Data File : VU048785.D
Acq On : 01 Jun 2022 17:19
Operator : SY/MD
Sample : VIBLK
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U052622W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
1H-Indene, 1-et...	15.224	5.2	ug/l	138798	4	11.812	1341780	50.0