


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060122\
Data File : VU048773.D
Acq On : 01 Jun 2022 09:05
Operator : SY/MD
Sample : BFB
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U052622W.M
Title : SW846 8260
Last Update : Fri May 27 06:42:31 2022

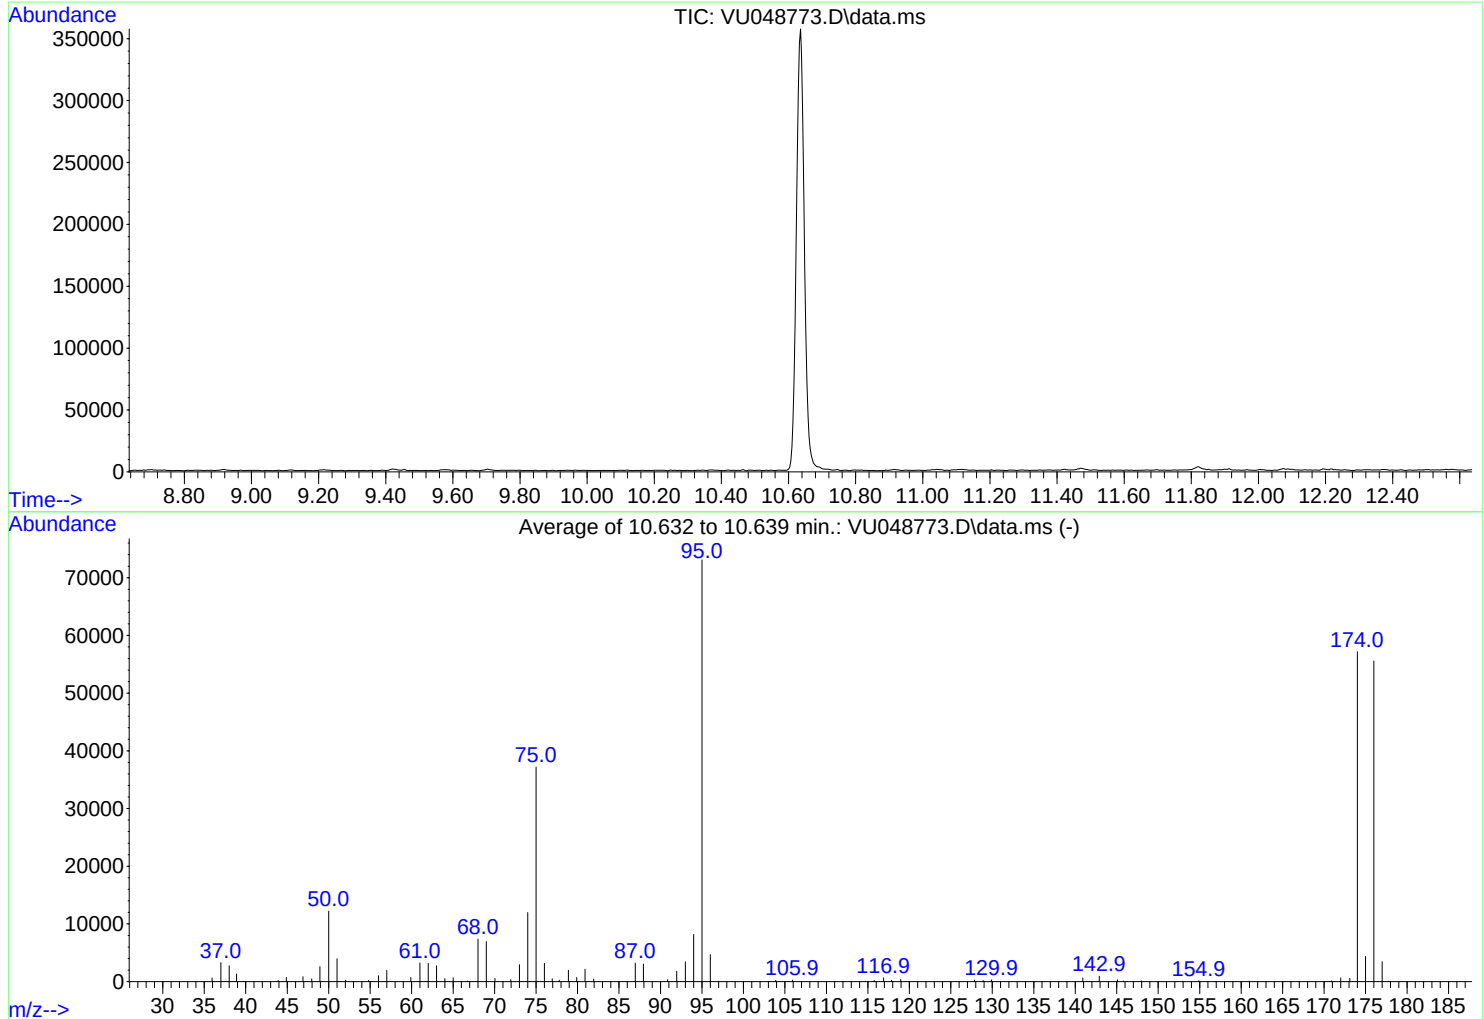

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2876

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.7	12236	PASS
75	95	30	60	50.9	37203	PASS
95	95	100	100	100.0	73101	PASS
96	95	5	9	6.4	4701	PASS
173	174	0.00	2	1.0	597	PASS
174	95	50	100	78.2	57181	PASS
175	174	5	9	7.6	4347	PASS
176	174	95	101	97.2	55576	PASS
177	176	5	9	6.3	3475	PASS