


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060123\
Data File : VU054375.D
Acq On : 01 Jun 2023 12:30
Operator : JC/MD
Sample : BFB191
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB191

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM060123WMA.M
Title : VOC Analysis
Last Update : Fri Jun 02 01:40:39 2023

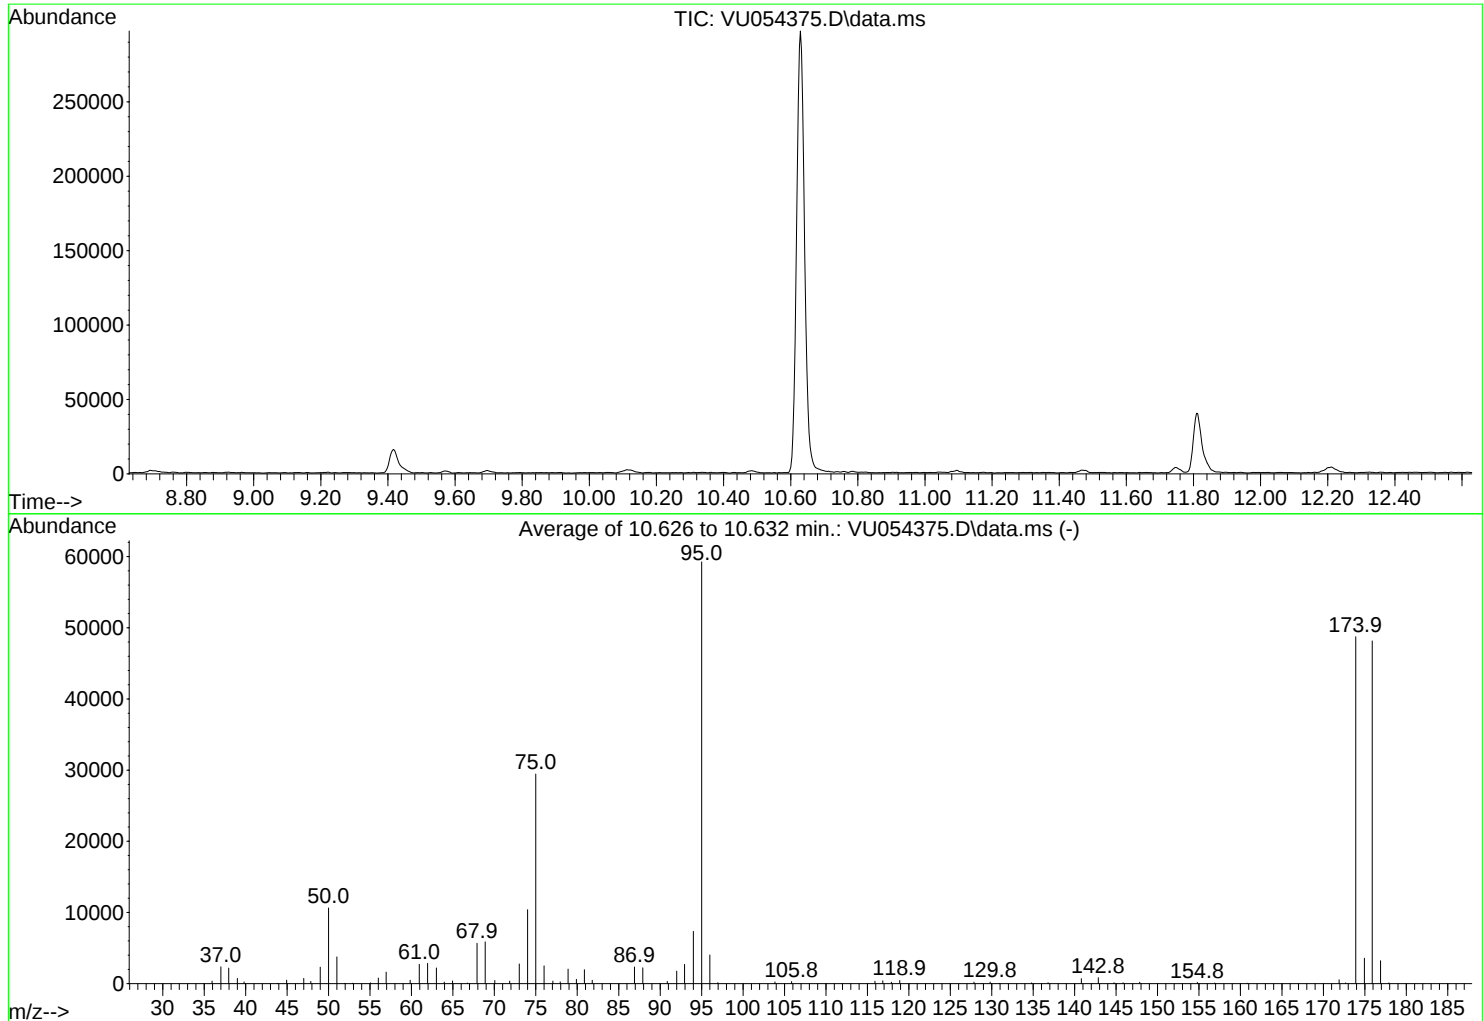

AutoFind: Scans 2888, 2889, 2890; Background Corrected with Scan 2877

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.9	10637	PASS
75	95	30	80	49.7	29456	PASS
95	95	100	100	100.0	59267	PASS
96	95	5	9	6.8	4017	PASS
173	174	0.00	2	0.2	118	PASS
174	95	50	120	82.2	48733	PASS
175	174	5	9	7.3	3577	PASS
176	174	95	101	98.8	48155	PASS
177	176	5	9	6.7	3222	PASS

m/z	Abundance
39.80	268.0
43.90	579.0

Instrument :
MSVOA_U
ClientSampleId :
BFB191

m/z	Abundance
35.90	455.0
37.00	2440.0
37.90	2239.0
39.00	747.0
39.80	553.0
43.90	558.0
45.00	539.0
47.00	794.0
47.90	292.0
49.00	2143.0
50.00	10821.0
51.00	3640.0
52.90	105.0
55.10	123.0
56.00	802.0
57.00	1817.0
59.90	463.0
60.90	2506.0
62.00	2936.0
63.00	2220.0
63.90	222.0
64.90	317.0
66.70	145.0
67.90	5805.0
68.90	5987.0
70.10	460.0
71.90	370.0
73.00	2719.0
74.00	10821.0
75.00	29040.0
76.00	2403.0
77.00	463.0
77.90	214.0
78.90	2059.0
79.90	643.0
80.90	1917.0
81.80	486.0
86.90	2385.0
87.90	2381.0
90.90	295.0
92.00	1761.0
92.90	2594.0
94.00	7250.0
95.00	59280.0
96.00	3765.0
96.90	105.0
103.90	249.0
105.80	310.0
115.90	293.0
116.80	406.0
118.00	202.0
118.90	457.0
127.90	252.0
128.80	126.0
129.80	239.0
134.80	109.0
136.80	135.0
140.80	812.0
142.80	860.0
144.80	147.0
145.90	129.0
147.80	216.0
154.80	200.0
171.90	528.0
172.70	355.0
173.90	47048.0
175.00	3526.0
175.90	46720.0
176.90	3342.0

Instrument :
MSVOA_U
ClientSampleId :
BFB191

m/z	Abundance
36.00	368.0
37.00	2428.0
38.00	2200.0
39.00	764.0
39.80	505.0
43.80	639.0
44.90	525.0
47.00	755.0
47.80	329.0
49.00	2358.0
50.00	10966.0
51.00	3934.0
52.90	115.0
55.00	133.0
56.00	804.0
56.90	1701.0
59.90	478.0
61.00	2801.0
62.00	3008.0
63.00	2270.0
63.90	226.0
65.00	377.0
66.80	104.0
67.90	5785.0
68.90	6044.0
70.00	436.0
71.90	379.0
73.00	2899.0
74.00	10708.0
75.00	30376.0
76.00	2529.0
77.00	341.0
78.00	244.0
78.90	2091.0
79.90	633.0
80.90	2014.0
81.80	511.0
86.90	2374.0
87.90	2242.0
90.80	350.0
92.00	1845.0
92.90	2789.0
94.00	7683.0
95.00	60800.0
96.00	4150.0
97.00	156.0
103.90	246.0
105.90	294.0
115.90	347.0
116.90	417.0
117.90	186.0
118.90	498.0
127.90	216.0
129.80	243.0
134.80	131.0
136.80	149.0
140.80	719.0
142.80	865.0
144.80	142.0
145.90	133.0
147.80	234.0
154.80	182.0
156.90	128.0
160.80	125.0
171.90	561.0
173.90	49936.0
174.90	3636.0
175.90	49560.0
176.90	3272.0
177.90	152.0

Instrument :
MSVOA_U
ClientSampleId :
BFB191

m/z	Abundance
36.00	242.0
37.00	2244.0
38.00	2113.0
39.00	734.0
39.90	474.0
43.80	676.0
44.90	440.0
47.00	659.0
47.80	333.0
49.00	2431.0
50.00	10125.0
51.00	3671.0
51.90	127.0
55.00	119.0
56.00	733.0
56.90	1373.0
59.80	465.0
61.00	2825.0
61.90	2657.0
63.00	2121.0
64.00	264.0
65.00	468.0
67.90	5434.0
68.90	5546.0
70.00	445.0
71.80	356.0
73.00	2695.0
74.00	9619.0
75.00	28952.0
76.00	2543.0
77.10	275.0
78.00	282.0
78.90	1961.0
79.90	552.0
80.80	1947.0
81.80	449.0
86.90	2234.0
87.90	2062.0
90.80	308.0
92.00	1681.0
93.00	2680.0
94.00	7116.0
95.00	57720.0
96.00	4135.0
97.00	161.0
103.80	278.0
105.90	263.0
115.90	374.0
116.90	413.0
117.80	205.0
118.90	428.0
127.80	205.0
129.80	200.0
130.90	107.0
134.80	127.0
136.80	127.0
140.80	571.0
142.10	106.0
142.90	767.0
144.70	134.0
145.80	127.0
147.90	187.0
154.80	132.0
156.90	126.0
160.80	102.0
171.90	535.0
173.90	49216.0
174.90	3570.0
175.90	48184.0
176.90	3051.0
177.90	172.0

Instrument :
MSVOA_U
ClientSampleId :
BFB191