
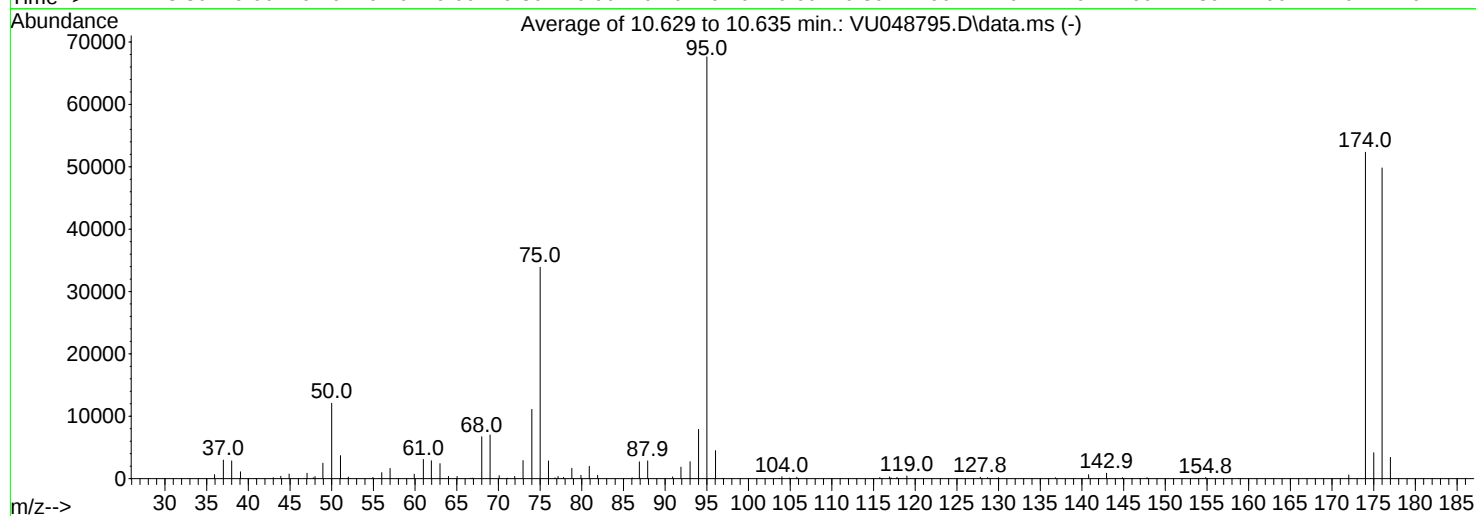


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060222\
 Data File : VU048795.D
 Acq On : 02 Jun 2022 09:30
 Operator : SY/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U052622W.M
 Title : SW846 8260
 Last Update : Fri May 27 06:42:31 2022

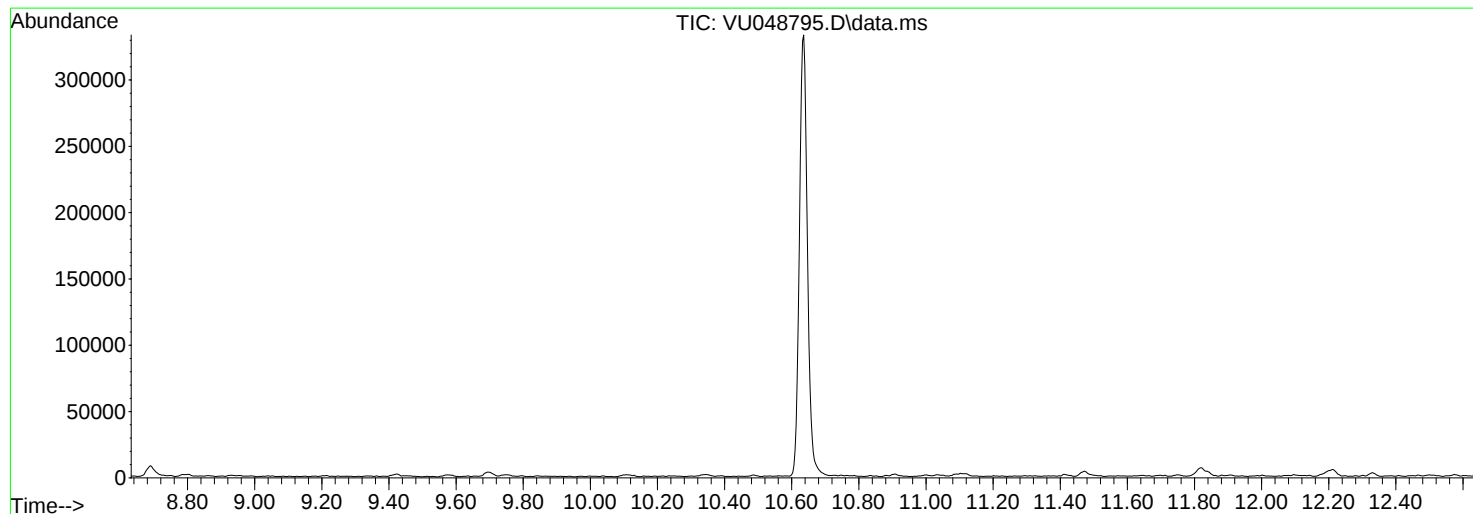

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2877

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.9	12073	PASS
75	95	30	60	50.1	33891	PASS
95	95	100	100	100.0	67624	PASS
96	95	5	9	6.6	4488	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	77.4	52333	PASS
175	174	5	9	8.0	4164	PASS
176	174	95	101	95.2	49813	PASS
177	176	5	9	6.8	3403	PASS