
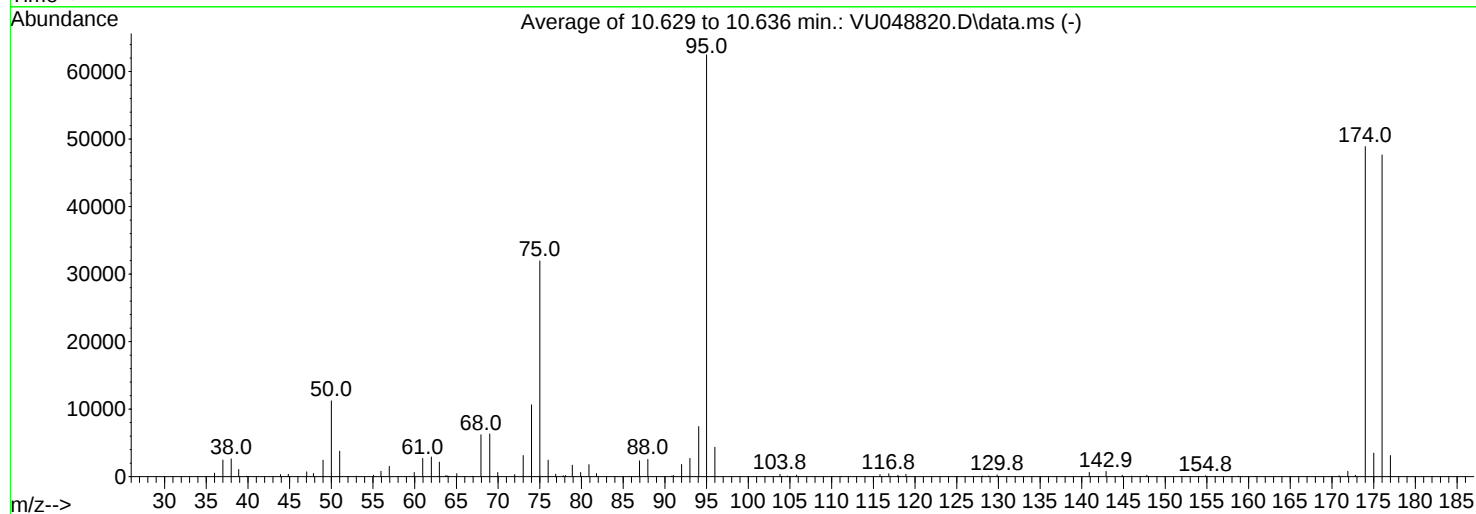


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060222\
Data File : VU048820.D
Acq On : 02 Jun 2022 22:05
Operator : SY/MD
Sample : BFB
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U052622W.M
Title : SW846 8260
Last Update : Fri May 27 06:42:31 2022

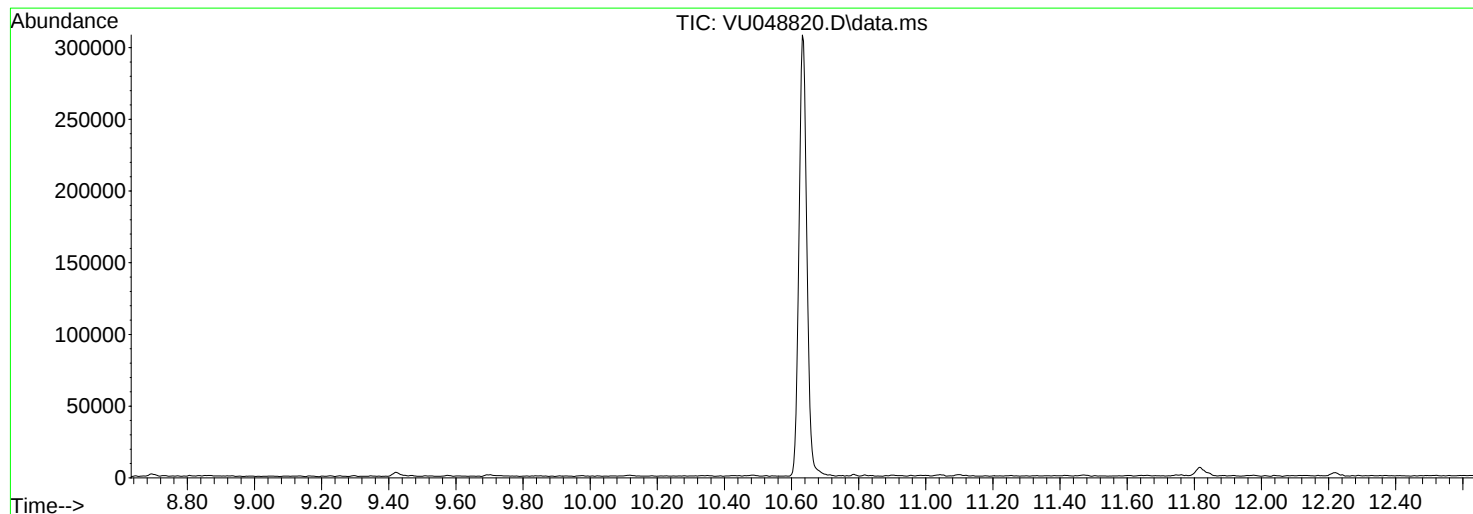

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2876

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.0	11239	PASS
75	95	30	60	51.2	31963	PASS
95	95	100	100	100.0	62480	PASS
96	95	5	9	7.0	4370	PASS
173	174	0.00	2	0.4	188	PASS
174	95	50	100	78.3	48899	PASS
175	174	5	9	7.1	3480	PASS
176	174	95	101	97.5	47653	PASS
177	176	5	9	6.6	3126	PASS