




Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU060319\
Data File : VU032411.D
Acq On : 03 Jun 2019 22:39
Operator : JC/SP
Sample : K3081-14
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GALE2

Manual Integrations
APPROVED

MMDadoda
6/18/2019 1:12:27 AM

Quant Time: Jun 04 09:00:23 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR060319WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Jun 04 08:55:15 2019
Response via : Initial Calibration

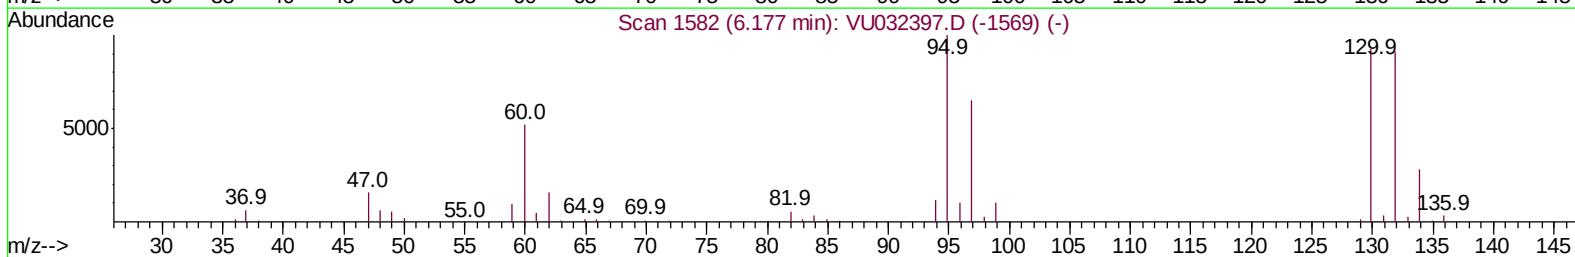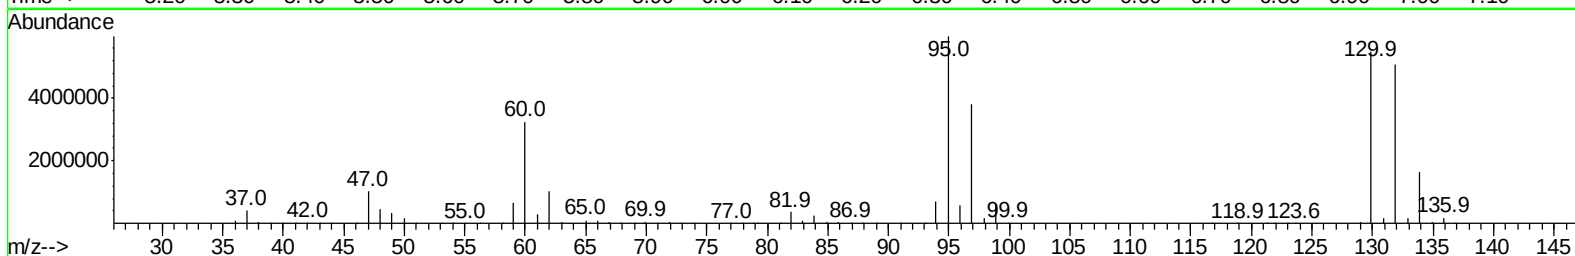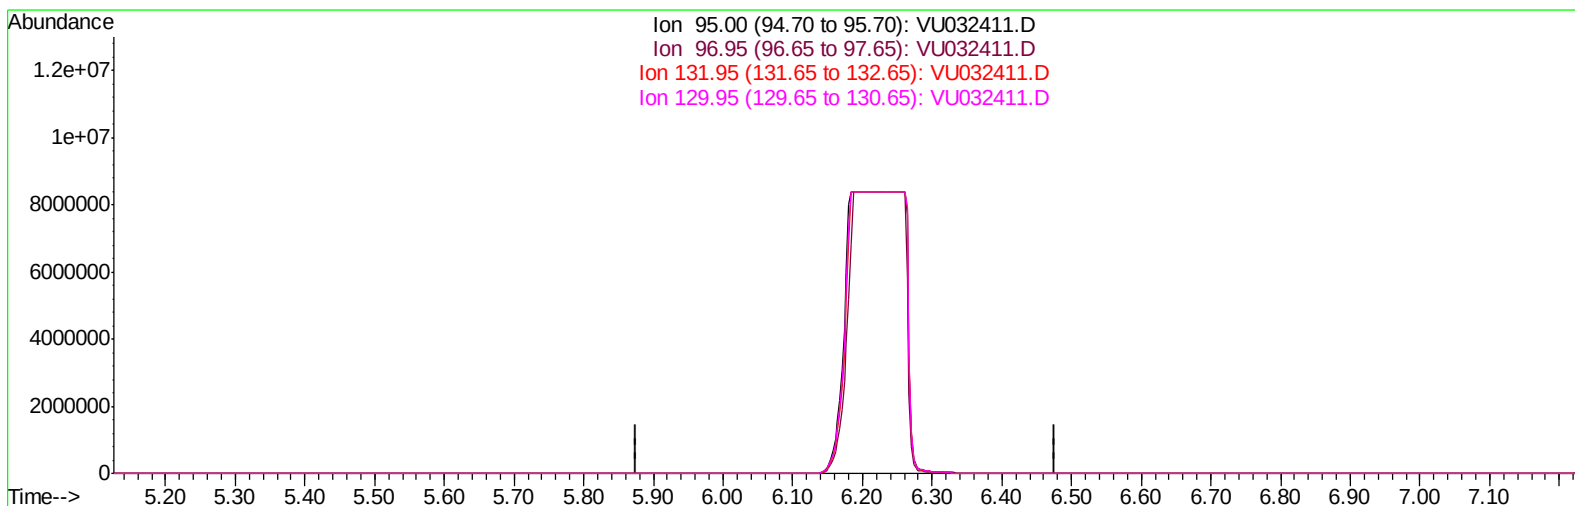

TIC: VU032411.D

(34) Trichloroethene (T)

6.177min (-6.177) 0.00ug/L

response 0

Ion	Exp%	Act%
95.00	100	0.00
96.95	65.40	0.00#
131.95	90.10	0.00#
129.95	94.30	0.00#




Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU060319\
Data File : VU032411.D
Acq On : 03 Jun 2019 22:39
Operator : JC/SP
Sample : K3081-14
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GALE2

Manual Integrations
APPROVED

MMDadoda
6/18/2019 1:12:27 AM

Quant Time: Jun 04 09:00:23 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR060319WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Jun 04 08:55:15 2019
Response via : Initial Calibration

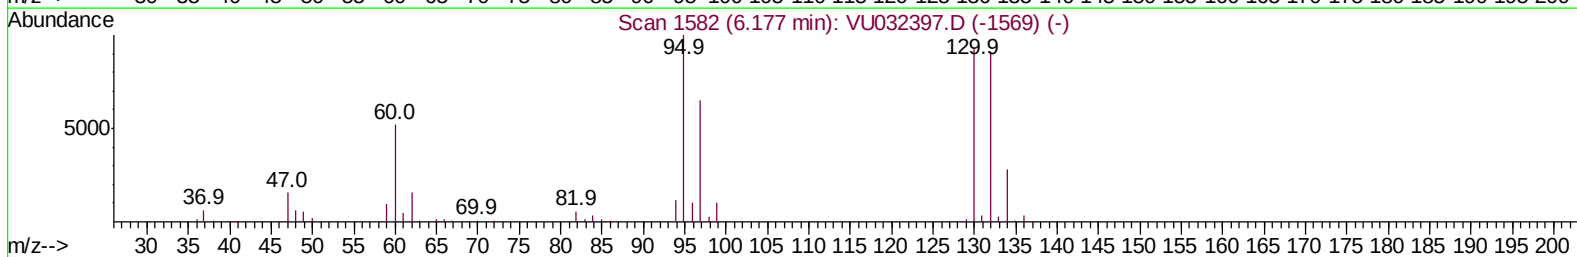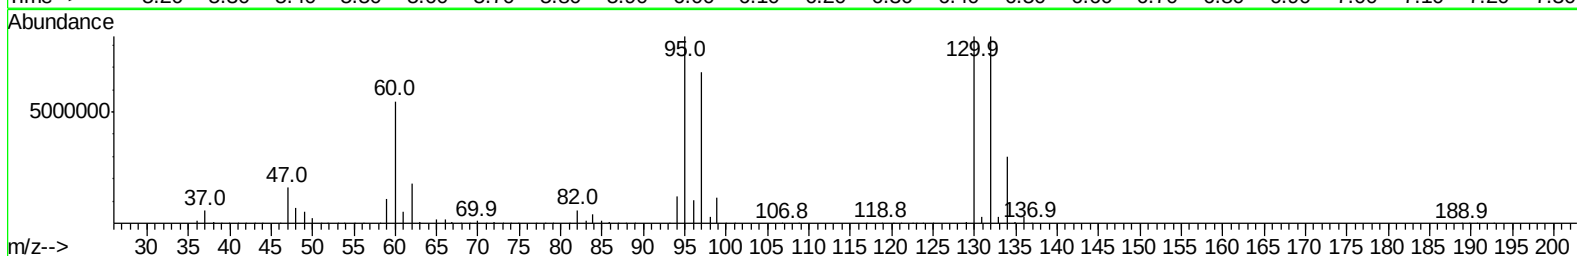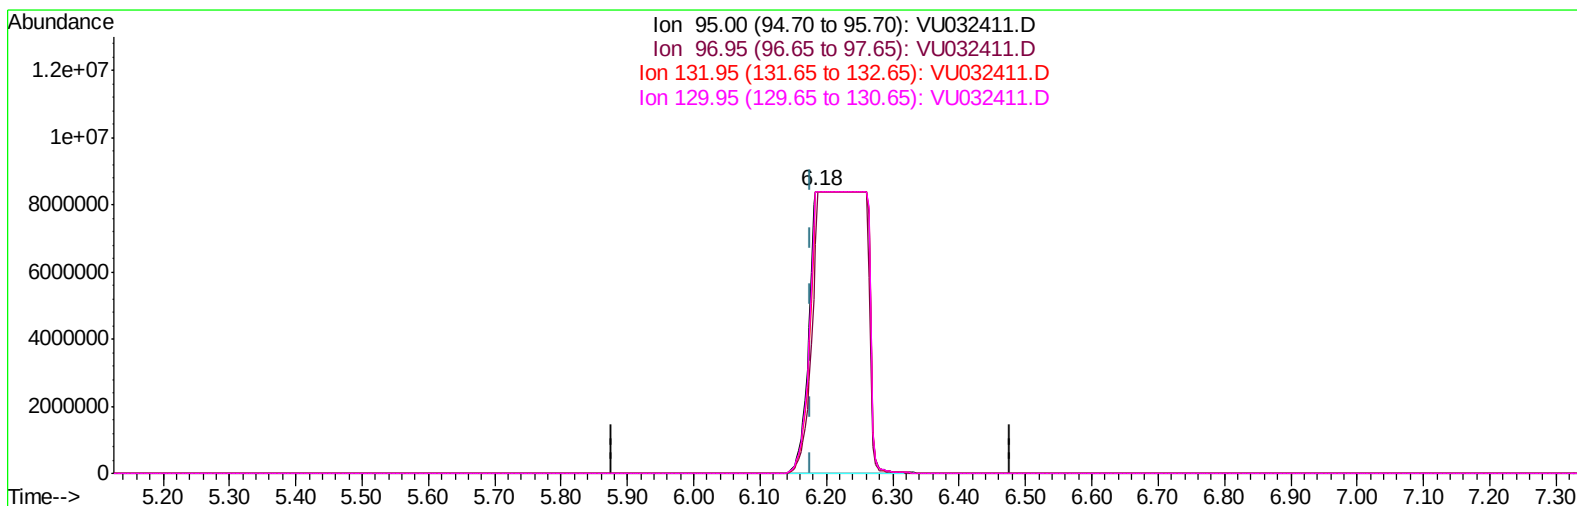

TIC: VU032411.D

(34) Trichloroethene (T)

6.183min (+0.007) 3025.20ug/L m

response 48472064

Ion	Exp%	Act%
95.00	100	100
96.95	65.40	81.18
131.95	90.10	100.00
129.95	94.30	100.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU060319\
Data File : VU032411.D
Acq On : 03 Jun 2019 22:39
Operator : JC/SP
Sample : K3081-14
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GALE2

Manual Integrations
APPROVED

MMDadoda
6/18/2019 1:12:27 AM

Quant Time: Jun 04 09:44:49 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR060319WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Jun 04 08:55:15 2019
Response via : Initial Calibration

