

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU060319\
 Data File : VU032404.D
 Acq On : 03 Jun 2019 19:46
 Operator : JC/SP
 Sample : K3081-17
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GALE5

Quant Time: Jun 04 09:26:34 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR060319WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Jun 04 08:55:15 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	106175	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	99724	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	44923	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	41708	4.19	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	83.80%
7) Chloroethane-d5	1.67	69	33616	3.15	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	63.00%#
11) 1,1-Dichloroethene-d2	2.27	63	66855	2.87	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	57.40%#
20) 2-Butanone-d5	4.18	46	103384	44.58	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	89.16%
24) Chloroform-d	4.64	84	66935	4.41	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	88.20%
26) 1,2-Dichloroethane-d4	5.31	65	38642	4.61	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	92.20%
32) Benzene-d6	5.33	84	130781	4.68	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.60%
36) 1,2-Dichloropropane-d6	6.32	67	43765	4.74	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	94.80%
41) Toluene-d8	7.56	98	124450	4.73	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	94.60%
43) trans-1,3-Dichloropropene-	7.85	79	18947	4.38	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	87.60%
46) 2-Hexanone-d5	8.31	63	83957	43.99	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	87.98%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	34190	4.40	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	88.00%
64) 1,2-Dichlorobenzene-d4	11.85	152	41146	4.77	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	95.40%


Target Compounds				Ovalue
13) Acetone	2.32	43	14514	3.746 ug/L 97
38) Bromodichloromethane	6.75	83	3536	0.170 ug/L 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU060319\
Data File : VU032404.D
Acq On : 03 Jun 2019 19:46
Operator : JC/SP
Sample : K3081-17
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GALE5

Quant Time: Jun 04 09:26:34 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR060319WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Jun 04 08:55:15 2019
Response via : Initial Calibration

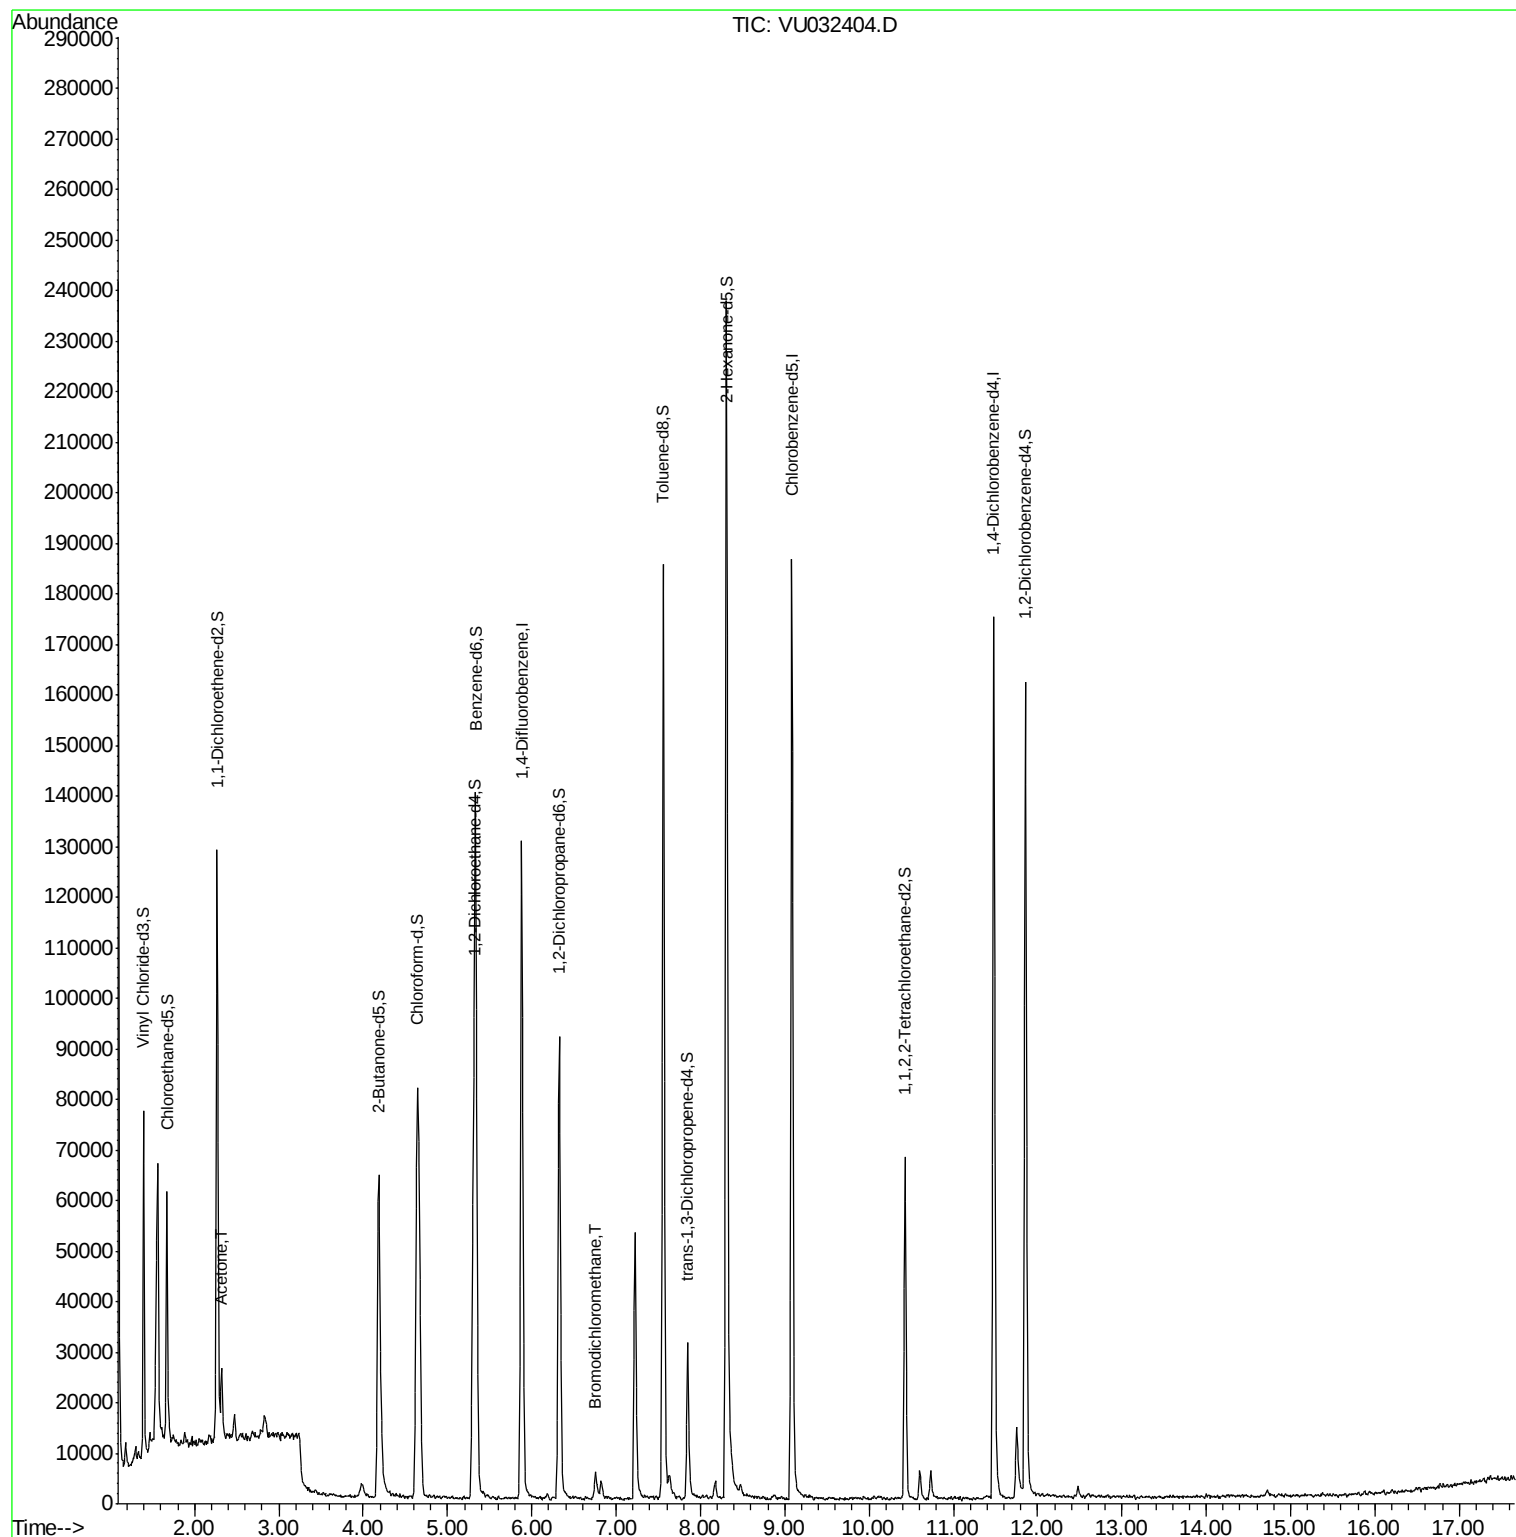

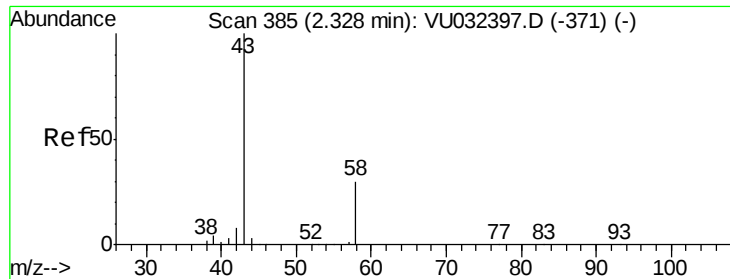

#13

Acetone

Concen: 3.746 ug/L

RT: 2.32 min Scan# 382

Delta R.T. -0.01 min

Lab File: VU032404.D

Acq: 03 Jun 2019 19:46

Instrument :

MSVOA_U

ClientSampled :


GALE5

Tot Ion: 43 Resp: 14514

Ion Ratio Lower Upper

43 100

58 32.7 0.0 62.2


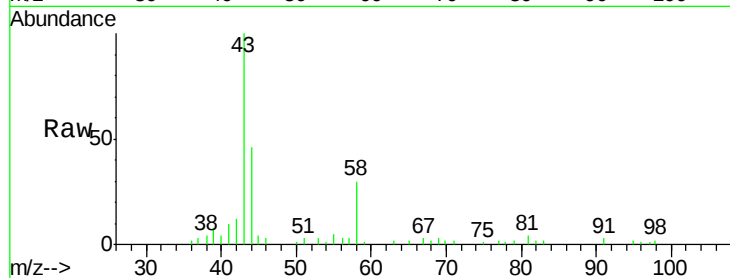


Abundance Ion 43.05 (42.75 to 43.75): VU032397.D (-371) (-)

Ion 58.05 (57.75 to 58.75): VU032397.D (-371) (-)

Time-->

2.25 2.30 2.35 2.40

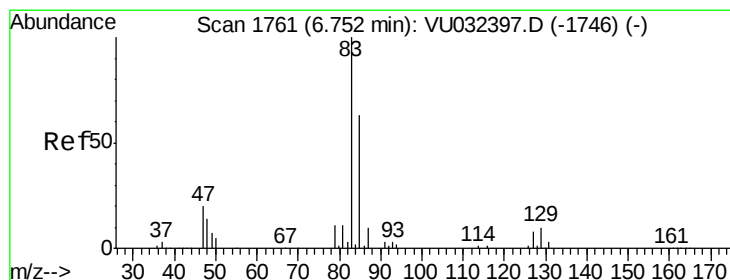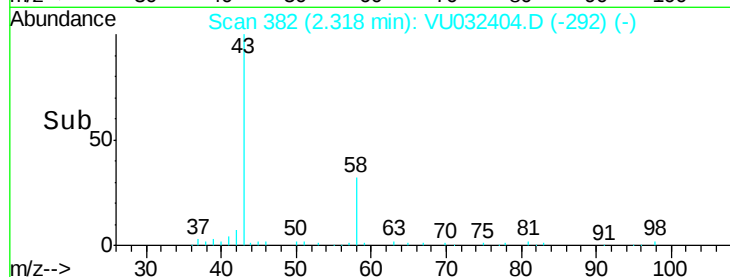

#38

Bromodichloromethane

Concen: 0.170 ug/L

RT: 6.75 min Scan# 1761

Delta R.T. -0.00 min

Lab File: VU032404.D

Acq: 03 Jun 2019 19:46


Tgt Ion: 83 Resp: 3536

Ion Ratio Lower Upper

83 100

85 61.3 45.4 84.4

127 7.5 6.5 9.7

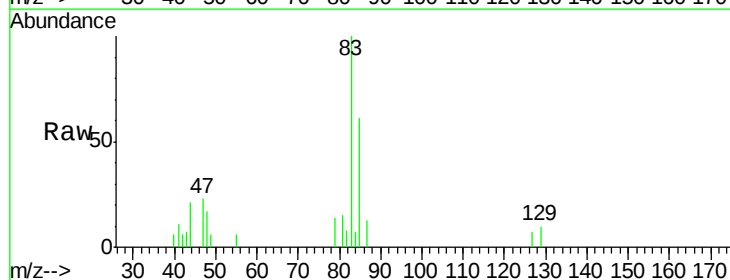

Abundance Ion 82.95 (82.65 to 83.65): VU032397.D (-1746) (-)

Ion 85.00 (84.70 to 85.70): VU032397.D (-1746) (-)

Ion 126.90 (126.60 to 127.60): VU032397.D (-1746) (-)

Time-->

6.70 6.75 6.80

