

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU060319\
 Data File : VU032411.D
 Acq On : 03 Jun 2019 22:39
 Operator : JC/SP
 Sample : K3081-14
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GALE2

Manual Integrations
 APPROVED

MMDadoda
 6/18/2019 1:12:27 AM

Quant Time: Jun 04 09:44:49 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR060319WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Jun 04 08:55:15 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	102163	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.08	117	101174	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	47822	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.39	65	37627	3.92	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	78.40%
7) Chloroethane-d5	1.67	69	36203	3.52	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	70.40%
11) 1,1-Dichloroethene-d2	2.26	63	62042	2.77	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	55.40%#
20) 2-Butanone-d5	4.18	46	122763	55.01	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	110.02%
24) Chloroform-d	4.64	84	68334	4.68	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.60%
26) 1,2-Dichloroethane-d4	5.30	65	42306	5.25	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	105.00%
32) Benzene-d6	5.33	84	133175	4.70	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.00%
36) 1,2-Dichloropropane-d6	6.34	67	46225	4.93	ug/L	0.02
Spiked Amount	5.000	Range	60 - 140	Recovery	=	98.60%
41) Toluene-d8	7.56	98	129735	4.86	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	97.20%
43) trans-1,3-Dichloropropene-	7.85	79	20259	4.61	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	92.20%
46) 2-Hexanone-d5	8.31	63	109931	56.77	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	113.54%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	40629	5.15	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	103.00%
64) 1,2-Dichlorobenzene-d4	11.86	152	44593	4.86	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	97.20%

Target Compounds

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
2) Dichlorodifluoromethane	1.20	85	2355	0.136	ug/L	96
10) 1,1,2-Trichloro-1,2,2-trif	2.28	101	2714	0.180	ug/L	88
22) cis-1,2-Dichloroethene	4.22	96	12700	0.843	ug/L	98
33) Benzene	5.39	78	11235	0.190	ug/L	100
34) Trichloroethene	6.18	95	48472064m	3025.200	ug/L	
47) Tetrachloroethene	8.22	164	27584	2.462	ug/L	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU060319\
Data File : VU032411.D
Acq On : 03 Jun 2019 22:39
Operator : JC/SP
Sample : K3081-14
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 22 Sample Multiplier: 1


Instrument :
MSVOA_U
ClientSampleId :
GALE2

Manual Integrations
APPROVED

MMDadoda
6/18/2019 1:12:27 AM

Quant Time: Jun 04 09:44:49 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR060319WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Jun 04 08:55:15 2019
Response via : Initial Calibration

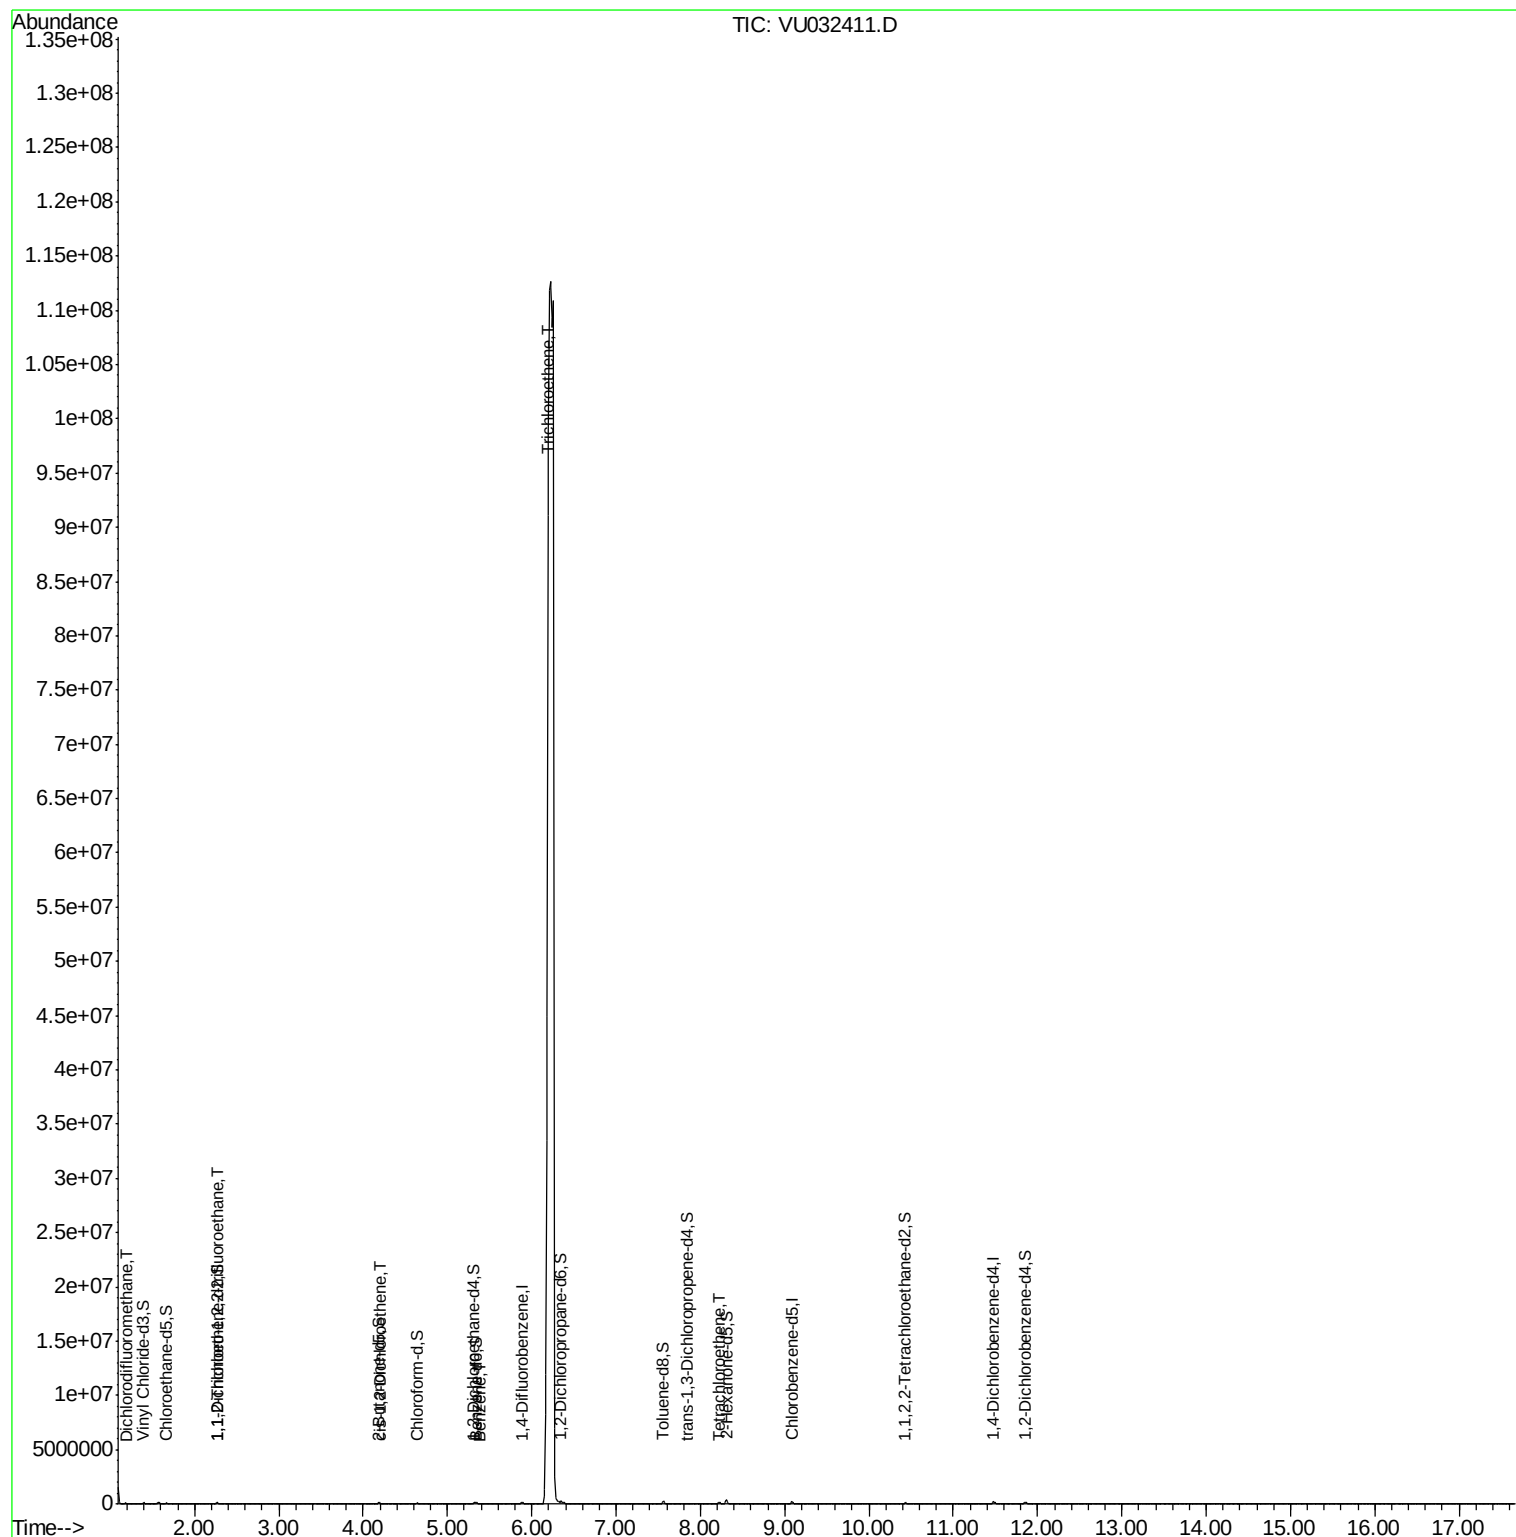

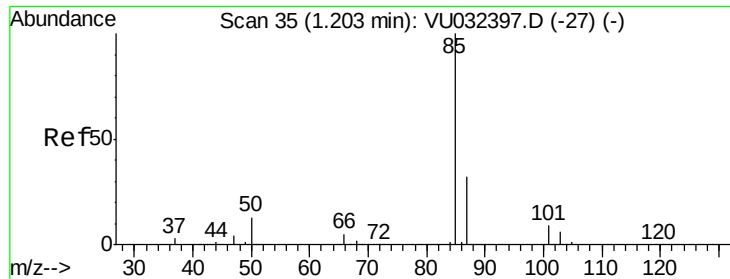

#2

Dichlorodifluoromethane

Concen: 0.136 ug/L

RT: 1.20 min Scan# 35

Delta R.T. 0.00 min

Lab File: VU032411.D

Acq: 03 Jun 2019 22:39

Instrument :

MSVOA_U

ClientSampled :

GALE2

Tot Ion: 85 Resp: 2355

Ion Ratio Lower Upper

85 100


87 30.1 25.8 38.8

Manual Integrations

APPROVED

MMDadoda

6/18/2019 1:12:27 AM

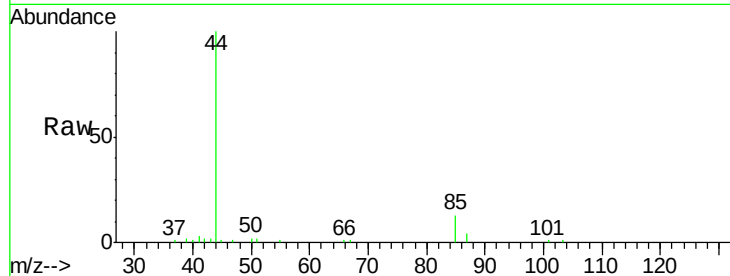

Abundance Ion 85.00 (84.70 to 85.70): VU032411.D (-1) (-)

Ion 87.00 (86.70 to 87.70): VU032411.D (-1) (-)

2500

2000

1500

1000



500

0

1.20

1.25

Time-->

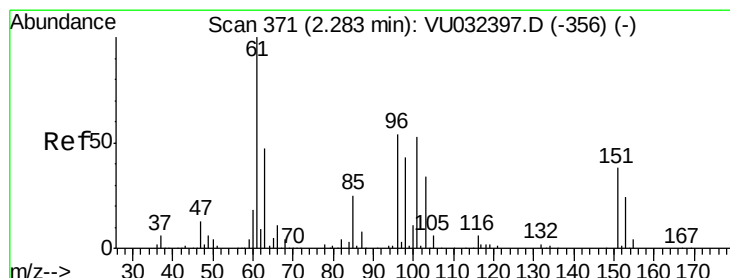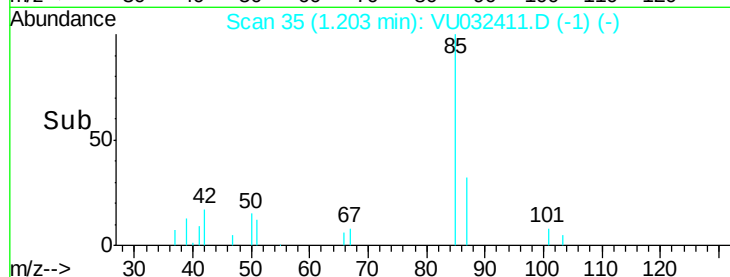

#10

1,1,2-Trichloro-1,2,2-trifluoroethane

Concen: 0.180 ug/L

RT: 2.28 min Scan# 369

Delta R.T. -0.01 min

Lab File: VU032411.D

Acq: 03 Jun 2019 22:39


Tgt Ion: 101 Resp: 2714

Ion Ratio Lower Upper

101 100

85 51.3 38.0 57.0

151 59.7 58.1 87.1

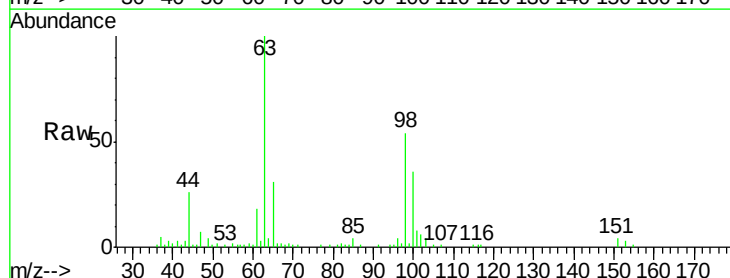

Abundance Ion 101.00 (100.70 to 101.70): VU032411.D (-278) (-)

Ion 85.00 (84.70 to 85.70): VU032411.D (-278) (-)

Ion 151.00 (150.70 to 151.70): VU032411.D (-278) (-)

2000

1500

1000


500


0

2.25

2.30

Time-->

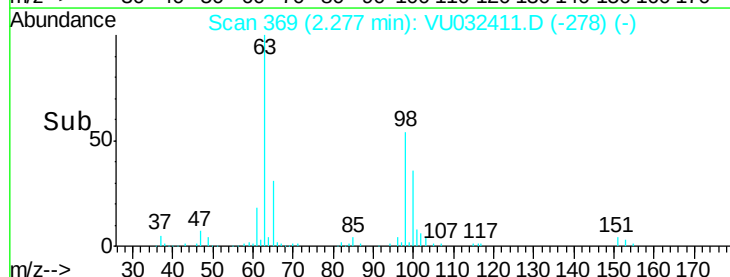

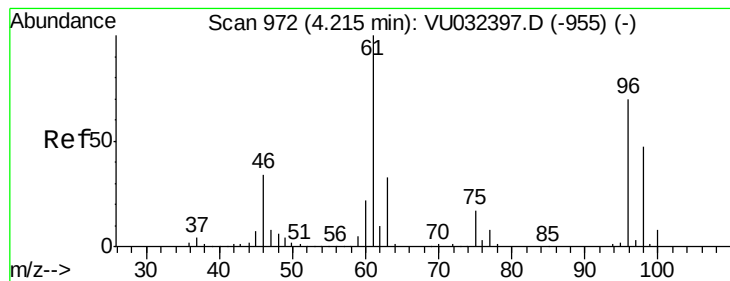

#22

cis-1,2-Dichloroethene

Concen: 0.843 ug/L

RT: 4.22 min Scan# 972

Delta R.T. 0.00 min

Lab File: VU032411.D

Acq: 03 Jun 2019 22:39

Instrument :

MSVOA_U





ClientSampled :

GALE2

Tot Ion:	96	Resp:	12700
Ion Ratio	Lower	Upper	
96	100		
61	139.1	99.0	183.8
68	0.0	0.0	0.0

Manual Integrations
APPROVED

MMDadoda
6/18/2019 1:12:27 AM

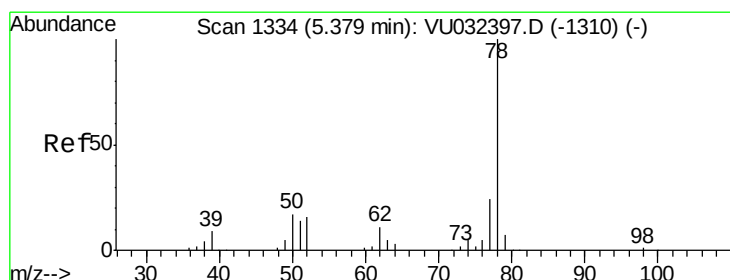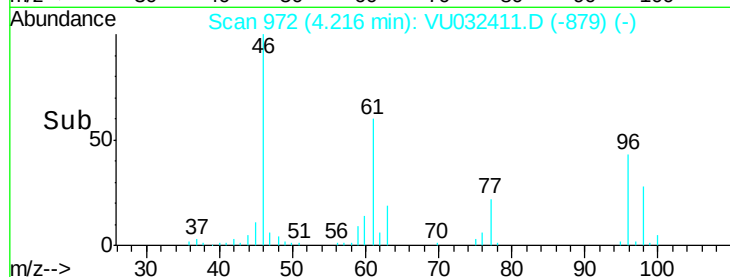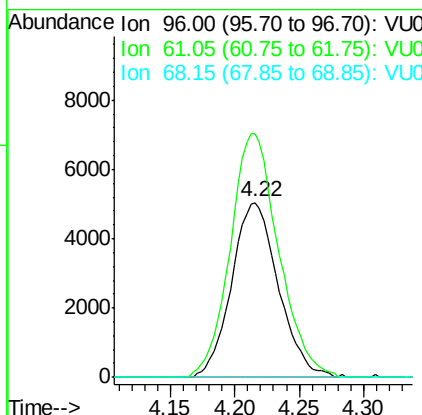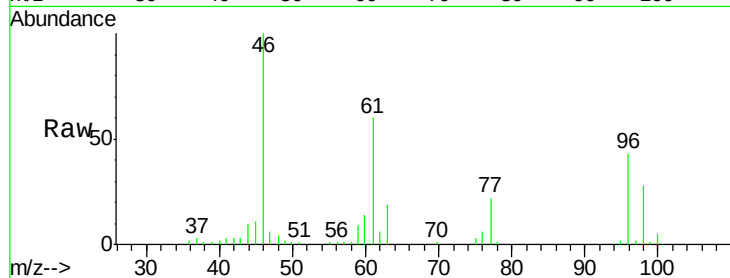

#33

Benzene

Concen: 0.190 ug/L




RT: 5.39 min Scan# 1336


Delta R.T. 0.01 min

Lab File: VU032411.D

Acq: 03 Jun 2019 22:39

Tgt Ion: 78 Resp: 11235

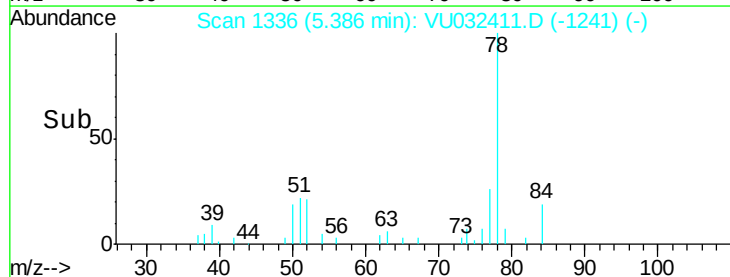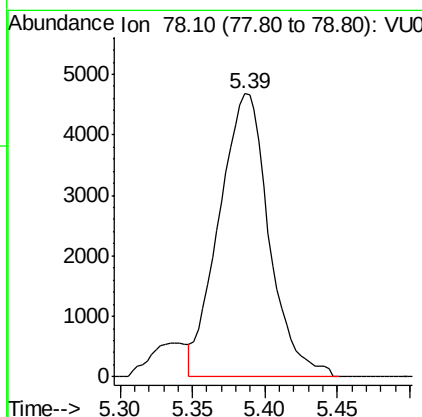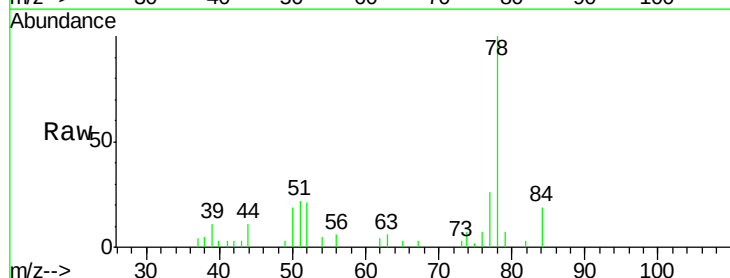

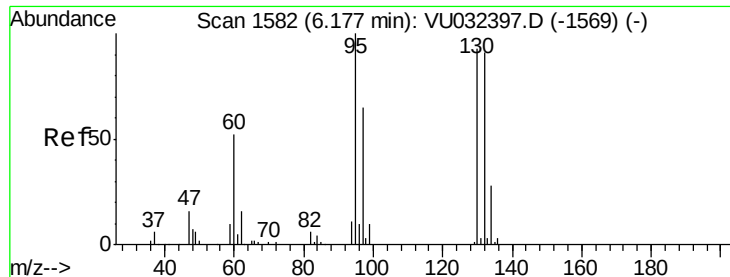

#34

Trichloroethene

Concen: 3025.200 ug/L m

RT: 6.18 min Scan# 1584

Delta R.T. 0.01 min

Lab File: VU032411.D

Acq: 03 Jun 2019 22:39

Instrument :

MSVOA_U

ClientSampleId :

GALE2

Tot Ion: 95 Resp: 48472064

Ion Ratio Lower Upper

95 100

97 81.2 45.8 85.0

132 100.0 63.1 117.1


130 100.0 66.0 122.6

Manual Integrations

APPROVED

MMDadoda

6/18/2019 1:12:27 AM

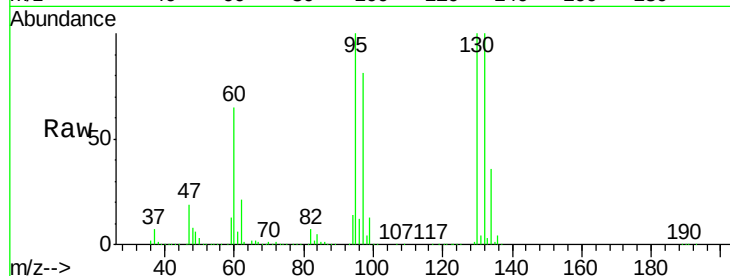


Abundance Ion 95.00 (94.70 to 95.70): VU0

Ion 96.95 (96.65 to 97.65): VU0


Ion 131.95 (131.65 to 132.65): V

Ion 129.95 (129.65 to 130.65): V

Time-->

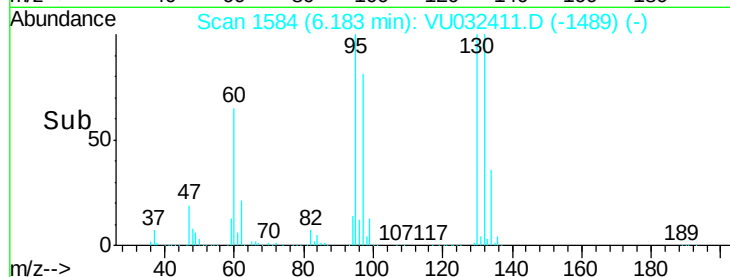

Time-->

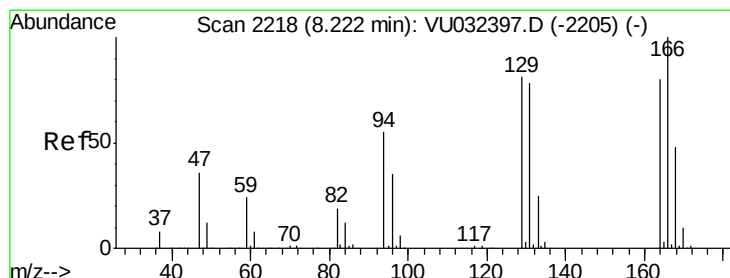

#47

Tetrachloroethene

Concen: 2.462 ug/L

RT: 8.22 min Scan# 2218

Delta R.T. 0.00 min

Lab File: VU032411.D

Acq: 03 Jun 2019 22:39

Tgt Ion: 164 Resp: 27584

Ion Ratio Lower Upper

164 100

129 100.9 72.1 133.9

131 98.5 71.9 133.5

166 124.0 89.0 165.4



Abundance Ion 163.90 (163.60 to 164.60): V

Ion 128.95 (128.65 to 129.65): V

Ion 130.95 (130.65 to 131.65): V

Ion 165.90 (165.60 to 166.60): V

Time-->

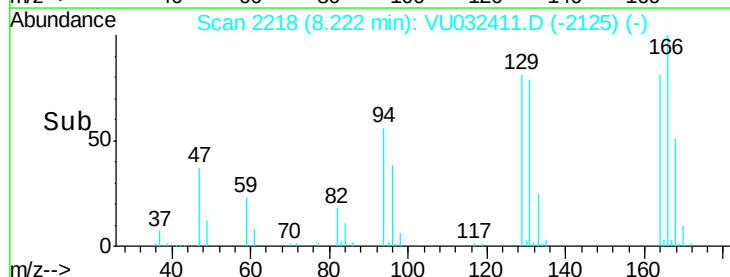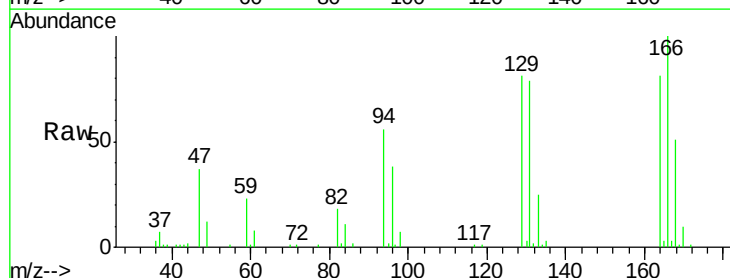

Time-->