


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060320\
 Data File : VU038507.D
 Acq On : 03 Jun 2020 08:58
 Operator : JC/MD
 Sample : BFB50
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB50

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM052820WMA.M
 Title : VOC Analysis
 Last Update : Thu Jun 04 11:55:02 2020

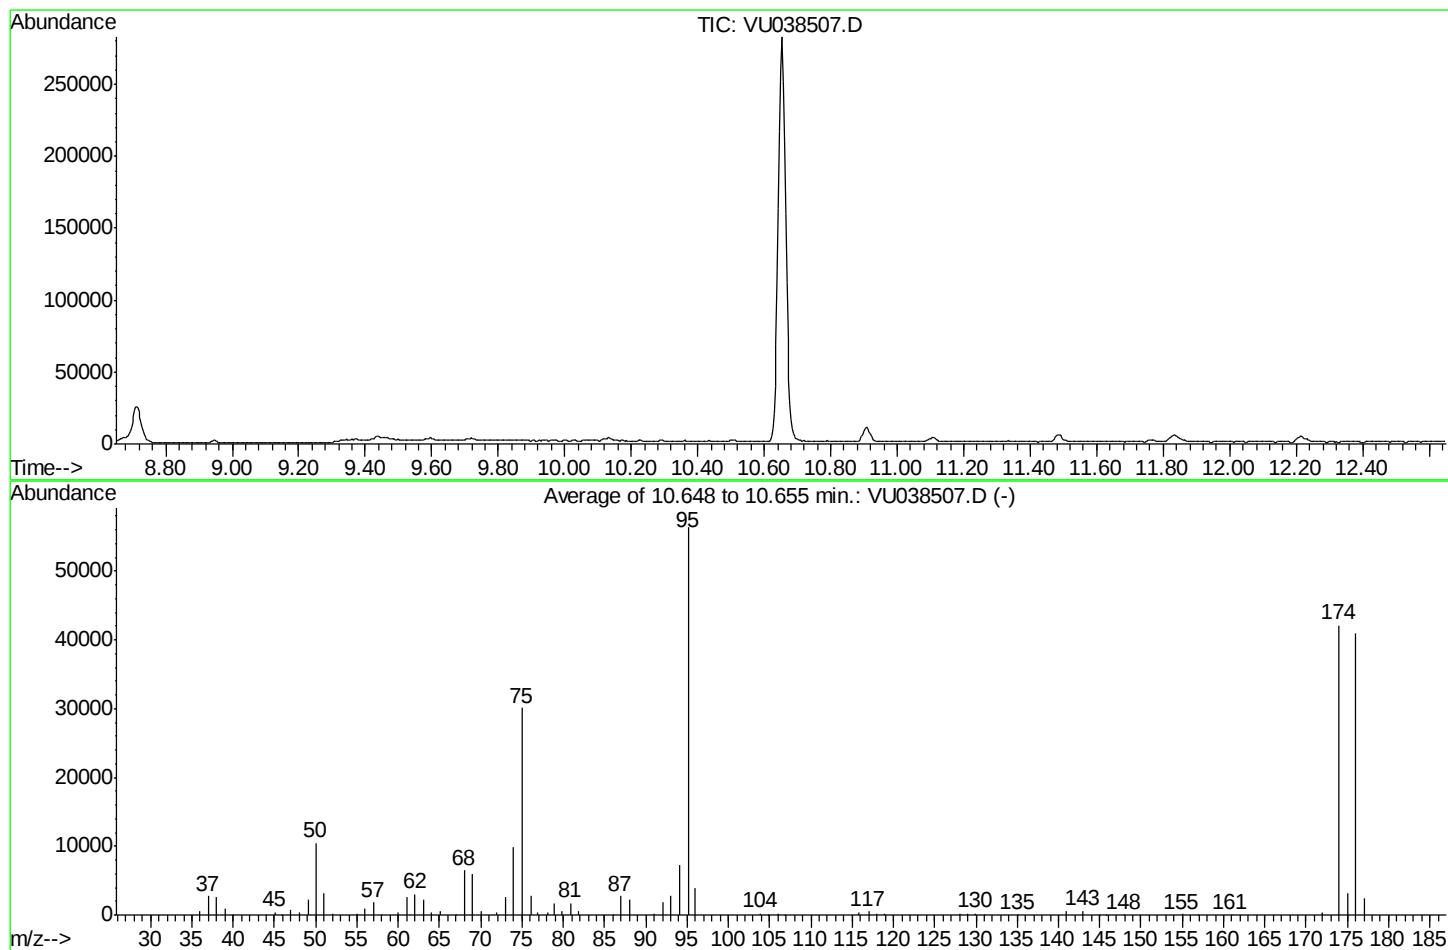

AutoFind: Scans 2895, 2896, 2897; Background Corrected with Scan 2884

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.6	10466	PASS
75	95	30	80	53.4	30114	PASS
95	95	100	100	100.0	56362	PASS
96	95	5	9	7.1	3990	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	74.7	42077	PASS
175	174	5	9	7.6	3197	PASS
176	174	95	101	97.5	41040	PASS
177	176	5	9	6.1	2489	PASS

m/z	Abundance
35.90	1238.0
37.00	2569.0
38.00	2779.0
39.00	1013.0
39.90	271.0
44.00	795.0
45.00	461.0
46.90	751.0
48.00	416.0
49.00	2119.0
50.00	10080.0
51.00	2997.0
52.00	174.0
55.00	238.0
56.00	847.0
57.00	1828.0
57.90	144.0
59.90	458.0
61.00	2654.0
62.00	2834.0
63.00	2175.0
64.10	478.0
65.10	518.0
66.90	156.0
68.00	6159.0
69.00	5838.0
70.00	588.0
71.90	337.0
73.00	2512.0
74.00	9633.0
75.00	28808.0
76.00	2638.0
76.90	398.0
78.10	293.0
78.90	1568.0
79.70	530.0
80.90	1642.0
81.90	543.0
86.90	2524.0
88.00	1973.0
91.00	201.0
92.00	1870.0
93.00	2682.0
94.10	6893.0
95.10	53968.0
96.00	3873.0
103.90	265.0
106.00	222.0
115.80	293.0
117.00	454.0
118.00	230.0
118.90	210.0
128.00	161.0
129.10	116.0
130.00	207.0
141.00	616.0
143.00	569.0
148.00	138.0
155.00	140.0
156.90	100.0
160.90	164.0
172.00	383.0
174.00	39192.0
175.00	3062.0
176.00	38224.0
177.00	2400.0

Instrument :
MSVOA_U
ClientSampleId :
BFB50

m/z	Abundance
35.90	1204.0
37.00	2788.0
38.00	2838.0
39.00	914.0
40.00	267.0
44.00	861.0
45.10	436.0
45.80	111.0
46.90	882.0
48.00	415.0
49.10	2274.0
50.00	10778.0
51.00	3219.0
52.00	160.0
55.10	182.0
56.00	936.0
57.00	1834.0
57.90	116.0
59.90	483.0
61.00	2715.0
62.00	3228.0
63.00	2383.0
64.00	478.0
65.00	576.0
68.00	6748.0
69.00	6221.0
70.00	621.0
71.90	388.0
73.00	2607.0
74.00	10170.0
75.00	31072.0
76.10	2858.0
76.90	508.0
78.00	314.0
79.00	1700.0
79.80	577.0
80.90	1772.0
81.90	579.0
86.10	115.0
86.90	2855.0
88.00	2238.0
90.90	219.0
92.00	1951.0
93.10	2852.0
94.10	7679.0
95.10	58088.0
96.00	4142.0
103.90	265.0
104.80	102.0
106.00	272.0
106.90	101.0
115.80	344.0
117.00	502.0
118.00	234.0
118.80	261.0
128.10	204.0
129.00	113.0
130.00	237.0
131.00	104.0
135.10	116.0
141.00	556.0
143.00	633.0
145.80	118.0
147.90	119.0
155.00	181.0
160.90	133.0
171.90	413.0
174.00	43472.0
175.00	3213.0
176.10	42256.0
177.00	2613.0

Instrument :
MSVOA_U
ClientSampleId :
BFB50

m/z	Abundance
35.00	1188.0
37.00	2807.0
38.00	2739.0
39.10	823.0
40.00	240.0
44.00	859.0
45.10	431.0
46.90	848.0
48.00	323.0
49.10	2136.0
50.00	10540.0
51.00	3162.0
52.00	154.0
55.10	187.0
56.00	862.0
57.00	1704.0
59.90	474.0
61.00	2689.0
62.00	3157.0
63.00	2396.0
64.00	431.0
65.00	606.0
68.00	6606.0
69.00	6030.0
70.00	547.0
72.00	305.0
73.00	2607.0
74.00	9968.0
75.00	30464.0
76.10	2674.0
76.90	484.0
78.00	308.0
79.00	1698.0
79.90	648.0
80.90	1851.0
81.90	627.0
86.00	163.0
86.90	2769.0
88.00	2266.0
90.90	236.0
92.00	1858.0
93.10	2769.0
94.10	7334.0
95.10	57032.0
96.00	3956.0
103.90	294.0
104.80	113.0
106.00	256.0
106.80	106.0
115.80	298.0
117.00	473.0
117.90	205.0
118.80	359.0
128.10	193.0
129.00	137.0
129.90	213.0
135.10	131.0
141.00	547.0
143.00	675.0
145.00	166.0
145.80	138.0
155.00	185.0
172.00	433.0
174.00	43568.0
175.10	3318.0
176.10	42640.0
177.00	2454.0

Instrument :
MSVOA_U
ClientSampleId :
BFB50

Scan 2884 (10.613 min): VU038507.D
BFB49

m/z	Abundance
35.90	702.0
37.80	143.0
40.00	223.0
43.90	764.0

Instrument :
MSVOA_U
ClientSampleId :
BFB50