

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060321\
 Data File : VU044034.D
 Acq On : 03 Jun 2021 12:16
 Operator : SY/MD
 Sample : VU0603WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0603WBL01

Quant Time: Jun 04 06:27:24 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U060221DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Thu Jun 03 11:17:14 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Fluorobenzene	6.124	96	16904	1.000	ug/l	# 0.00
System Monitoring Compounds						
57) 4-Bromofluorobenzene	10.642	95	4270	0.726	ug/l	0.00
Spiked Amount 1.000			Recovery	=	73.000%	
68) 1,2-Dichlorobenzene-d4	12.201	152	4366	0.697	ug/l	0.00
Spiked Amount 1.000			Recovery	=	70.000%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060321\
Data File : VU044034.D
Acq On : 03 Jun 2021 12:16
Operator : SY/MD
Sample : VU0603WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0603WBL01

Quant Time: Jun 04 06:27:24 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U060221DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Thu Jun 03 11:17:14 2021
Response via : Initial Calibration




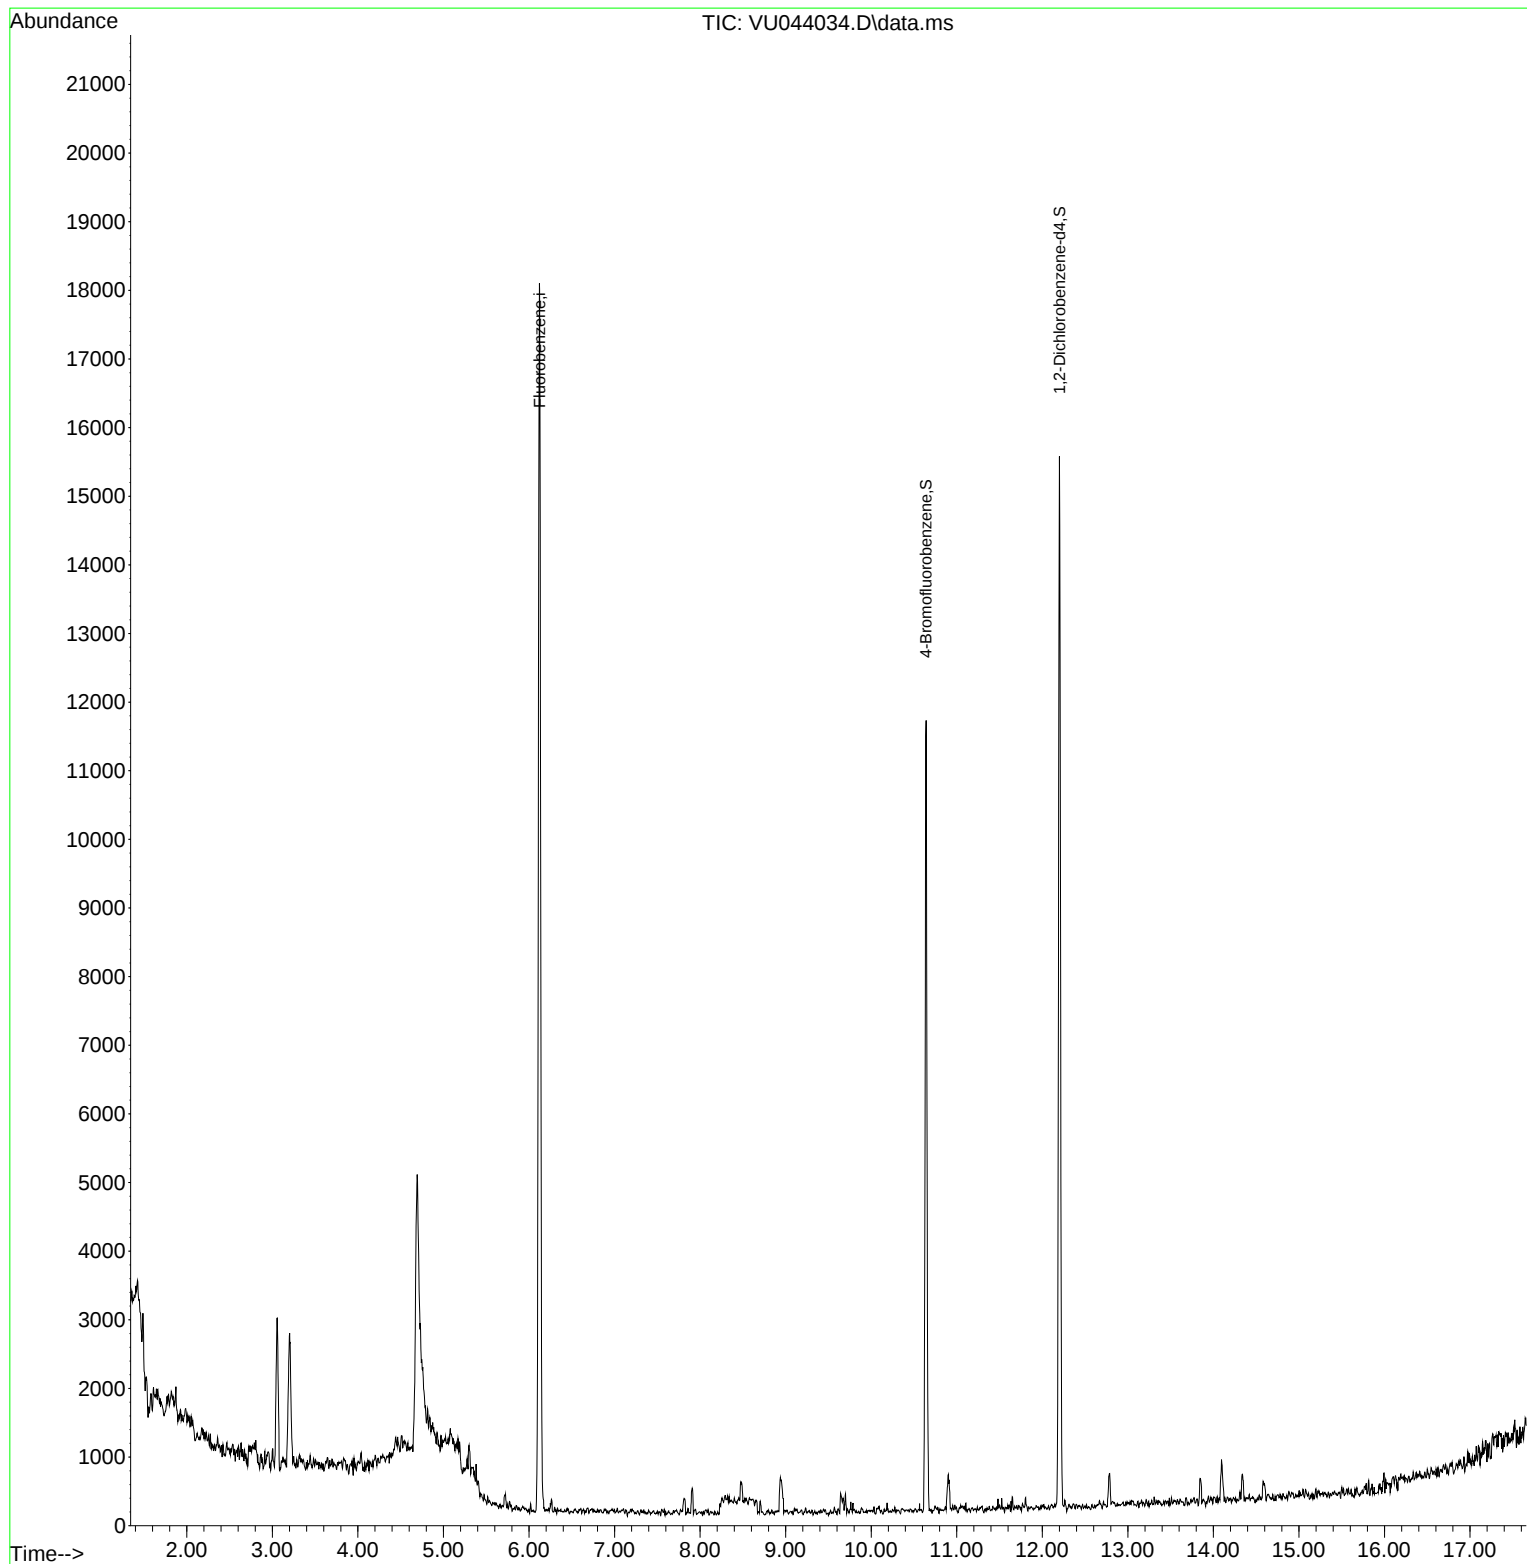


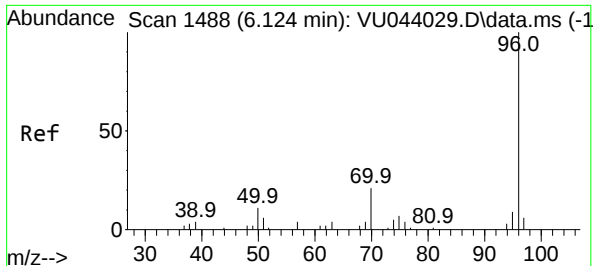

#1
Fluorobenzene
Concen: 1.000 ug/l
RT: 6.124 min Scan# 1488
Delta R.T. 0.000 min
Lab File: VU044034.D
Acq: 03 Jun 2021 12:16




Instrument :
MSVOA_U
ClientSampleId :
VU0603WBL01


Tgt Ion: 96	Resp: 16904
Ion Ratio	Lower Upper
96 100	
70 20.2	16.6 25.0
95 8.2	7.0 10.4
97 5.8	0.0 0.0#

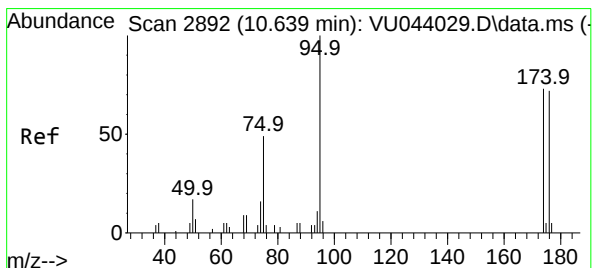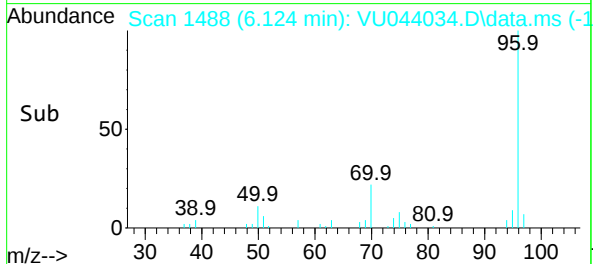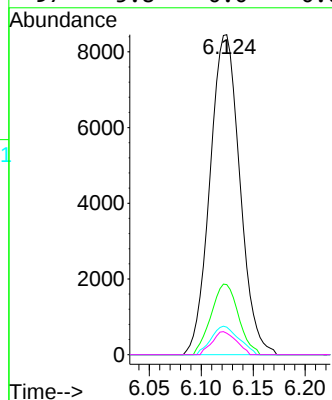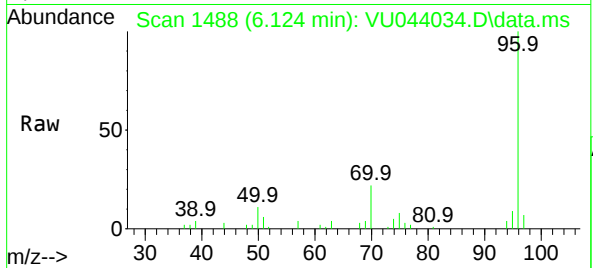

#57
4-Bromofluorobenzene
Concen: 0.726 ug/l
RT: 10.642 min Scan# 2893
Delta R.T. 0.003 min
Lab File: VU044034.D
Acq: 03 Jun 2021 12:16

Tgt Ion: 95	Resp: 4270
Ion Ratio	Lower Upper
95 100	
174 74.4	59.1 88.7
176 72.0	56.4 84.6

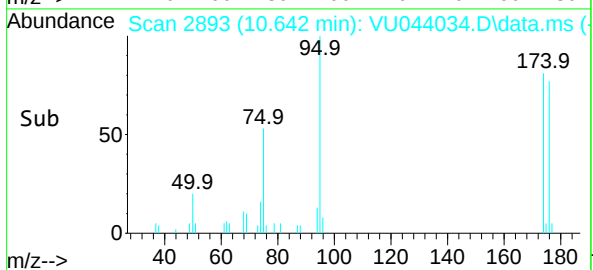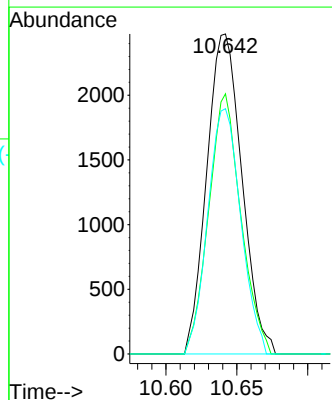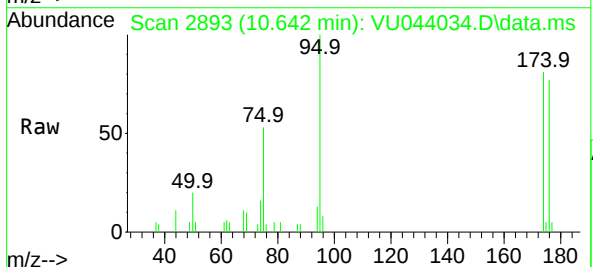

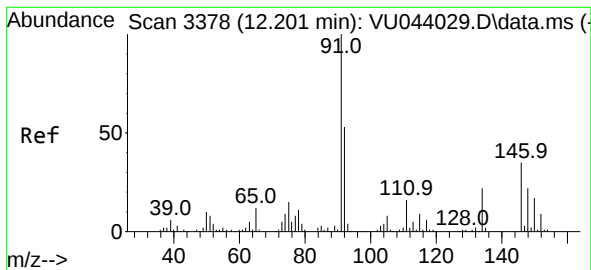

#68
 1,2-Dichlorobenzene-d4
 Concen: 0.697 ug/l
 RT: 12.201 min Scan# 3378
 Delta R.T. 0.000 min
 Lab File: VU044034.D
 Acq: 03 Jun 2021 12:16

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0603WBL01

Tgt Ion:152 Resp: 4366
 Ion Ratio Lower Upper
 152 100
 115 70.2 0.0 320.6
 150 160.4 0.0 687.2

