


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060321\
 Data File : VU044032.D
 Acq On : 03 Jun 2021 10:41
 Operator : SY/MD
 Sample : BFB
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U060221DW.M
 Title : METHOD 524.2 VOLATILES DRINKING WATER
 Last Update : Thu Jun 03 11:17:14 2021

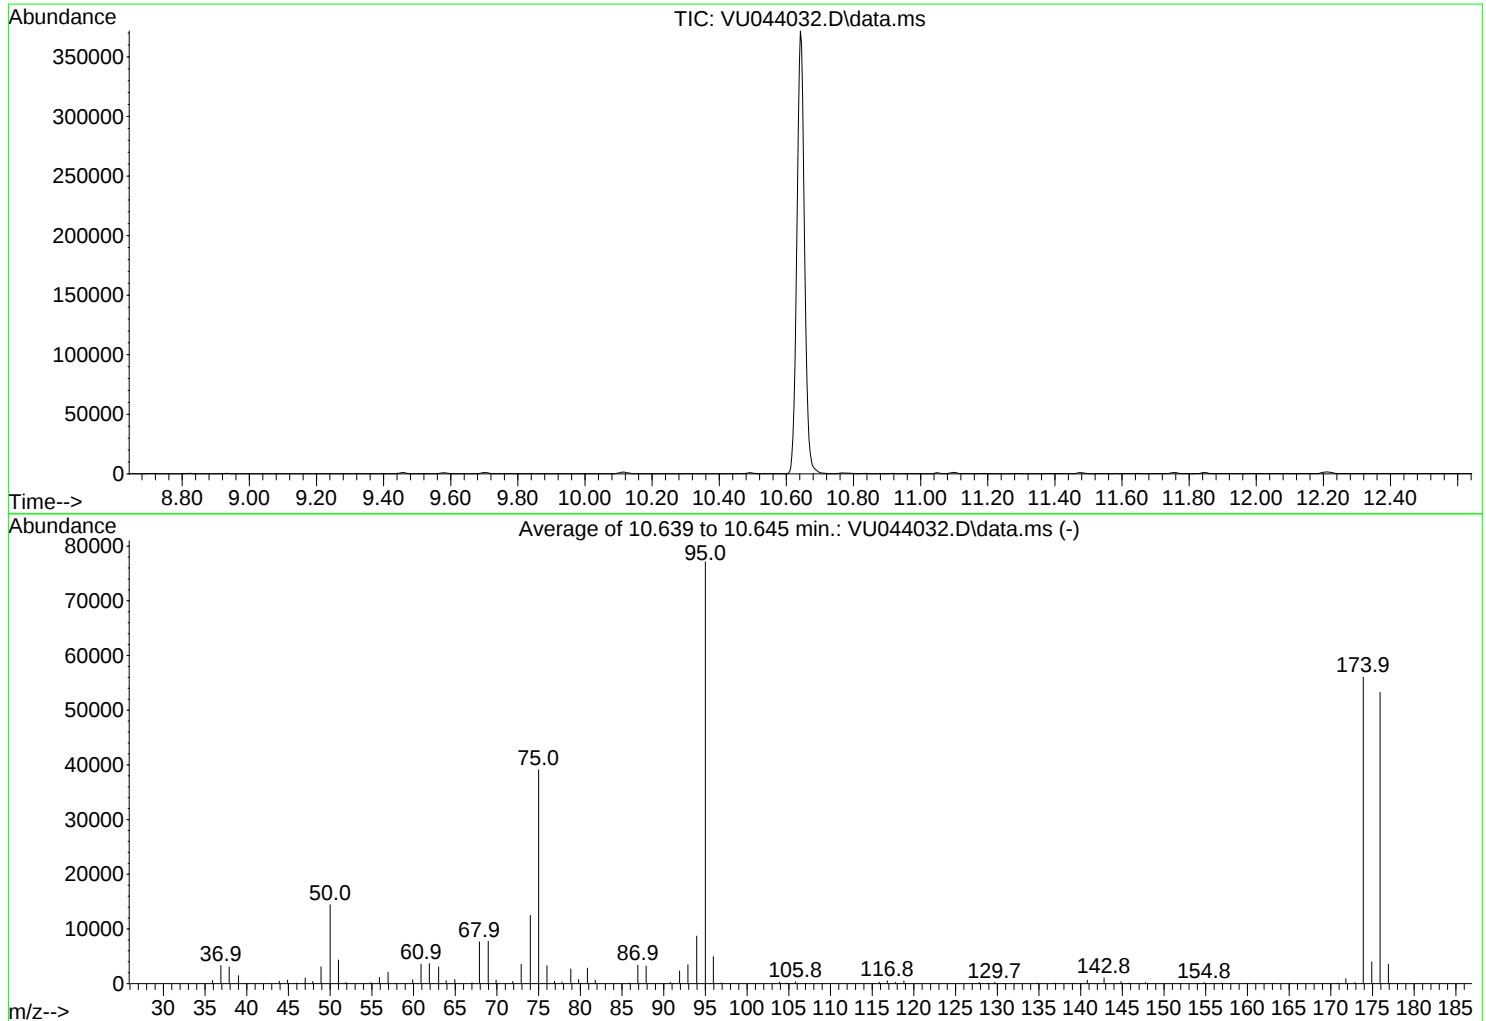

AutoFind: Scans 2892, 2893, 2894; Background Corrected with Scan 2879

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.7	14424	PASS
75	95	30	60	50.7	39120	PASS
95	95	100	100	100.0	77128	PASS
96	95	5	9	6.4	4950	PASS
173	174	0.00	2	0.4	215	PASS
174	95	50	100	72.6	56027	PASS
175	174	5	9	7.1	3982	PASS
176	174	95	101	95.1	53256	PASS
177	176	5	9	6.7	3572	PASS