

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU060419\
 Data File : VU032445.D
 Acq On : 04 Jun 2019 22:27
 Operator : JC/SP
 Sample : VIBLK40
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK40

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.1
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR060419WMA.M
 Title : TRACE VOA SOM01.0

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.180	23	28	33	rBV3	4535	4910	1.40%	0.171%
2	1.395	88	95	107	rBV	47679	51580	14.70%	1.794%
3	1.569	135	149	150	rBV5	13969	26105	7.44%	0.908%
4	1.669	172	180	192	rBV	36717	45955	13.10%	1.599%
5	2.267	356	366	378	rBV	82551	122269	34.84%	4.254%
6	4.183	949	962	1003	rBV	50404	139336	39.71%	4.848%
7	4.640	1086	1104	1126	rBV	54341	128752	36.69%	4.479%
8	5.331	1297	1319	1341	rBV3	113124	310400	88.46%	10.799%
9	5.878	1476	1489	1508	rBV	125417	243024	69.26%	8.455%
10	6.183	1573	1584	1594	rVB6	3894	7679	2.19%	0.267%
11	6.324	1616	1628	1647	rBV	71901	142484	40.61%	4.957%
12	7.225	1898	1908	1934	rBV	38126	70008	19.95%	2.436%
13	7.559	1999	2012	2033	rBV	148580	262766	74.88%	9.142%
14	7.848	2092	2102	2117	rBV	21750	38514	10.98%	1.340%
15	8.308	2234	2245	2281	rBV	189071	350899	100.00%	12.208%
16	9.086	2475	2487	2511	rBV	170741	293770	83.72%	10.220%
17	10.427	2893	2904	2922	rBV	58111	93577	26.67%	3.256%
18	11.479	3219	3231	3261	rBV	173291	293368	83.60%	10.206%
19	11.858	3336	3349	3375	rBV	137605	241357	68.78%	8.397%
20	17.350	5050	5057	5067	rBV2	4574	7632	2.17%	0.266%


Sum of corrected areas: 2874385

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU060419\
Data File : VU032445.D
Acq On : 04 Jun 2019 22:27
Operator : JC/SP
Sample : VIBLK40
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK40

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR060419WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

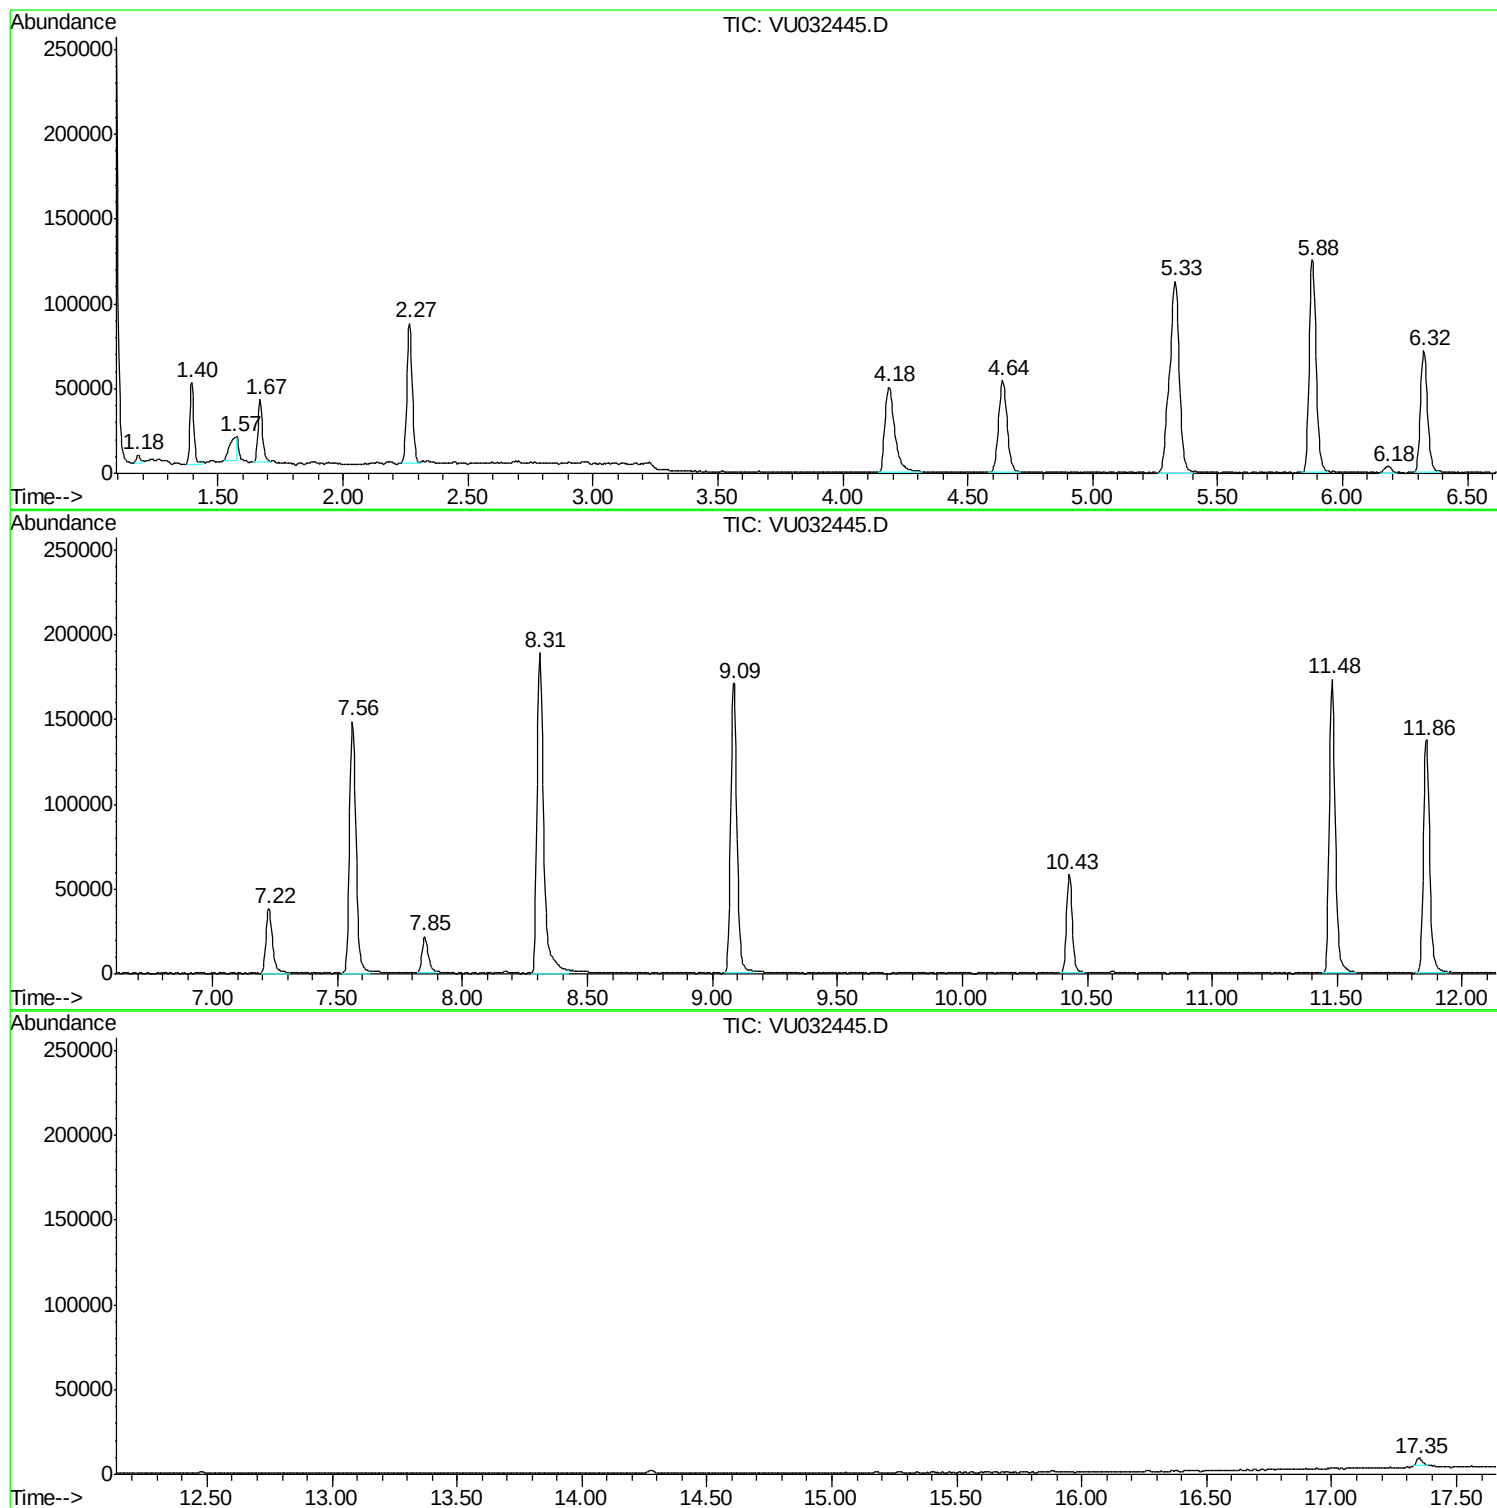

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU060419\
Data File : VU032445.D
Acq On : 04 Jun 2019 22:27
Operator : JC/SP
Sample : VIBLK40
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK40










Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR060419WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown-01 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.57	0.54 ug/L	26105	1,4-Difluorobenzene	5.88

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Propanoic acid, 2-chloro-, ethyl...	136	C5H9ClO2	000535-13-7	14
2		Methane, chloromethoxy-	80	C2H5ClO	000107-30-2	12
3		Carbonic acid, isohexyl propyl e...	188	C10H20O3	1000314-53-3	9
4		Methylthio-2-propanone	104	C4H8OS	014109-72-9	9
5		Isobutyl chloroformate	136	C5H9ClO2	000543-27-1	4

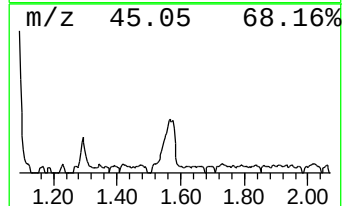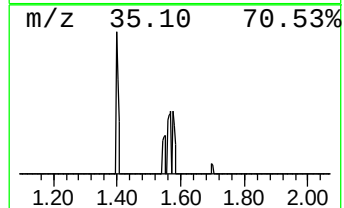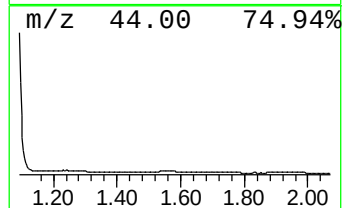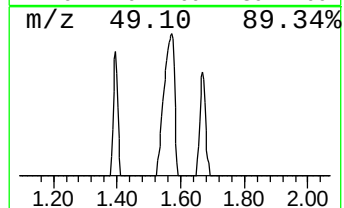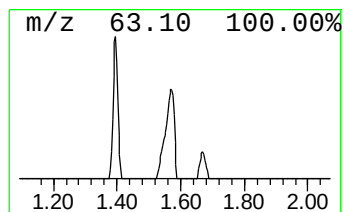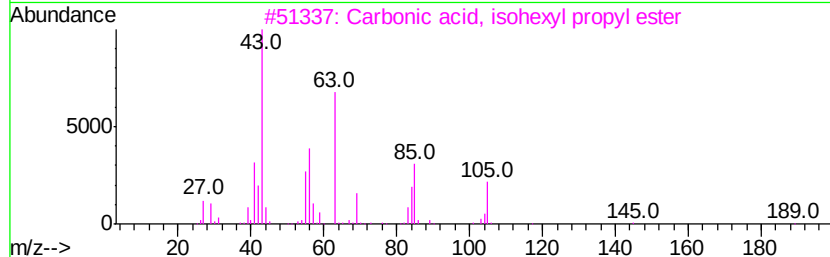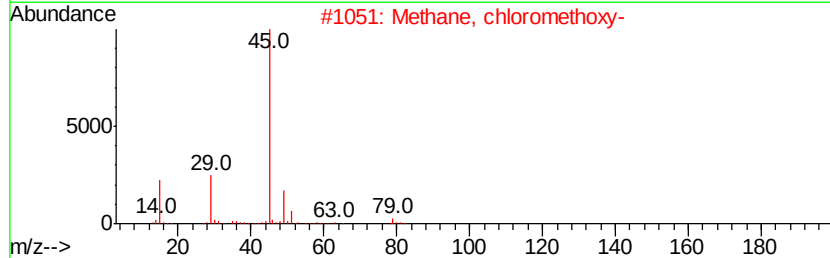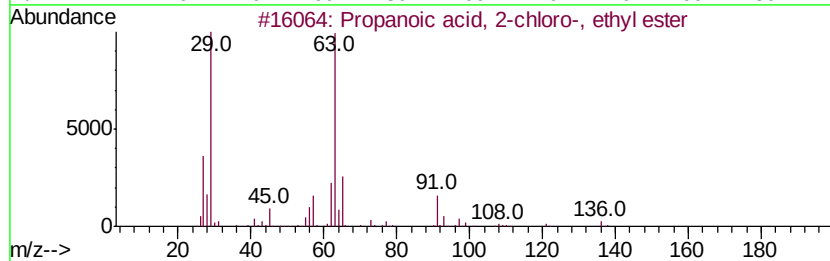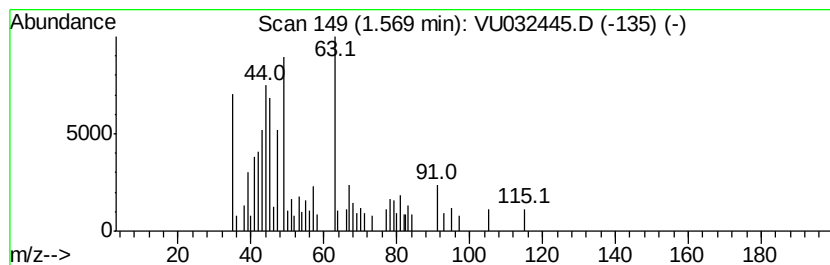

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU060419\
Data File : VU032445.D
Acq On : 04 Jun 2019 22:27
Operator : JC/SP
Sample : VIBLK40
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK40

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR060419WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown-01	1.57	0.5	ug/L	26105	1	5.88	243024	5.0