


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU060419\
 Data File : VU032420.D
 Acq On : 04 Jun 2019 11:57
 Operator : JC/SP
 Sample : BFB15
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB15

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR060419WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Tue Jun 04 22:54:09 2019

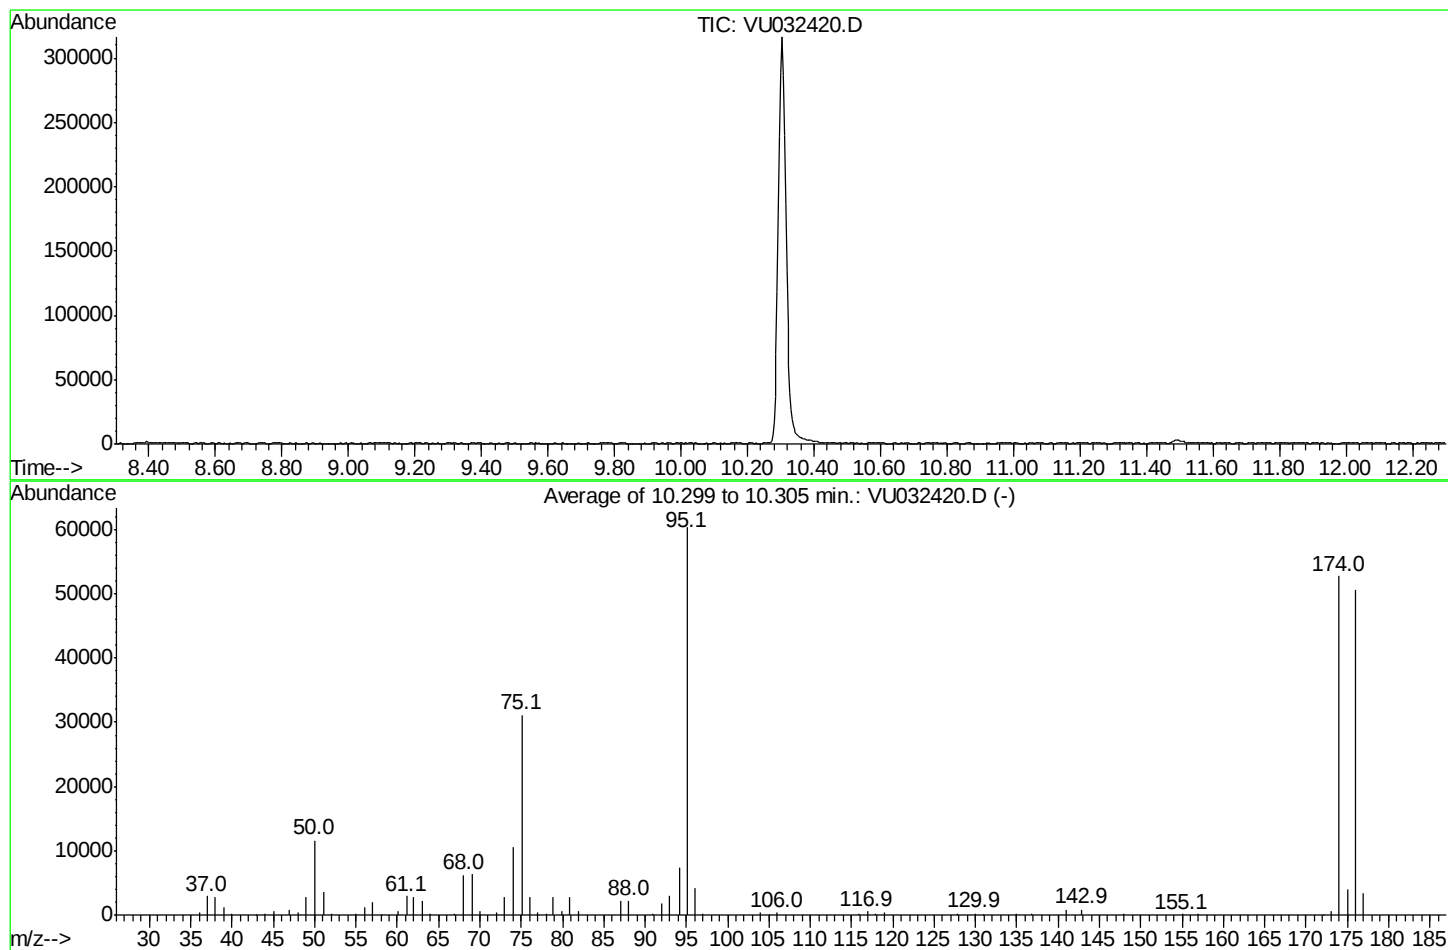

AutoFind: Scans 2864, 2865, 2866; Background Corrected with Scan 2852

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.3	11640	PASS
75	95	30	80	51.6	31112	PASS
95	95	100	100	100.0	60346	PASS
96	95	5	9	6.8	4100	PASS
173	174	0.00	2	1.3	663	PASS
174	95	50	120	87.4	52749	PASS
175	174	5	9	7.5	3956	PASS
176	174	95	101	96.1	50672	PASS
177	176	5	9	6.7	3376	PASS

m/z	Abundance
44.00	561.0

Instrument :
MSVOA_U
ClientSampleId :
BFB15

m/z	Abundance
36.00	503.0
37.00	2832.0
38.00	2638.0
39.00	1056.0
39.90	148.0
42.90	101.0
44.00	866.0
45.00	512.0
46.90	674.0
48.00	398.0
49.00	2597.0
50.00	11086.0
51.00	3478.0
52.00	133.0
55.00	236.0
56.00	1079.0
57.00	1831.0
60.10	461.0
61.10	2711.0
62.00	2598.0
63.00	2109.0
64.00	282.0
66.90	186.0
68.00	5958.0
69.00	6235.0
70.00	609.0
72.00	334.0
73.00	2734.0
74.00	10052.0
75.10	29608.0
76.00	2699.0
77.00	345.0
78.00	249.0
78.90	2572.0
79.90	656.0
80.90	2616.0
81.90	490.0
87.00	2113.0
88.00	2220.0
90.90	252.0
92.00	1750.0
93.00	2842.0
94.10	7207.0
95.10	57384.0
96.10	3868.0
97.00	140.0
103.90	308.0
106.00	332.0
115.90	210.0
116.90	513.0
117.90	232.0
118.90	357.0
127.80	144.0
129.90	192.0
130.90	100.0
134.90	166.0
136.90	104.0
141.00	621.0
142.90	842.0
148.00	163.0
155.10	160.0
156.90	118.0
173.10	615.0
174.00	48408.0
175.00	3749.0
176.00	46608.0
177.00	3197.0

Instrument :
MSVOA_U
ClientSampleId :
BFB15

m/z	Abundance
36.00	512.0
37.00	3070.0
38.00	2985.0
39.00	1161.0
39.90	125.0
43.00	102.0
44.00	842.0
45.00	585.0
46.90	757.0
48.00	434.0
49.00	2857.0
50.00	11978.0
51.10	3705.0
52.00	157.0
55.00	271.0
56.00	1137.0
57.10	1984.0
58.00	104.0
60.00	536.0
61.10	2984.0
62.00	2834.0
63.00	2217.0
64.00	321.0
67.00	207.0
68.00	6373.0
69.00	6519.0
70.10	654.0
72.00	341.0
73.00	2980.0
74.00	10806.0
75.10	32104.0
76.00	2867.0
76.90	335.0
78.00	278.0
78.90	2854.0
79.90	698.0
80.90	2919.0
81.90	536.0
87.00	2274.0
88.00	2302.0
91.00	277.0
92.00	1893.0
93.00	3008.0
94.10	7733.0
95.10	62224.0
96.10	4203.0
97.00	145.0
103.90	338.0
105.00	107.0
106.00	362.0
115.90	226.0
116.90	539.0
117.80	242.0
118.90	356.0
127.80	182.0
129.90	228.0
130.90	108.0
134.90	170.0
136.90	125.0
141.00	743.0
142.90	893.0
147.90	165.0
155.10	155.0
156.90	124.0
172.00	126.0
173.10	689.0
174.00	54536.0
175.00	4066.0
176.00	52192.0
177.00	3502.0

Instrument :
MSVOA_U
ClientSampleId :
BFB15

m/z	Abundance
36.00	493.0
37.00	3066.0
38.00	3000.0
39.00	1169.0
40.00	115.0
44.10	851.0
45.00	572.0
46.90	722.0
48.00	449.0
49.00	2818.0
50.00	11856.0
51.10	3574.0
52.00	166.0
55.00	273.0
56.00	1104.0
57.10	1895.0
60.00	592.0
61.10	2995.0
62.00	2769.0
63.00	2166.0
64.00	300.0
67.00	195.0
68.00	6353.0
69.00	6244.0
70.00	643.0
72.00	324.0
73.00	2892.0
74.00	10711.0
75.10	31624.0
76.00	2725.0
76.90	309.0
78.00	266.0
78.90	2740.0
79.90	679.0
80.90	2976.0
82.00	555.0
87.00	2257.0
88.00	2264.0
91.00	287.0
92.00	1805.0
93.00	2840.0
94.10	7404.0
95.10	61432.0
96.10	4229.0
97.00	155.0
103.90	330.0
105.00	116.0
106.00	339.0
115.90	266.0
116.90	487.0
117.80	263.0
118.90	338.0
127.90	223.0
129.90	242.0
130.90	107.0
135.00	178.0
136.80	133.0
140.90	799.0
142.90	772.0
147.90	172.0
155.00	140.0
156.90	118.0
172.10	137.0
173.10	687.0
174.00	55304.0
175.00	4055.0
176.00	53216.0
177.00	3429.0

Instrument :
MSVOA_U
ClientSampleId :
BFB15