

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU060420\
 Data File : VU038524.D
 Acq On : 03 Jun 2020 19:21
 Operator : SY/MD
 Sample : L2844-14
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AE8

Quant Time: Jun 04 03:46:23 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR053120WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Jun 04 01:48:03 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.28	114	284653	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.44	117	288704	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.82	152	138093	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.61	65	55627	3.02	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	60.40%
7) Chloroethane-d5	1.93	69	58061	4.10	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	82.00%
11) 1,1-Dichloroethene-d2	2.59	63	98731	2.72	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	54.40%#
20) 2-Butanone-d5	4.67	46	342606	61.22	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	122.44%
24) Chloroform-d	5.10	84	176991	5.11	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	102.20%
26) 1,2-Dichloroethane-d4	5.74	65	109744	5.59	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	111.80%
32) Benzene-d6	5.76	84	334808	4.65	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.00%
36) 1,2-Dichloropropane-d6	6.72	67	107831	4.87	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	97.40%
41) Toluene-d8	7.92	98	272004	4.21	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	84.20%
43) trans-1,3-Dichloropropene-	8.20	79	44012	4.62	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	92.40%
46) 2-Hexanone-d5	8.66	63	285805	60.72	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	121.44%
57) 1,1,2,2-Tetrachloroethane-	10.77	84	102334	5.44	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	108.80%
64) 1,2-Dichlorobenzene-d4	12.20	152	121409	5.10	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	102.00%


Target Compounds					Ovalue
13) Acetone	2.67	43	8134	2.221 ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU060420\
Data File : VU038524.D
Acq On : 03 Jun 2020 19:21
Operator : SY/MD
Sample : L2844-14
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AE8

Quant Time: Jun 04 03:46:23 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR053120WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Jun 04 01:48:03 2020
Response via : Initial Calibration

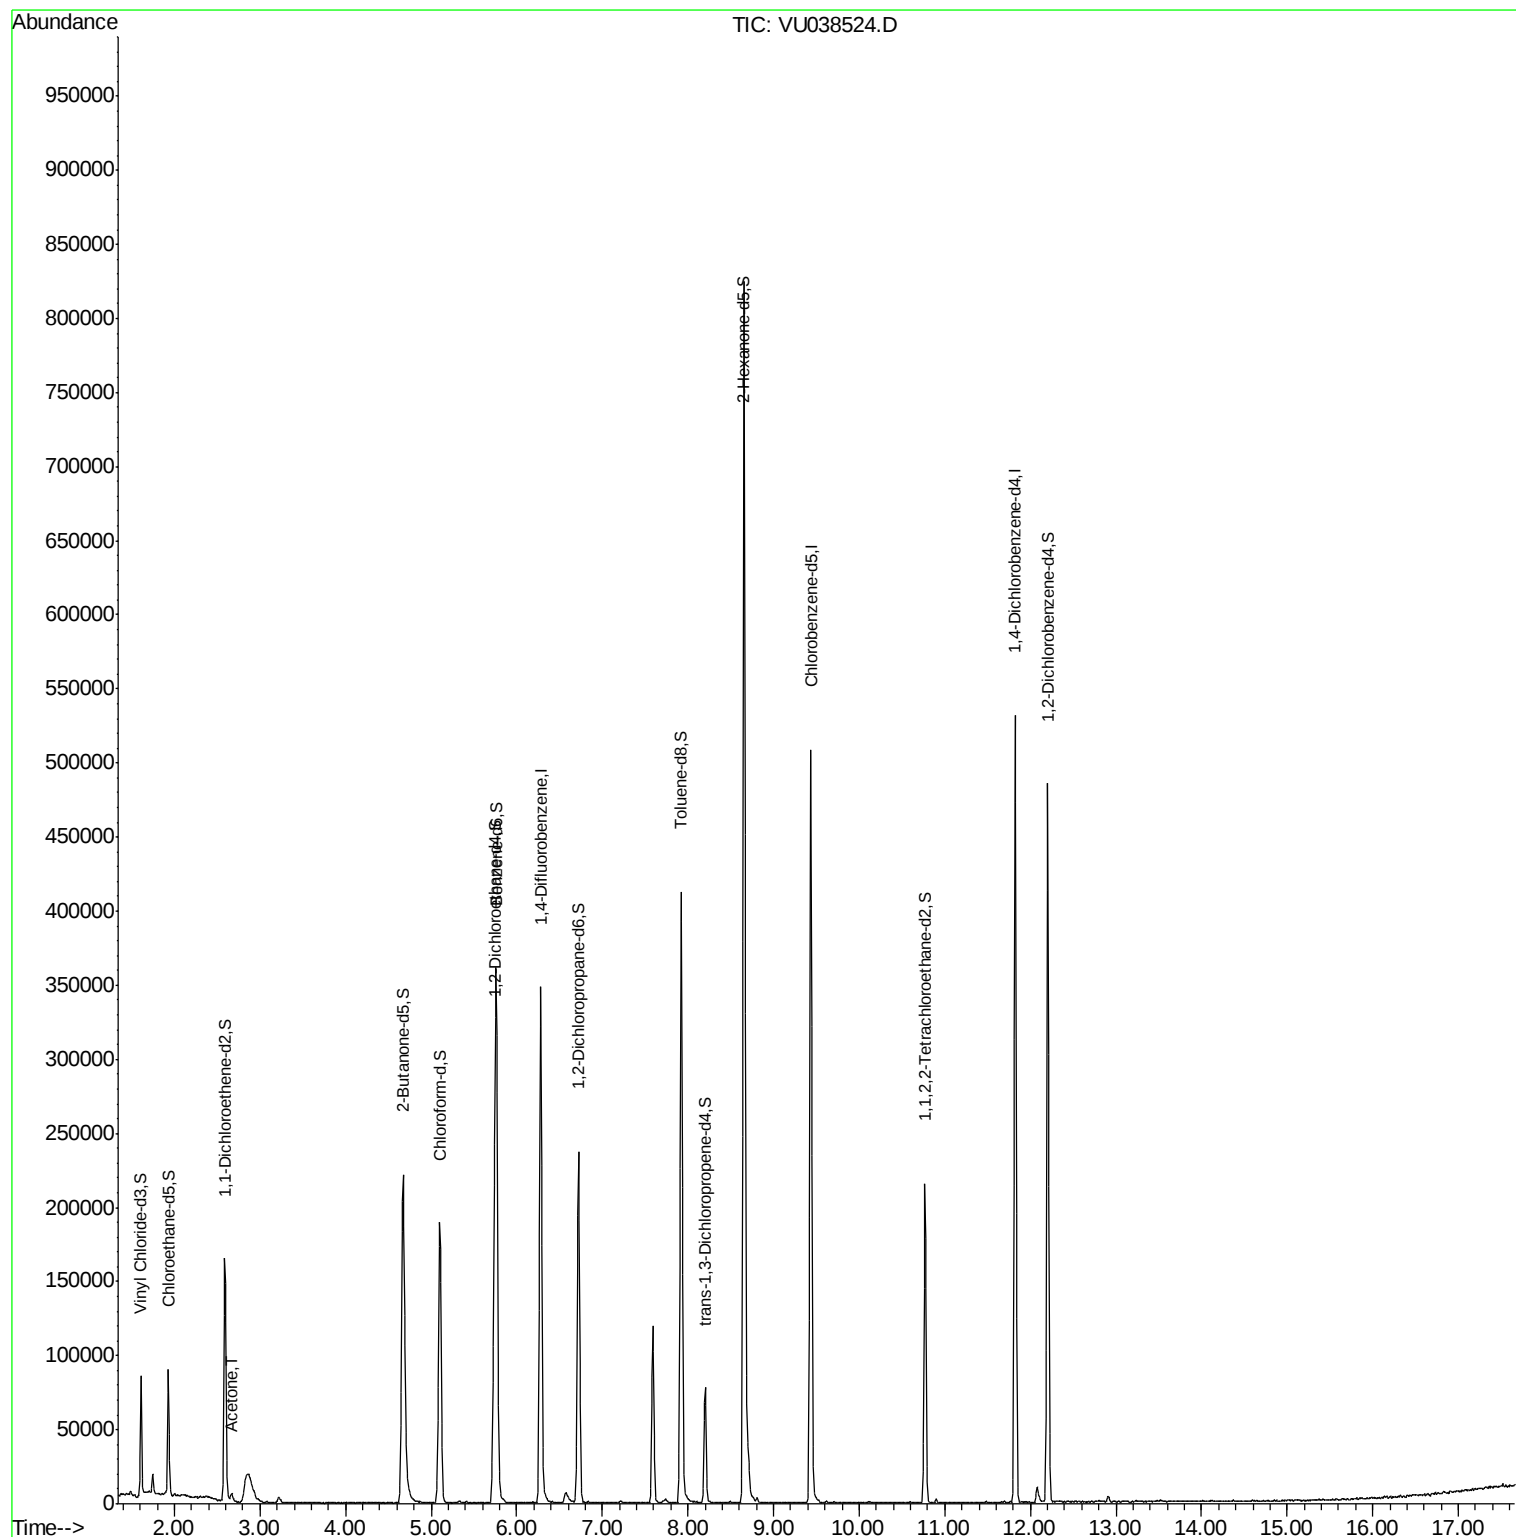

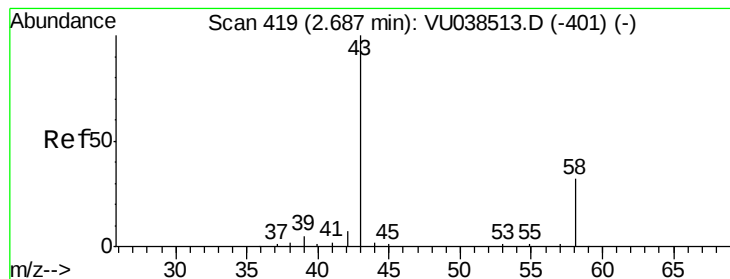

#13
 Acetone
 Concen: 2.221 ug/L
 RT: 2.67 min Scan# 414
 Delta R.T. -0.02 min
 Lab File: VU038524.D
 Acq: 03 Jun 2020 19:21

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AE8

Tot Ion: 43 Resp: 8134
 Ion Ratio Lower Upper
 43 100
 58 31.2 0.0 65.6

