

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU060420\
 Data File : VU038528.D
 Acq On : 03 Jun 2020 20:54
 Operator : SY/MD
 Sample : L2844-20
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AG1

Quant Time: Jun 04 04:36:53 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR053120WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Jun 04 01:48:03 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.28	114	296284	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.44	117	290593	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.82	152	142843	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.61	65	52534	2.74	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	54.80%
7) Chloroethane-d5	1.93	69	57728	3.92	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	78.40%
11) 1,1-Dichloroethene-d2	2.59	63	94574	2.51	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	50.20%#
20) 2-Butanone-d5	4.67	46	327965	56.30	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	112.60%
24) Chloroform-d	5.10	84	166751	4.63	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	92.60%
26) 1,2-Dichloroethane-d4	5.74	65	106125	5.19	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	103.80%
32) Benzene-d6	5.76	84	325818	4.49	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.80%
36) 1,2-Dichloropropane-d6	6.72	67	104724	4.69	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	93.80%
41) Toluene-d8	7.92	98	269183	4.14	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	82.80%
43) trans-1,3-Dichloropropene-	8.20	79	41573	4.33	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	86.60%
46) 2-Hexanone-d5	8.66	63	281854	59.49	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	118.98%
57) 1,1,2,2-Tetrachloroethane-	10.77	84	101280	5.35	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	107.00%
64) 1,2-Dichlorobenzene-d4	12.20	152	121129	4.92	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	98.40%


Target Compounds					Ovalue
13) Acetone	2.67	43	12534	3.288 ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU060420\
Data File : VU038528.D
Acq On : 03 Jun 2020 20:54
Operator : SY/MD
Sample : L2844-20
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AG1

Quant Time: Jun 04 04:36:53 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR053120WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Jun 04 01:48:03 2020
Response via : Initial Calibration

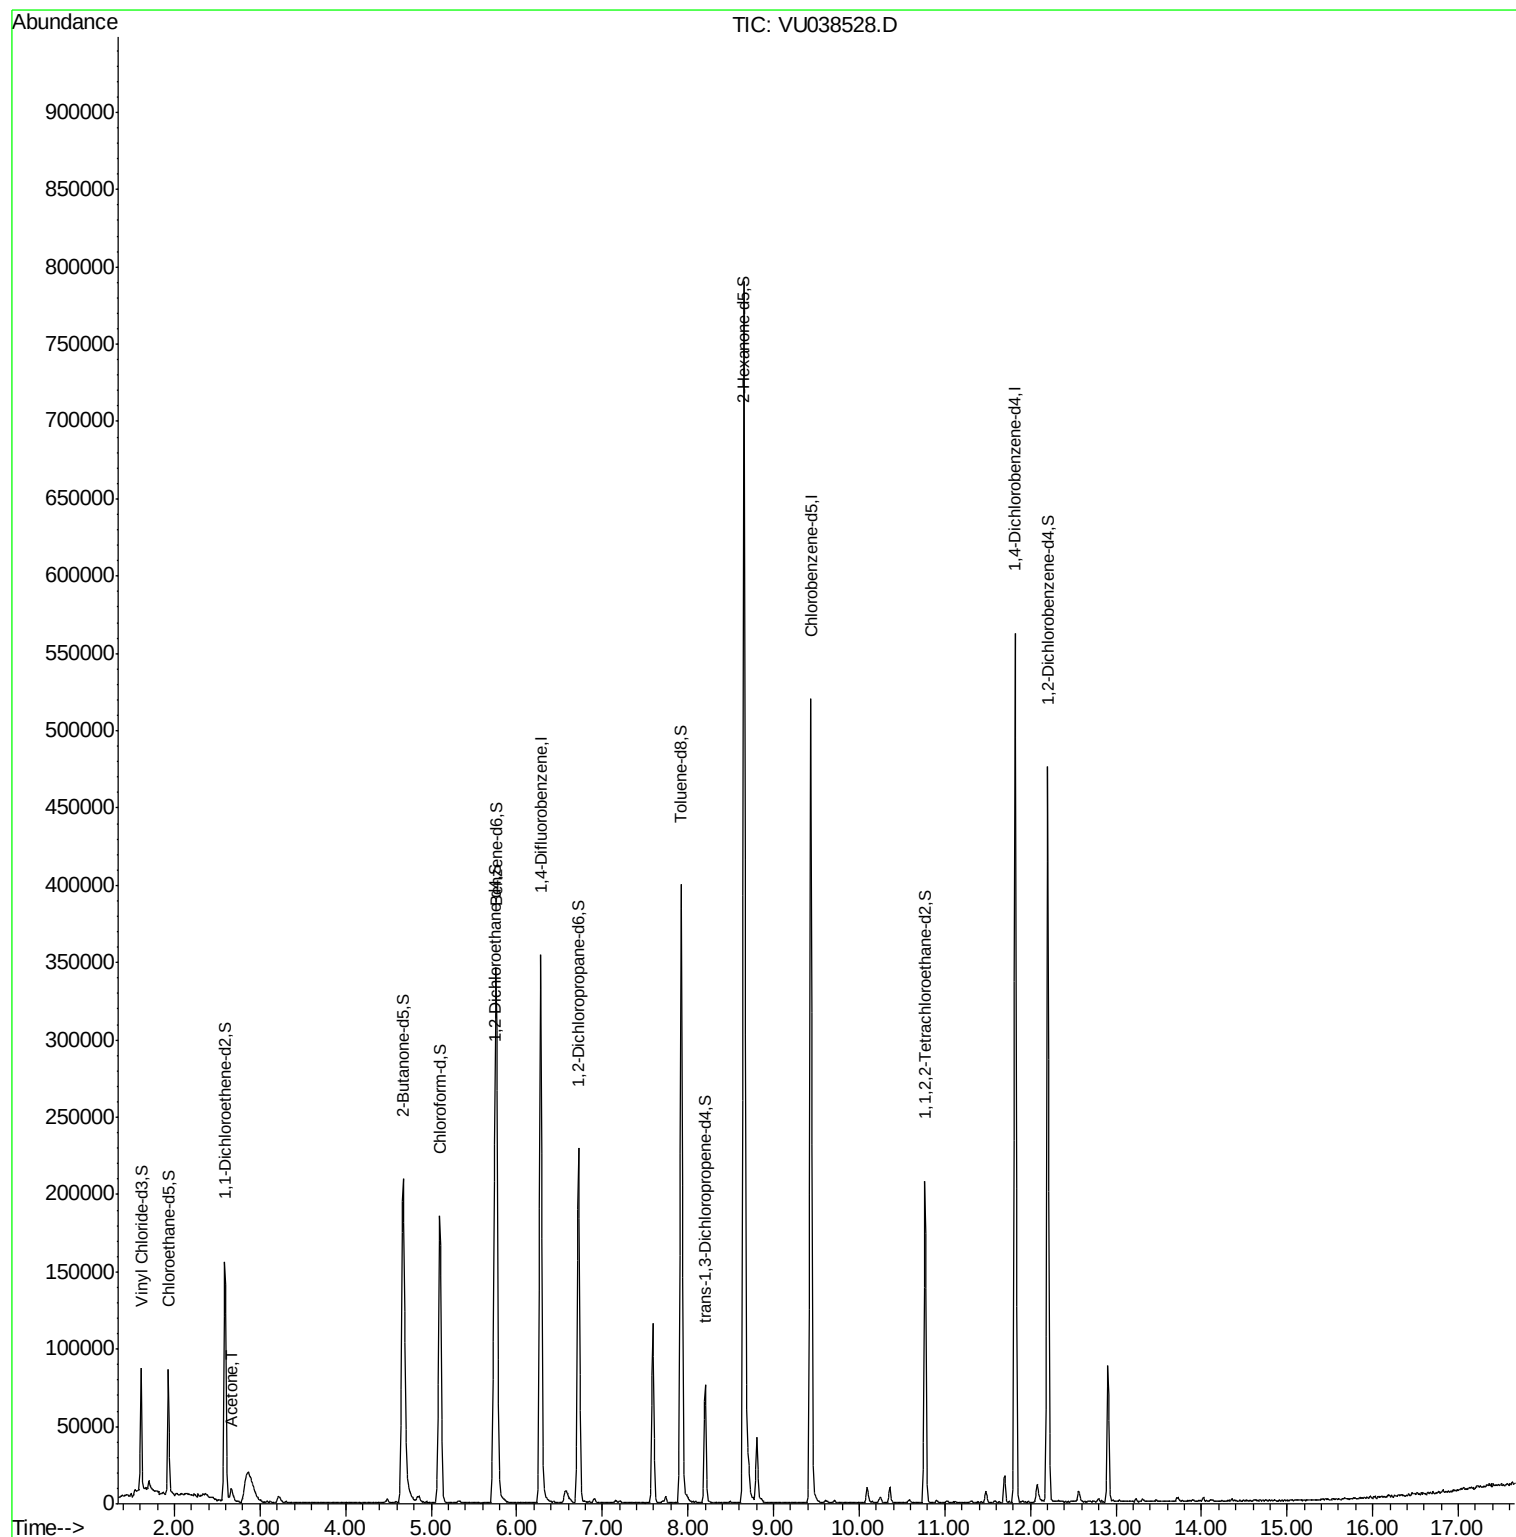

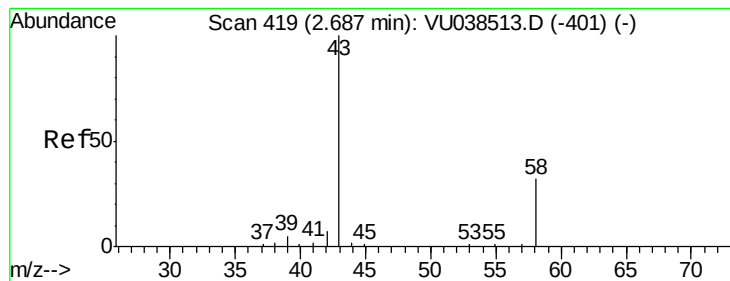

#13

Acetone

Concen: 3.288 ug/L

RT: 2.67 min Scan# 412

Delta R.T. -0.02 min

Lab File: VU038528.D

Acq: 03 Jun 2020 20:54

Instrument :
MSVOA_U
ClientSampleId :
C0AG1

Tot Ion: 43 Resp: 12534

Ion Ratio Lower Upper

43 100

58 33.7 0.0 65.6

