

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU060420\
 Data File : VU038530.D
 Acq On : 03 Jun 2020 21:40
 Operator : SY/MD
 Sample : L2844-22
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AG3

Quant Time: Jun 04 04:43:05 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR053120WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Jun 04 01:48:03 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.28	114	295906	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.44	117	292616	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.82	152	141020	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.61	65	54678	2.86	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	57.20%
7) Chloroethane-d5	1.93	69	58514	3.98	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	79.60%
11) 1,1-Dichloroethene-d2	2.59	63	98833	2.62	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	52.40%#
20) 2-Butanone-d5	4.67	46	346705	59.59	ug/L	-0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	119.18%
24) Chloroform-d	5.10	84	175100	4.87	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.40%
26) 1,2-Dichloroethane-d4	5.74	65	107886	5.28	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	105.60%
32) Benzene-d6	5.76	84	339859	4.65	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.00%
36) 1,2-Dichloropropane-d6	6.72	67	110540	4.92	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	98.40%
41) Toluene-d8	7.92	98	273887	4.18	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	83.60%
43) trans-1,3-Dichloropropene-	8.20	79	43384	4.49	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	89.80%
46) 2-Hexanone-d5	8.65	63	299278	62.73	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	125.46%
57) 1,1,2,2-Tetrachloroethane-	10.77	84	101731	5.33	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	106.60%
64) 1,2-Dichlorobenzene-d4	12.20	152	122866	5.05	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	101.00%


Target Compounds					Ovalue
13) Acetone	2.68	43	14231	3.738 ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU060420\
Data File : VU038530.D
Acq On : 03 Jun 2020 21:40
Operator : SY/MD
Sample : L2844-22
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AG3

Quant Time: Jun 04 04:43:05 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR053120WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Jun 04 01:48:03 2020
Response via : Initial Calibration

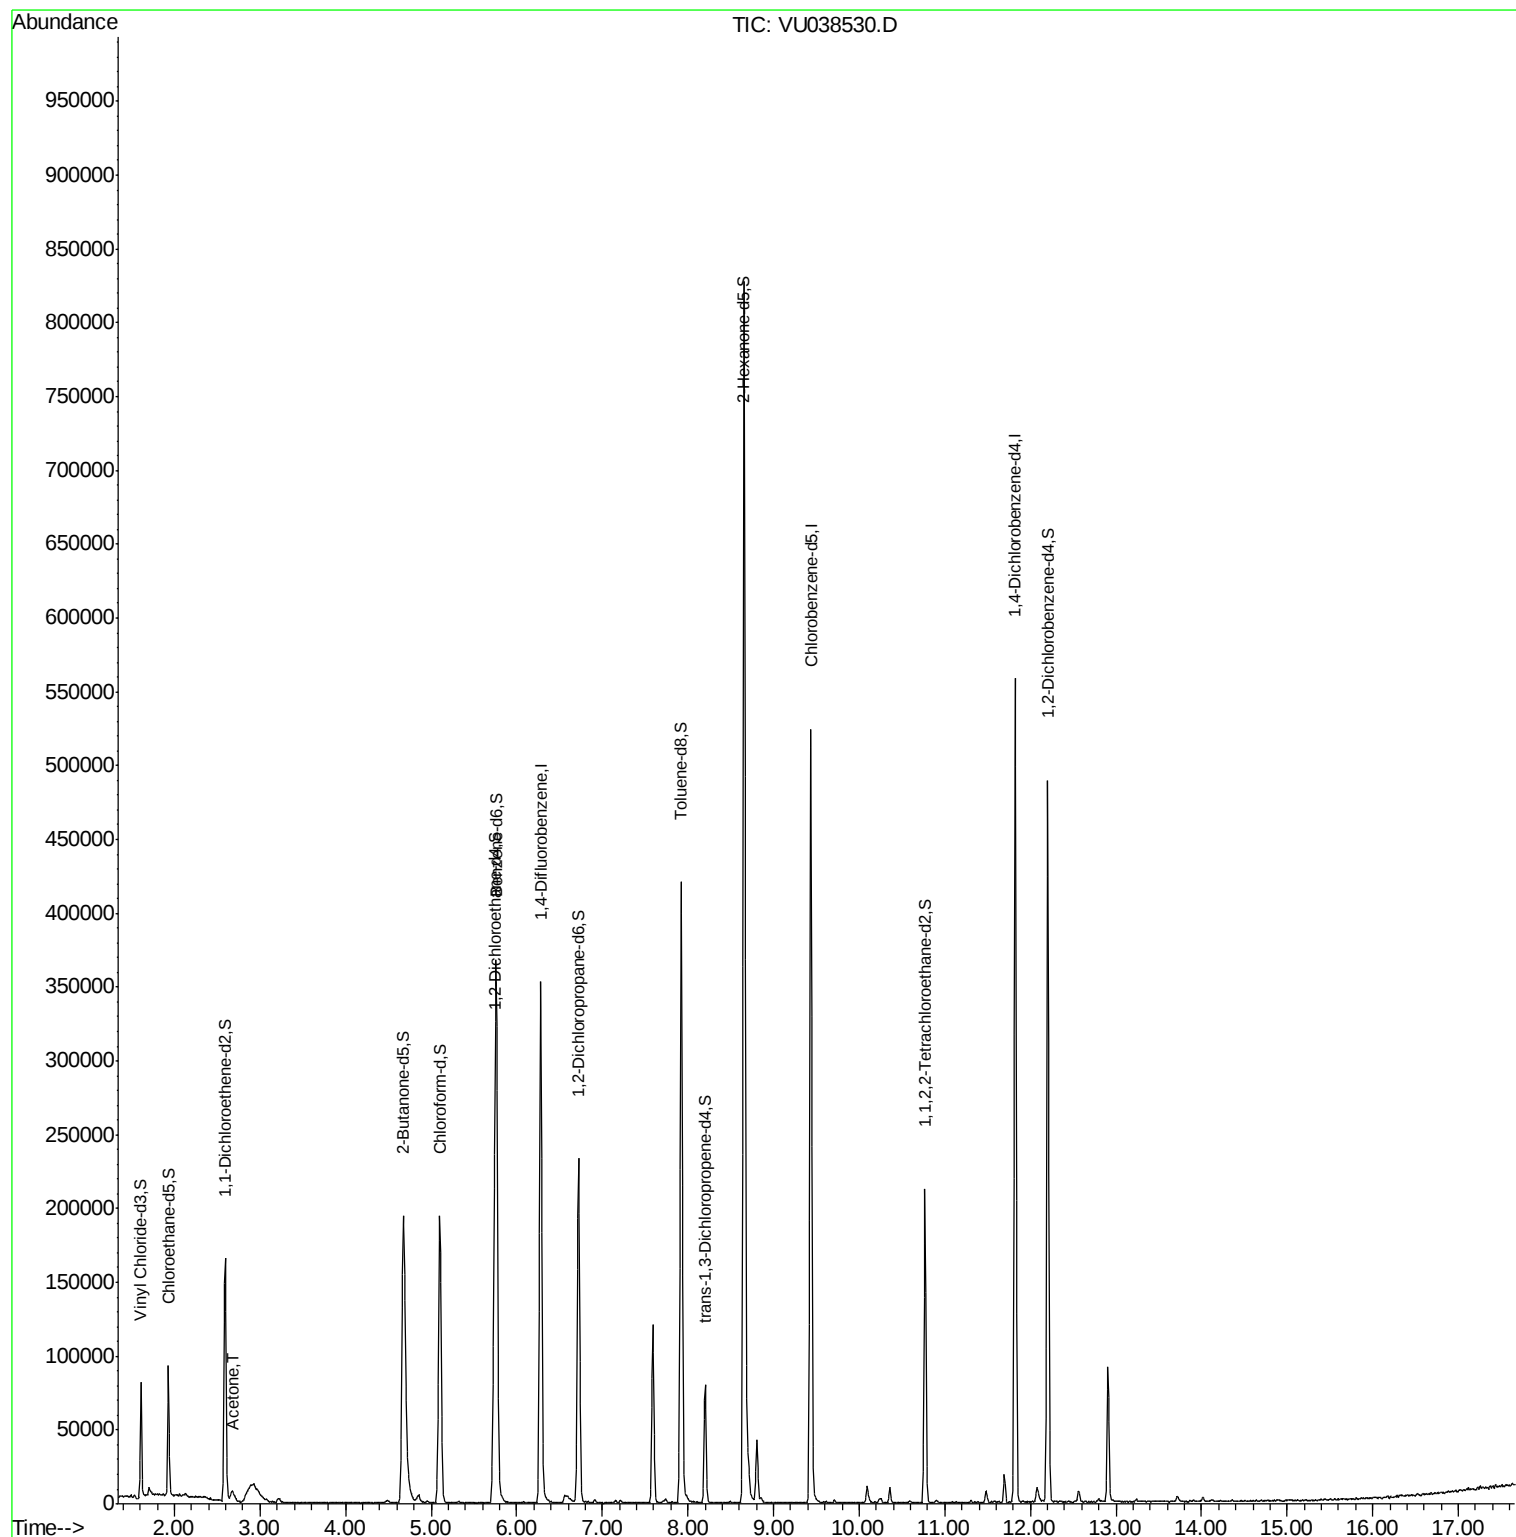

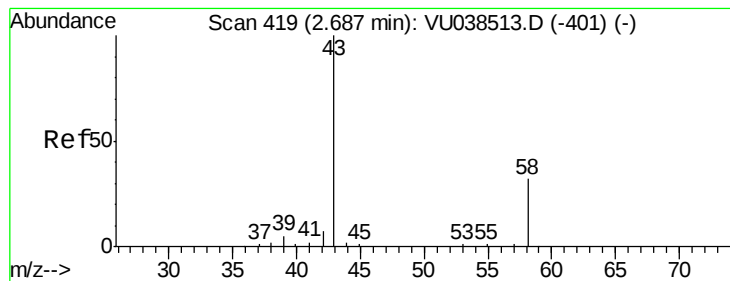

#13
 Acetone
 Concen: 3.738 ug/L
 RT: 2.68 min Scan# 416
 Delta R.T. -0.01 min
 Lab File: VU038530.D
 Acq: 03 Jun 2020 21:40

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AG3

Tot Ion: 43 Resp: 14231
 Ion Ratio Lower Upper
 43 100
 58 31.6 0.0 65.6

