

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU060420\
 Data File : VU038544.D
 Acq On : 04 Jun 2020 13:18
 Operator : SY/MD
 Sample : L2662-21
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK01

Quant Time: Jun 05 01:58:21 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR053120WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Jun 05 01:11:12 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.28	114	301781	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.44	117	292246	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.83	152	137501	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.61	65	109103	5.59	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	111.80%
7) Chloroethane-d5	1.93	69	85647	5.71	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	114.20%
11) 1,1-Dichloroethene-d2	2.59	63	169765	4.42	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	88.40%
20) 2-Butanone-d5	4.68	46	339193	57.17	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	114.34%
24) Chloroform-d	5.10	84	203217	5.54	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	110.80%
26) 1,2-Dichloroethane-d4	5.74	65	119350	5.73	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	114.60%
32) Benzene-d6	5.76	84	426022	5.84	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	116.80%
36) 1,2-Dichloropropane-d6	6.72	67	126294	5.63	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	112.60%
41) Toluene-d8	7.92	98	365243	5.58	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	111.60%
43) trans-1,3-Dichloropropene-	8.20	79	51962	5.38	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	107.60%
46) 2-Hexanone-d5	8.66	63	284659	59.74	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	119.48%
57) 1,1,2,2-Tetrachloroethane-	10.77	84	105332	5.53	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	110.60%
64) 1,2-Dichlorobenzene-d4	12.20	152	142110	5.99	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	119.80%


Target Compounds					Ovalue
16) Methylene chloride	3.08	84	2027	0.096 ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU060420\
Data File : VU038544.D
Acq On : 04 Jun 2020 13:18
Operator : SY/MD
Sample : L2662-21
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK01

Quant Time: Jun 05 01:58:21 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR053120WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Jun 05 01:11:12 2020
Response via : Initial Calibration

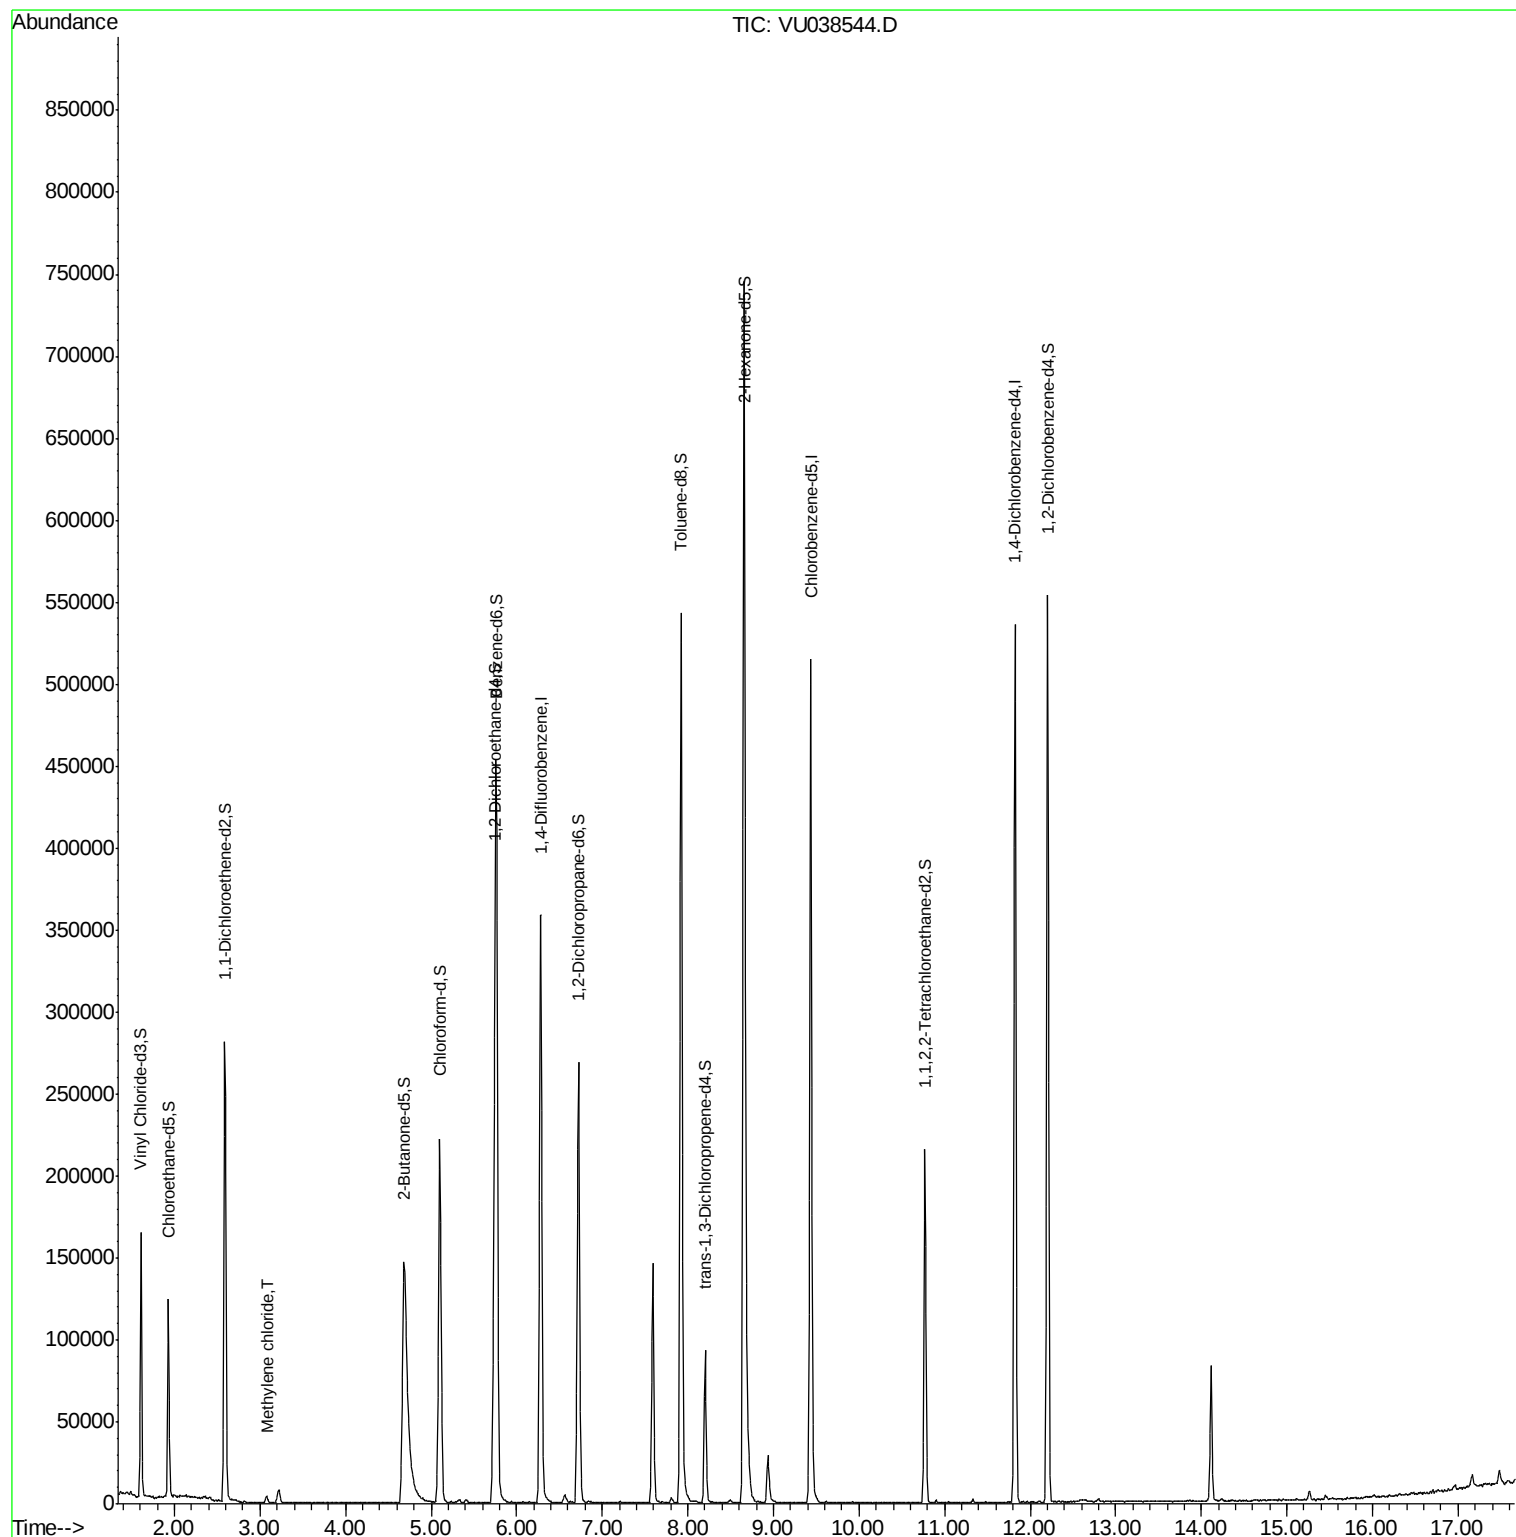

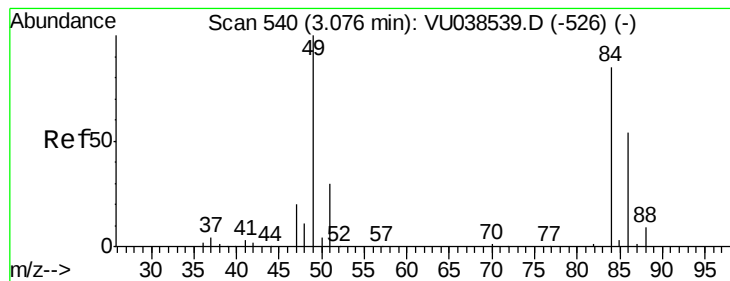

#16
 Methvlene chloride
 Concen: 0.096 ug/L
 RT: 3.08 min Scan# 540
 Delta R.T. -0.00 min
 Lab File: VU038544.D
 Acq: 04 Jun 2020 13:18

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK01

Tot Ion: 84 Resp: 2027
 Ion Ratio Lower Upper
 84 100
 86 56.3 45.0 83.6
 49 123.0 85.5 158.9

