


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU060420\
 Data File : VU038512.D
 Acq On : 03 Jun 2020 13:34
 Operator : JC/MD
 Sample : BFB06
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB06

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR053120WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Thu Jun 04 03:42:25 2020

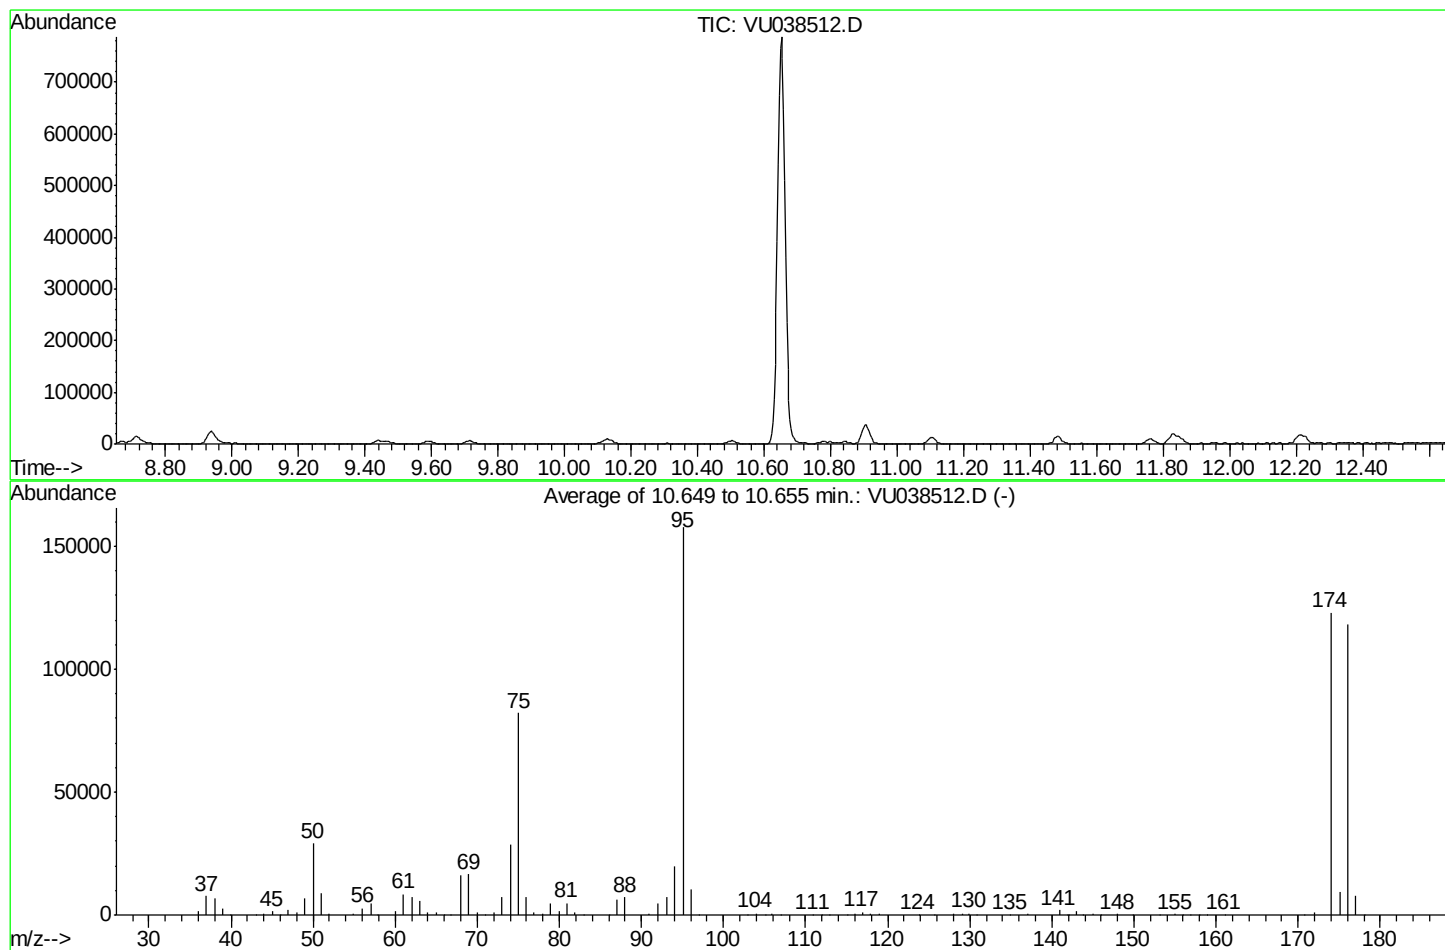

AutoFind: Scans 2895, 2896, 2897; Background Corrected with Scan 2881

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.5	29157	PASS
75	95	30	80	52.2	82264	PASS
95	95	100	100	100.0	157738	PASS
96	95	5	9	6.5	10280	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	78.1	123170	PASS
175	174	5	9	7.7	9439	PASS
176	174	95	101	96.1	118346	PASS
177	176	5	9	6.5	7639	PASS

m/z	Abundance
36.10	1506.0
37.00	7837.0
38.00	7119.0
39.00	3009.0
39.80	401.0
44.00	1446.0
45.00	1496.0
46.00	157.0
47.00	2066.0
48.00	1008.0
49.00	6842.0
50.00	30216.0
51.00	8718.0
51.90	329.0
55.00	398.0
56.00	2666.0
57.00	5078.0
57.90	105.0
60.00	1388.0
61.00	8322.0
62.00	7617.0
63.10	5895.0
64.00	1015.0
65.00	832.0
66.00	166.0
66.80	281.0
68.00	16424.0
69.00	16480.0
70.00	1128.0
71.00	110.0
72.00	1177.0
73.00	7449.0
74.00	28944.0
75.00	82592.0
76.00	7581.0
77.00	860.0
78.00	546.0
78.90	4832.0
80.00	1615.0
80.90	4982.0
81.90	1314.0
82.90	232.0
86.00	241.0
87.00	6841.0
87.90	6905.0
90.90	659.0
92.00	4445.0
93.00	7203.0
94.10	19976.0
95.10	158272.0
96.10	10203.0
97.00	292.0
102.90	116.0
104.00	713.0
105.00	250.0
105.90	638.0
107.00	121.0
110.90	150.0
111.90	102.0
112.90	134.0
115.00	208.0
115.90	565.0
116.90	1107.0
117.90	677.0
118.90	780.0
123.80	156.0
128.00	494.0
129.00	372.0
130.00	531.0
130.90	247.0
135.00	256.0
137.00	263.0
140.90	1858.0
142.00	198.0
143.00	1780.0
143.80	180.0
145.10	312.0
145.90	246.0
148.00	440.0
149.80	109.0
153.10	126.0
155.00	366.0
155.90	116.0
156.90	194.0
158.80	131.0
161.10	163.0
170.70	123.0
172.10	1002.0
174.00	120280.0
175.10	9173.0
176.00	115696.0
177.00	7581.0

Instrument :
MSVOA_U
ClientSampleId :
BFB06

178.10

191.0

Instrument :
MSVOA_U
ClientSampleId :
BFB06

m/z	Abundance
36.10	1526.0
37.00	7911.0
38.00	6884.0
39.00	2880.0
39.80	381.0
43.00	116.0
43.90	1501.0
45.00	1567.0
46.00	214.0
47.00	2070.0
48.00	983.0
49.00	6757.0
50.00	29912.0
51.00	8912.0
52.00	319.0
55.00	410.0
56.00	2870.0
57.00	4987.0
57.90	100.0
60.00	1519.0
61.00	8567.0
62.00	7530.0
63.10	6150.0
64.00	1016.0
64.90	862.0
66.00	165.0
66.80	276.0
68.00	16832.0
69.00	16792.0
70.00	1158.0
72.00	1144.0
73.00	7216.0
74.00	29248.0
75.10	84736.0
76.00	7415.0
77.00	939.0
78.90	4969.0
80.00	1558.0
80.90	4970.0
81.90	1272.0
82.90	198.0
86.00	226.0
87.00	6544.0
88.00	7422.0
91.00	576.0
92.00	4646.0
93.10	7343.0
94.10	20328.0
95.10	162176.0
96.10	10638.0
96.90	289.0
102.90	114.0
104.00	702.0
105.00	247.0
105.90	698.0
106.90	104.0
110.90	126.0
112.90	140.0
115.00	200.0
116.00	542.0
117.00	1144.0
118.00	648.0
118.90	836.0
123.80	170.0
127.90	425.0
129.10	347.0
129.90	558.0
130.90	279.0
135.00	288.0
137.00	357.0
140.90	2031.0
141.80	179.0
143.00	1879.0
143.80	178.0
145.00	308.0
145.90	257.0
148.10	479.0
149.80	110.0
153.10	148.0
155.00	380.0
156.90	248.0
158.00	102.0
158.90	144.0
161.00	155.0
172.00	1127.0
174.00	127120.0
175.10	9732.0
176.00	122008.0
177.00	7845.0
178.10	173.0

Instrument :
MSVOA_U
ClientSampleId :
BFB06

m/z	Abundance
36.00	1464.0
37.00	7156.0
38.00	6107.0
39.00	2622.0
39.90	300.0
43.00	121.0
43.90	1559.0
45.00	1485.0
46.00	191.0
47.00	1849.0
48.00	945.0
49.00	6272.0
50.00	27344.0
51.00	8700.0
52.00	290.0
54.90	425.0
56.00	2751.0
57.00	4415.0
60.10	1475.0
61.00	8164.0
62.00	7045.0
63.00	5853.0
64.00	835.0
64.90	902.0
65.90	126.0
68.00	16005.0
69.00	16056.0
70.00	1227.0
72.00	953.0
73.00	6659.0
74.00	27528.0
75.10	79464.0
76.00	6881.0
76.90	977.0
78.00	502.0
78.90	4646.0
80.00	1432.0
80.90	4741.0
81.90	1120.0
82.90	179.0
87.00	6170.0
88.00	7361.0
91.00	520.0
92.00	4607.0
93.10	6796.0
94.10	19120.0
95.10	152768.0
96.10	10000.0
96.90	245.0
103.90	646.0
105.10	227.0
105.90	710.0
106.90	138.0
112.90	109.0
115.00	165.0
116.00	482.0
117.00	1040.0
118.00	541.0
118.90	780.0
123.80	105.0
125.70	100.0
128.10	338.0
129.10	275.0
129.90	537.0
130.90	280.0
134.90	276.0
137.00	405.0
140.90	1977.0
142.10	166.0
143.00	1736.0
143.80	143.0
144.90	241.0
145.90	250.0
148.10	462.0
153.00	121.0
155.00	341.0
156.90	241.0
158.00	120.0
158.90	166.0
161.00	162.0
172.00	1059.0
174.00	122112.0
175.10	9413.0
176.00	117336.0
177.00	7493.0
177.90	201.0

Instrument :
MSVOA_U
ClientSampleId :
BFB06

Scan 2881 (10.604 min): VU038512.D
BFB06

m/z	Abundance
39.90	284.0
44.00	744.0

Instrument :
MSVOA_U
ClientSampleId :
BFB06