


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU060420\
 Data File : VU038538.D
 Acq On : 04 Jun 2020 08:34
 Operator : SY/MD
 Sample : BFB07
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB07

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR053120WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Fri Jun 05 13:35:40 2020

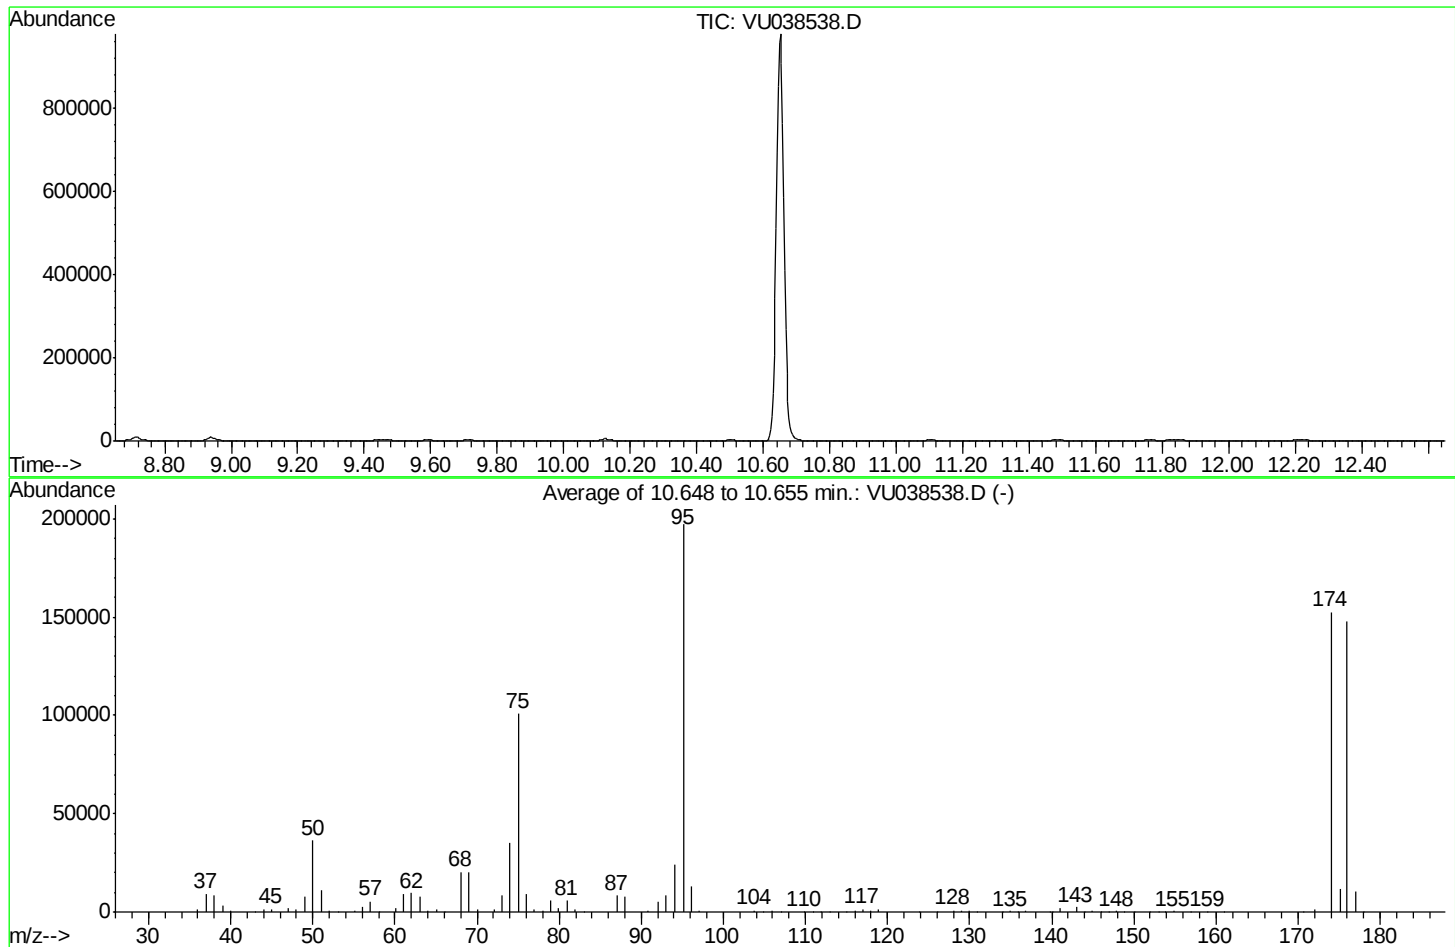

AutoFind: Scans 2895, 2896, 2897; Background Corrected with Scan 2880

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.5	36394	PASS
75	95	30	80	51.1	100821	PASS
95	95	100	100	100.0	197162	PASS
96	95	5	9	6.5	12798	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	77.3	152341	PASS
175	174	5	9	7.6	11647	PASS
176	174	95	101	97.1	147904	PASS
177	176	5	9	6.9	10217	PASS

m/z	Abundance
36.00	1477.0
37.00	9724.0
38.00	8184.0
39.10	3327.0
40.10	351.0
42.90	106.0
44.00	1880.0
44.90	1472.0
46.90	2345.0
47.90	1353.0
49.00	8253.0
50.00	36904.0
51.00	11581.0
52.10	598.0
53.00	224.0
55.10	610.0
56.00	2956.0
57.00	5706.0
58.00	222.0
60.00	1912.0
61.00	9501.0
62.00	9750.0
63.00	8198.0
64.00	1010.0
65.00	1195.0
66.00	125.0
68.00	20904.0
69.00	20976.0
70.10	1593.0
72.00	1239.0
73.00	8655.0
74.00	34464.0
75.00	103008.0
76.00	9488.0
77.00	938.0
78.00	806.0
78.90	6034.0
79.90	1908.0
81.00	6077.0
81.90	1468.0
83.00	120.0
87.00	8326.0
88.00	8158.0
90.90	698.0
92.00	5653.0
93.10	8808.0
94.10	24312.0
95.10	200448.0
96.10	13130.0
97.00	455.0
103.80	837.0
104.80	244.0
106.00	752.0
107.10	136.0
109.90	215.0
110.90	194.0
111.90	100.0
112.90	245.0
115.00	162.0
116.00	737.0
117.00	1528.0
118.00	745.0
118.90	1260.0
123.90	104.0
128.00	806.0
128.90	364.0
130.00	638.0
130.90	281.0
134.00	166.0
135.00	407.0
135.90	108.0
136.80	427.0
139.70	116.0
141.00	2052.0
143.00	2566.0
143.90	131.0
144.90	431.0
145.90	276.0
146.90	136.0
148.00	439.0
150.00	137.0
152.00	129.0
153.00	117.0
153.80	132.0
154.90	482.0
157.00	294.0
159.00	196.0
160.90	174.0
170.70	131.0
172.10	1379.0
174.00	152000.0
175.10	11822.0

Instrument :
MSVOA_U
ClientSampleId :
BFB07

176.00

177.00

177.90

146432.0

10136.0

279.0

Instrument :

MSVOA_U

ClientSampleId :

BFB07

m/z	Abundance
35.90	1486.0
37.00	9478.0
38.00	8523.0
39.10	3265.0
40.00	389.0
44.00	1944.0
45.00	1379.0
47.00	2255.0
47.90	1475.0
49.00	8383.0
50.00	37664.0
51.00	11559.0
52.00	597.0
53.00	187.0
55.00	628.0
56.00	2803.0
57.00	5530.0
58.00	251.0
60.00	1854.0
61.00	9716.0
62.00	9914.0
63.00	8265.0
64.00	1042.0
65.00	1112.0
68.00	21096.0
69.00	20952.0
70.10	1592.0
72.00	1150.0
73.10	8928.0
74.00	36208.0
75.00	103808.0
76.00	9559.0
77.00	1060.0
78.10	1014.0
79.00	6035.0
79.90	1950.0
80.90	5957.0
81.90	1531.0
83.10	182.0
87.00	8915.0
88.00	8194.0
90.80	718.0
92.00	5557.0
93.10	8909.0
94.10	24816.0
95.10	203584.0
96.10	13231.0
97.00	413.0
103.80	844.0
104.80	242.0
105.90	738.0
107.00	109.0
109.90	217.0
110.90	211.0
112.90	276.0
115.00	223.0
116.00	715.0
117.00	1595.0
117.90	857.0
118.90	1213.0
123.90	116.0
128.00	818.0
129.00	375.0
129.90	663.0
131.00	351.0
134.00	134.0
135.00	397.0
135.90	102.0
136.80	359.0
140.00	103.0
141.00	2056.0
143.00	2451.0
143.90	149.0
144.90	399.0
146.00	289.0
146.90	153.0
148.00	428.0
150.00	171.0
152.00	141.0
153.00	135.0
153.80	185.0
154.90	442.0
157.00	355.0
159.00	246.0
160.90	188.0
170.70	188.0
172.10	1488.0
174.00	157056.0
175.10	12121.0
176.00	152512.0
177.00	10633.0
178.00	279.0

Instrument :
MSVOA_U
ClientSampleId :
BFB07

m/z	Abundance
35.90	1415.0
37.00	8405.0
38.00	7953.0
39.10	2832.0
40.00	405.0
44.00	1817.0
45.00	1271.0
47.10	2080.0
47.90	1311.0
49.00	7540.0
50.00	34616.0
51.00	10383.0
52.00	488.0
53.00	122.0
55.00	517.0
56.00	2456.0
57.00	4867.0
58.10	239.0
60.10	1728.0
61.00	9018.0
62.00	9059.0
63.00	7174.0
64.00	903.0
65.10	1015.0
66.00	111.0
68.00	19288.0
69.00	19248.0
70.10	1376.0
72.10	980.0
73.10	8386.0
74.00	34184.0
75.00	95648.0
76.00	8500.0
77.00	1088.0
78.00	1008.0
79.00	5483.0
79.90	1764.0
80.90	5467.0
82.00	1371.0
83.10	224.0
87.00	8132.0
88.00	7613.0
90.90	658.0
92.00	5230.0
93.00	8049.0
94.10	22880.0
95.10	187456.0
96.10	12033.0
97.10	346.0
103.80	790.0
104.80	199.0
105.80	736.0
107.00	112.0
109.90	174.0
110.90	198.0
112.90	282.0
114.90	248.0
116.10	630.0
117.00	1440.0
117.90	880.0
118.90	1000.0
123.90	141.0
126.10	115.0
128.00	765.0
129.00	343.0
129.90	652.0
131.00	387.0
135.00	315.0
136.90	308.0
140.00	128.0
141.00	1982.0
143.00	2050.0
143.90	138.0
144.90	401.0
145.90	278.0
147.00	140.0
147.90	402.0
148.80	114.0
150.00	158.0
152.00	129.0
152.90	133.0
153.80	170.0
154.80	393.0
156.90	341.0
159.00	290.0
160.90	200.0
170.70	181.0
172.10	1382.0
174.00	147968.0
175.10	10998.0
176.00	144768.0
177.00	9883.0

Instrument :
MSVOA_U
ClientSampleId :
BFB07

178.00

249.0

Instrument :
MSVOA_U
ClientSampleId :
BFB07

Scan 2880 (10.600 min): VU038538.D
BFB07

m/z	Abundance
39.80	231.0
44.00	666.0

Instrument :
MSVOA_U
ClientSampleId :
BFB07