

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060421\
 Data File : VU044045.D
 Acq On : 04 Jun 2021 11:21
 Operator : SY/MD
 Sample : VU0604WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0604WBL01

Quant Time: Jun 07 02:16:04 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U060221DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Thu Jun 03 11:17:14 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Fluorobenzene	6.124	96	14564	1.000	ug/l	# 0.00
System Monitoring Compounds						
57) 4-Bromofluorobenzene	10.642	95	3821	0.755	ug/l	0.00
Spiked Amount 1.000			Recovery	=	75.000%	
68) 1,2-Dichlorobenzene-d4	12.201	152	3851	0.713	ug/l	0.00
Spiked Amount 1.000			Recovery	=	71.000%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060421\
Data File : VU044045.D
Acq On : 04 Jun 2021 11:21
Operator : SY/MD
Sample : VU0604WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0604WBL01

Quant Time: Jun 07 02:16:04 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U060221DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Thu Jun 03 11:17:14 2021
Response via : Initial Calibration

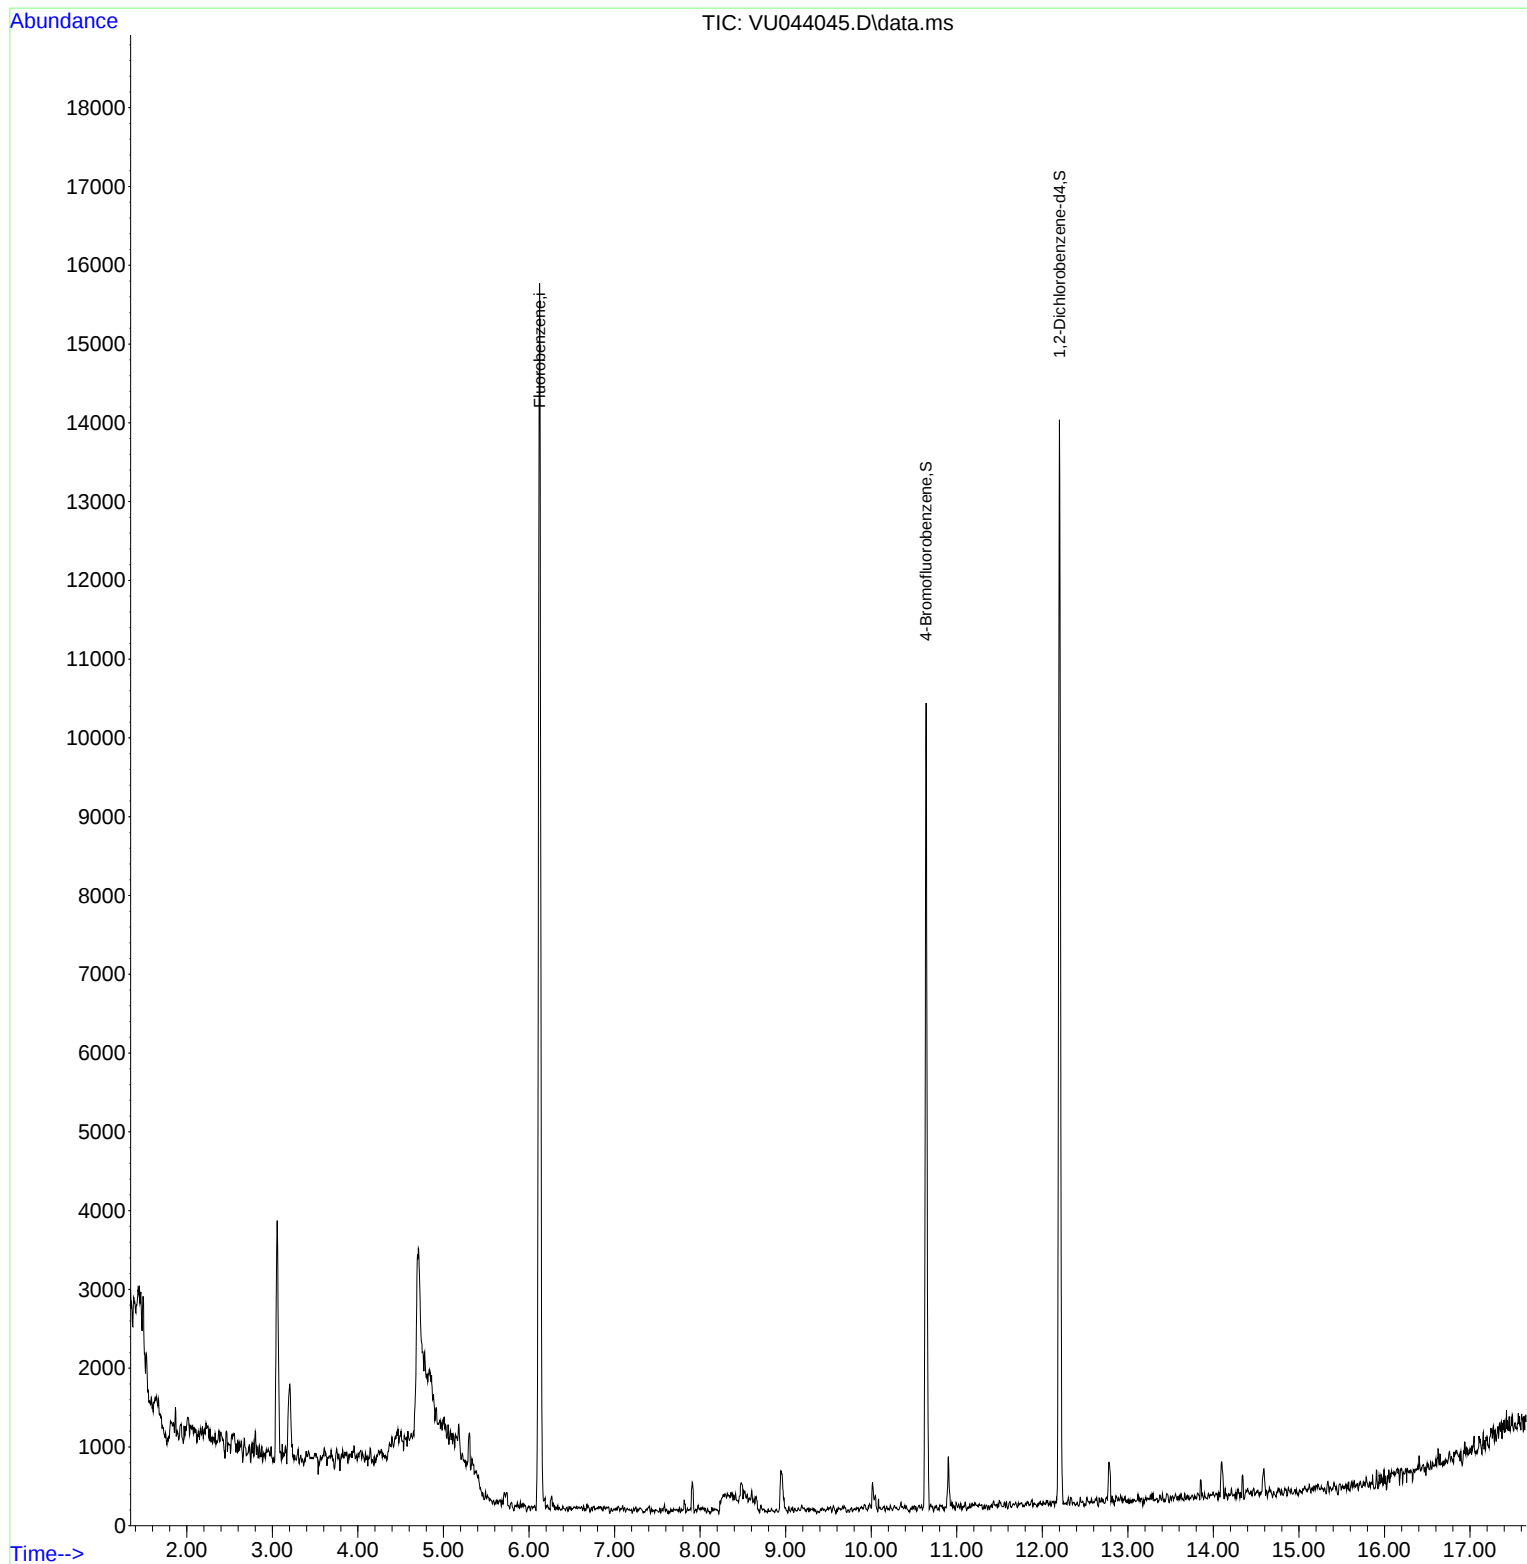




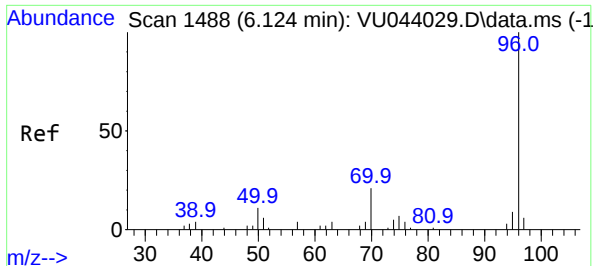


#1
Fluorobenzene
Concen: 1.000 ug/l
RT: 6.124 min Scan# 1488
Delta R.T. 0.000 min
Lab File: VU044045.D
Acq: 04 Jun 2021 11:21

Instrument :
MSVOA_U
ClientSampleId :
VU0604WBL01

Tgt Ion: 96 Resp: 14564




Ion	Ratio	Lower	Upper
96	100		
70	20.2	16.6	25.0
95	8.6	7.0	10.4
97	5.8	0.0	0.0#

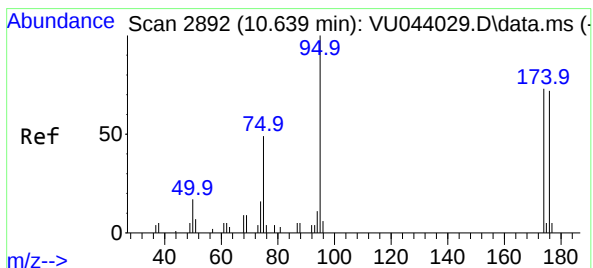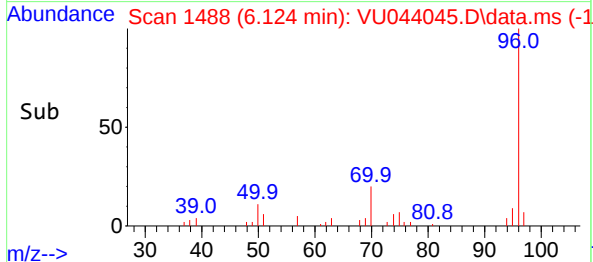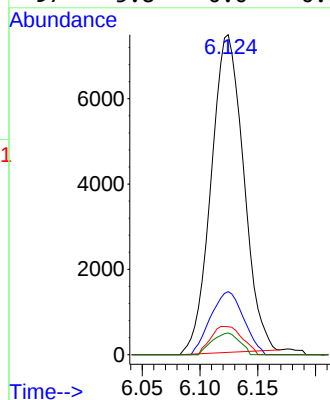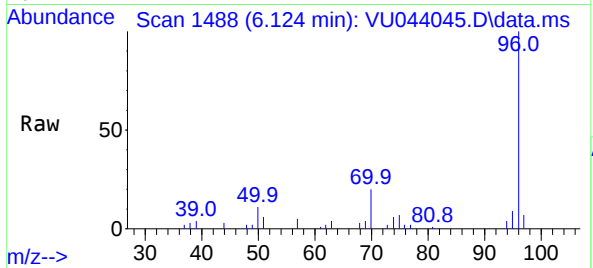


#57
4-Bromofluorobenzene
Concen: 0.755 ug/l
RT: 10.642 min Scan# 2893
Delta R.T. 0.003 min
Lab File: VU044045.D
Acq: 04 Jun 2021 11:21

Tgt Ion: 95 Resp: 3821

Ion	Ratio	Lower	Upper
95	100		
174	74.6	59.1	88.7
176	72.2	56.4	84.6

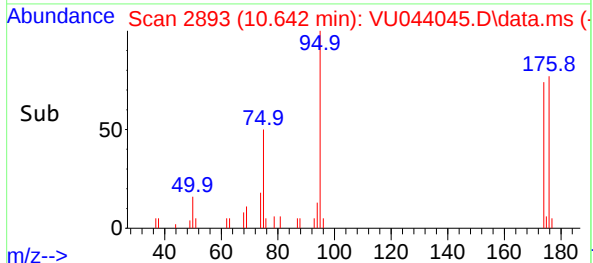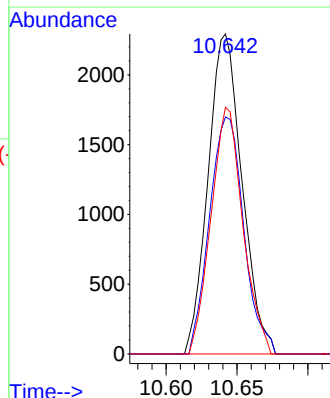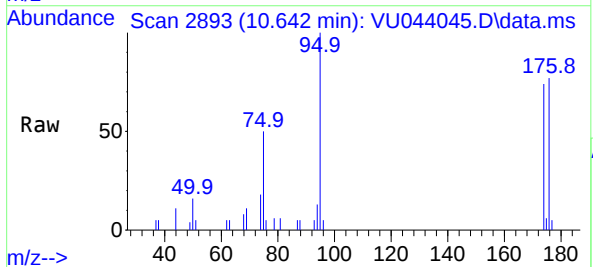

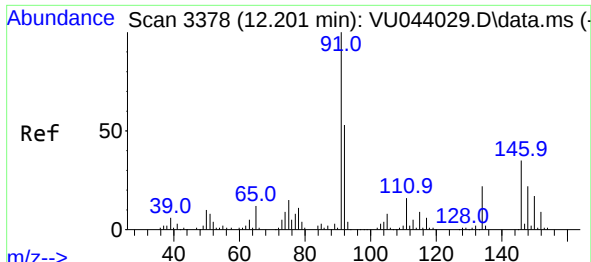

#68
 1,2-Dichlorobenzene-d4
 Concen: 0.713 ug/l
 RT: 12.201 min Scan# 3378
 Delta R.T. -0.000 min
 Lab File: VU044045.D
 Acq: 04 Jun 2021 11:21

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0604WBL01

Tgt Ion:152 Resp: 3851

Ion	Ratio	Lower	Upper
152	100		
115	69.0	0.0	320.6
150	172.5	0.0	687.2

