

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060421\
 Data File : VU044045.D
 Acq On : 04 Jun 2021 11:21
 Operator : SY/MD
 Sample : VU0604WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0604WBL01

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U060221DW.M
 Title : METHOD 524.2 VOLATILES DRINKING WATER

Signal : TIC: VU044045.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.462	345	349	353	rBV2	316	343	1.20%	0.418%
2	3.057	524	534	544	rBV2	3068	5540	19.31%	6.746%
3	3.205	569	580	587	rBV2	1011	2245	7.82%	2.734%
4	4.697	1031	1044	1045	rBV2	2306	3025	10.54%	3.684%
5	5.304	1227	1233	1237	rVB3	466	599	2.09%	0.729%
6	6.124	1475	1488	1503	rBV	15577	28692	100.00%	34.940%
7	7.909	2038	2043	2050	rVB2	385	533	1.86%	0.649%
8	8.481	2216	2221	2227	rVB2	210	332	1.16%	0.404%
9	8.944	2355	2365	2368	rBV3	528	674	2.35%	0.821%
10	10.015	2694	2698	2704	rBV	328	385	1.34%	0.469%
11	10.642	2883	2893	2904	rVB2	10236	14858	51.78%	18.093%
12	10.902	2966	2974	2981	rBV	644	783	2.73%	0.954%
13	12.201	3368	3378	3391	rVB2	13768	21676	75.55%	26.396%
14	12.780	3552	3558	3565	rVB2	511	808	2.82%	0.984%
15	14.095	3961	3967	3976	rVB2	470	761	2.65%	0.927%
16	14.339	4040	4043	4048	rVB2	307	297	1.04%	0.362%
17	14.590	4113	4121	4127	rVB2	346	567	1.98%	0.690%


Sum of corrected areas: 82118

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060421\
Data File : VU044045.D
Acq On : 04 Jun 2021 11:21
Operator : SY/MD
Sample : VU0604WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0604WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U060221DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

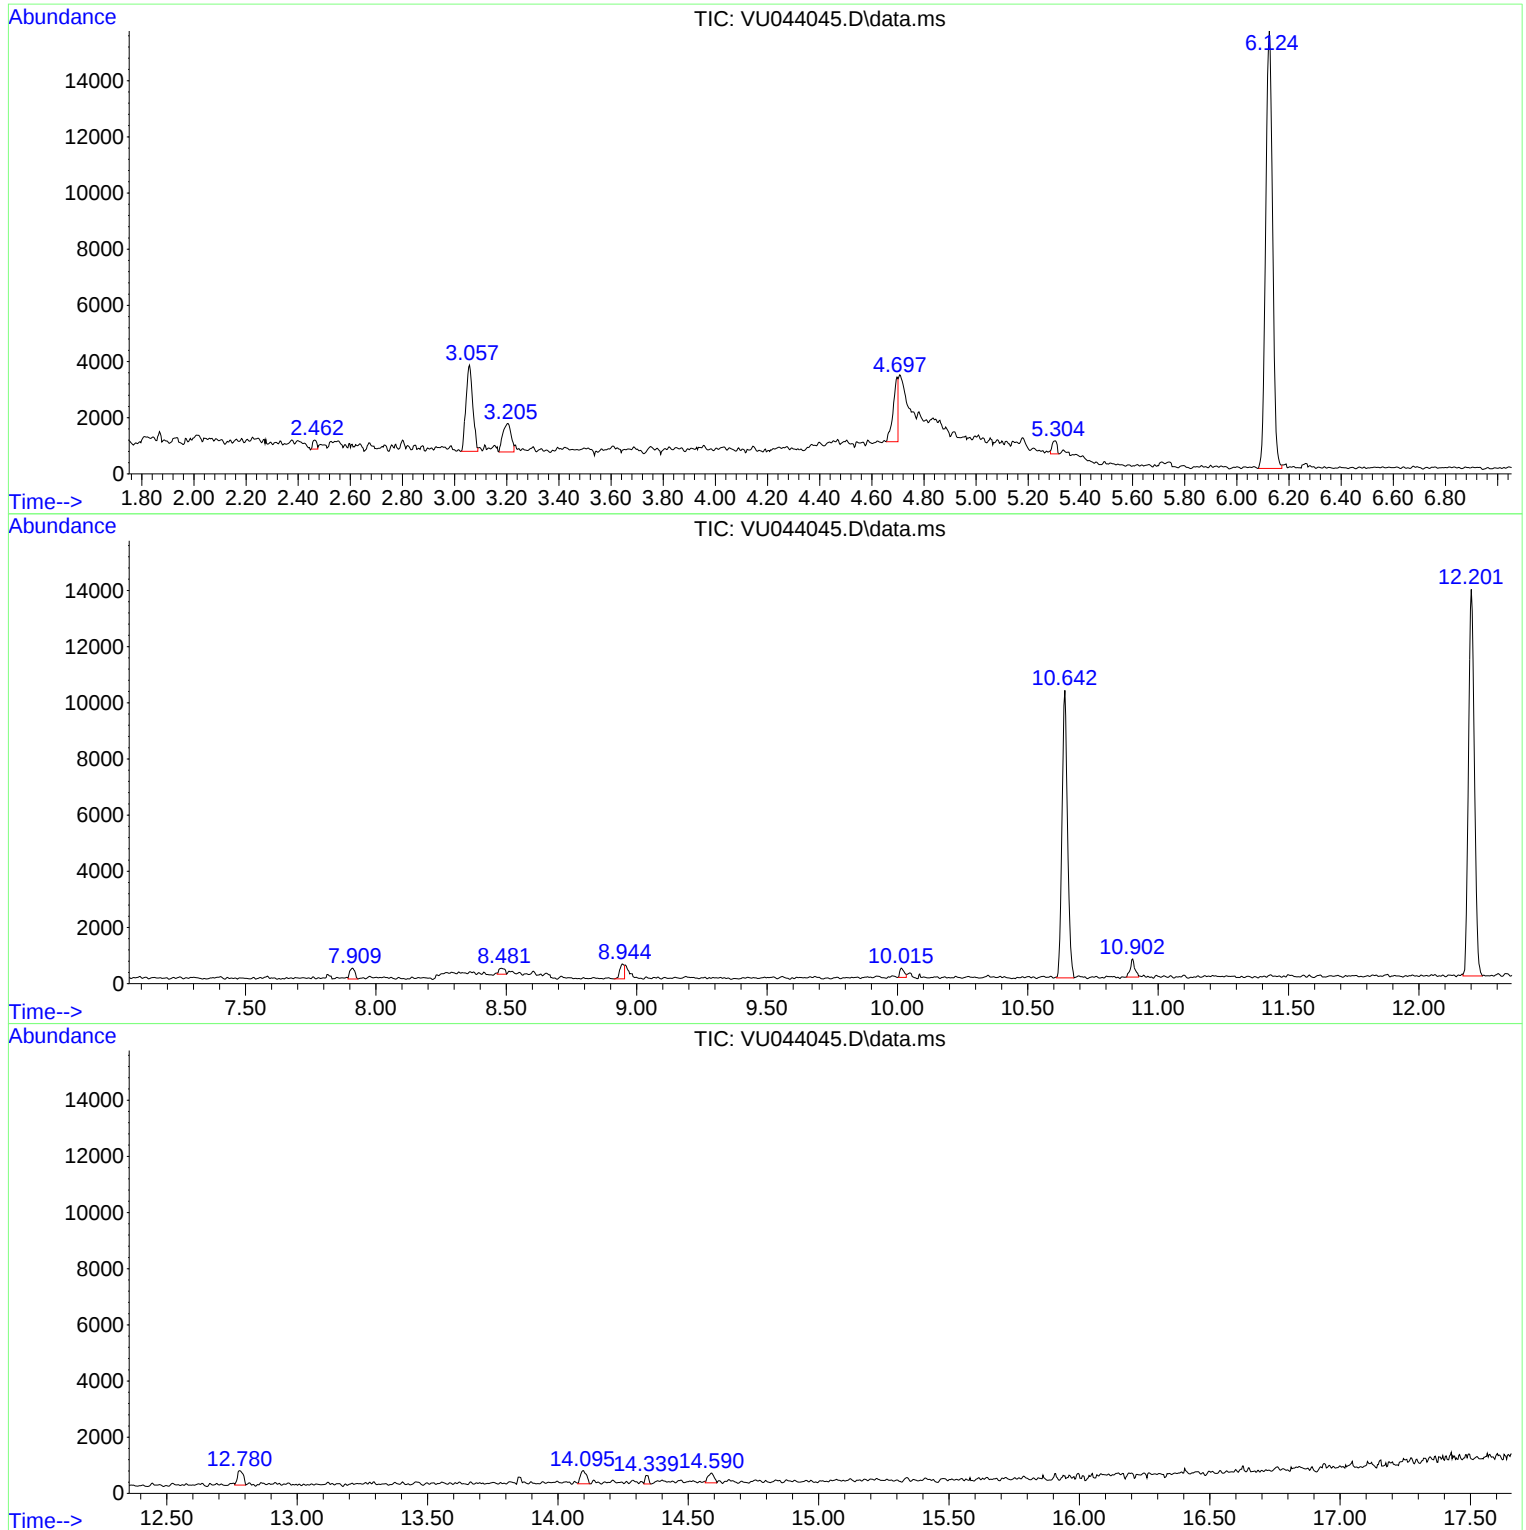

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060421\
Data File : VU044045.D
Acq On : 04 Jun 2021 11:21
Operator : SY/MD
Sample : VU0604WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0604WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U060221DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060421\
Data File : VU044045.D
Acq On : 04 Jun 2021 11:21
Operator : SY/MD
Sample : VU0604WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0604WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U060221DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------