


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060421\
Data File : VU044043.D
Acq On : 04 Jun 2021 09:43
Operator : SY/MD
Sample : BFB
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U060221DW.M
Title : METHOD 524.2 VOLATILES DRINKING WATER
Last Update : Thu Jun 03 11:17:14 2021

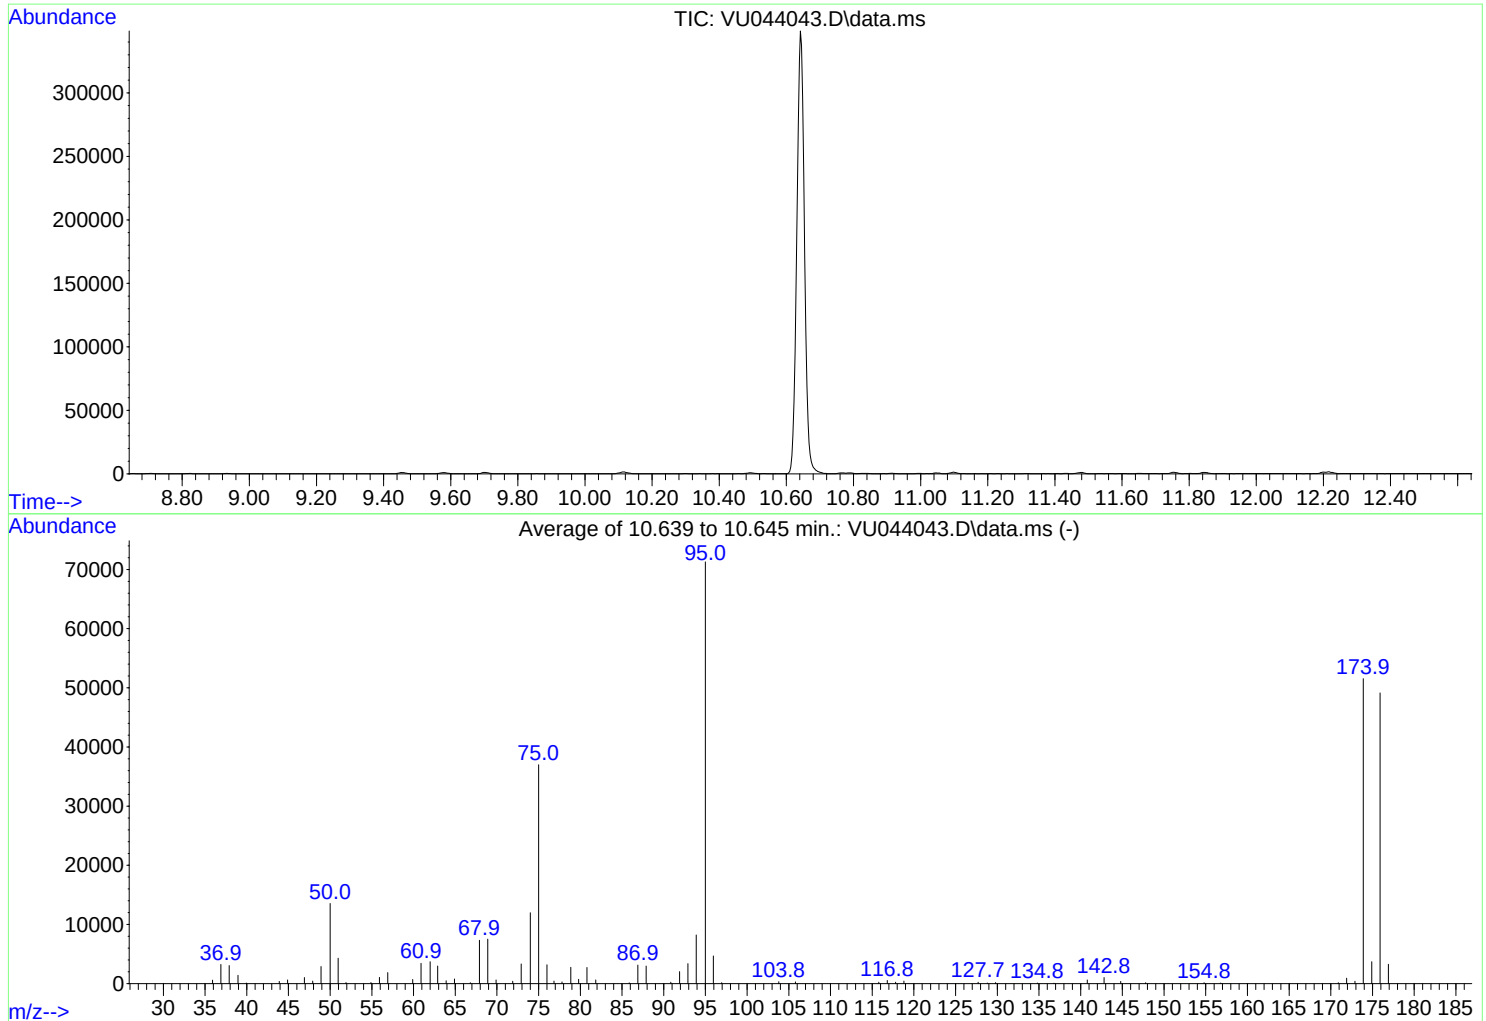

AutoFind: Scans 2892, 2893, 2894; Background Corrected with Scan 2879

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.0	13545	PASS
75	95	30	60	51.9	37003	PASS
95	95	100	100	100.0	71293	PASS
96	95	5	9	6.6	4678	PASS
173	174	0.00	2	0.8	422	PASS
174	95	50	100	72.3	51552	PASS
175	174	5	9	7.2	3704	PASS
176	174	95	101	95.3	49128	PASS
177	176	5	9	6.7	3273	PASS