


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU060519\
 Data File : VU032448.D
 Acq On : 05 Jun 2019 08:33
 Operator : JC/SP
 Sample : BFB16
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB16

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR060419WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Thu Jun 06 01:05:42 2019

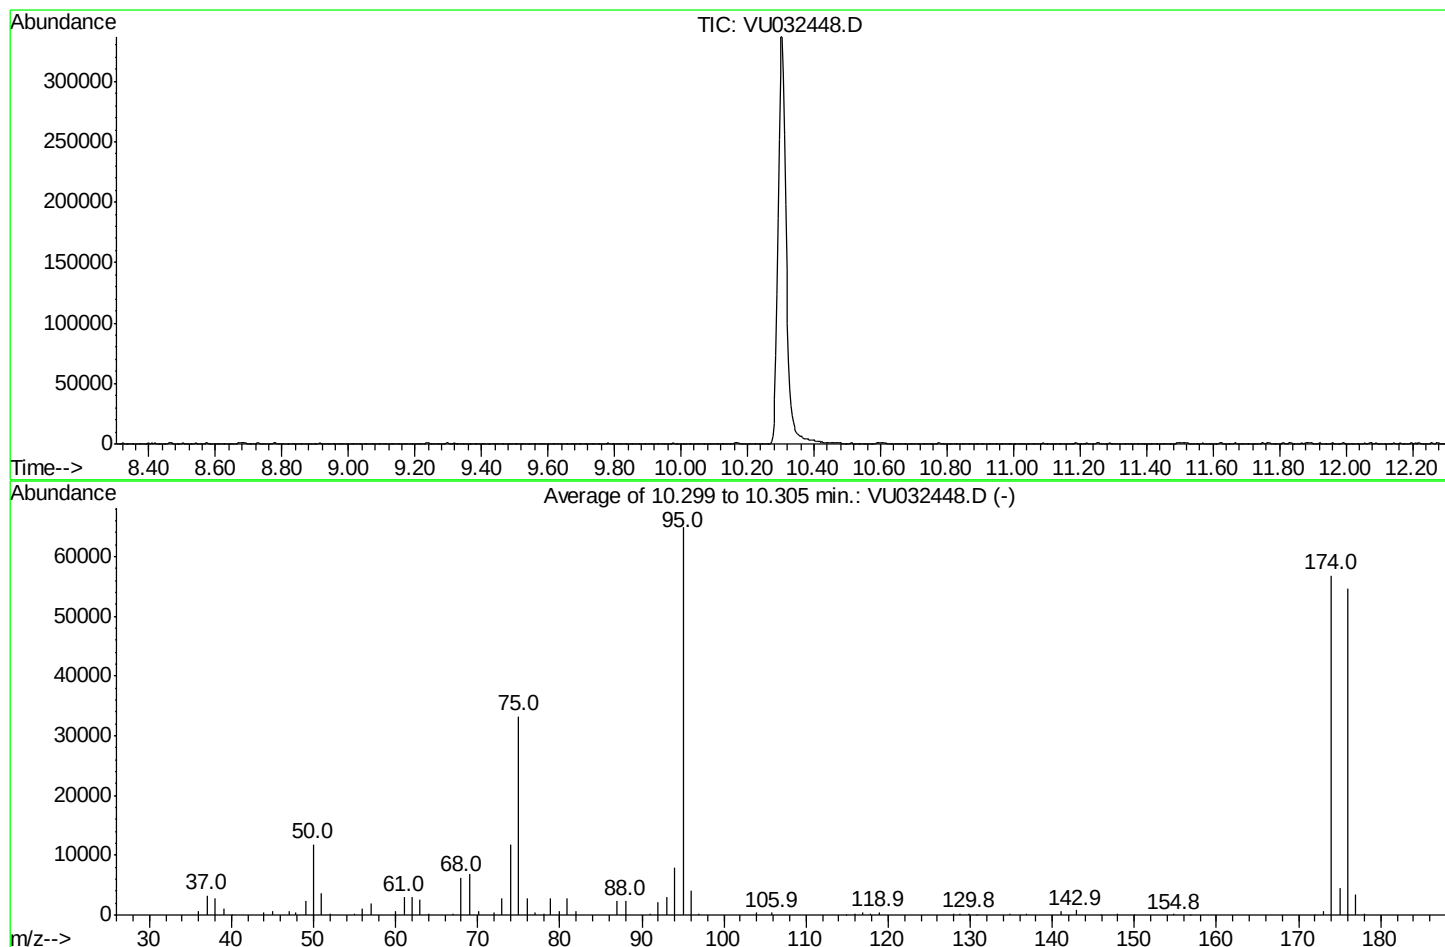

AutoFind: Scans 2864, 2865, 2866; Background Corrected with Scan 2852

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.2	11794	PASS
75	95	30	80	51.3	33314	PASS
95	95	100	100	100.0	64890	PASS
96	95	5	9	6.3	4091	PASS
173	174	0.00	2	1.1	627	PASS
174	95	50	120	87.6	56840	PASS
175	174	5	9	7.8	4424	PASS
176	174	95	101	96.1	54618	PASS
177	176	5	9	6.4	3470	PASS

Scan 2852 (10.260 min): VU032448.D
BFB16

m/z	Abundance
39.90	107.0
44.00	390.0

Instrument :
MSVOA_U
ClientSampleId :
BFB16

m/z	Abundance
36.00	651.0
37.00	3277.0
38.00	2796.0
39.10	994.0
40.10	129.0
44.00	758.0
45.00	508.0
47.00	592.0
47.90	374.0
49.00	2232.0
50.00	11142.0
51.00	3578.0
52.00	134.0
55.00	205.0
56.00	1008.0
57.00	1768.0
60.00	549.0
61.00	2763.0
62.00	2892.0
63.00	2357.0
64.00	267.0
66.90	183.0
68.00	6310.0
69.00	6536.0
70.10	582.0
72.00	358.0
73.00	2693.0
74.00	11209.0
75.00	31848.0
76.00	2601.0
77.00	423.0
78.00	206.0
78.90	2786.0
79.90	673.0
80.90	2578.0
81.90	566.0
87.00	2240.0
88.00	2311.0
91.00	222.0
92.00	1892.0
93.00	2709.0
94.00	7429.0
95.00	61376.0
96.10	4015.0
97.00	125.0
103.90	375.0
105.90	364.0
115.90	212.0
116.90	438.0
117.80	175.0
118.90	421.0
127.90	231.0
128.80	131.0
129.80	246.0
134.90	107.0
136.80	145.0
141.00	705.0
142.90	725.0
145.90	129.0
148.00	139.0
154.80	149.0
156.80	104.0
173.10	518.0
174.00	51784.0
175.00	4267.0
176.00	50016.0
177.00	3277.0
178.00	141.0

Instrument :
MSVOA_U
ClientSampleId :
BFB16

m/z	Abundance
36.00	700.0
37.00	3380.0
38.00	2980.0
39.10	1069.0
40.00	132.0
44.00	788.0
45.00	573.0
47.00	640.0
47.90	403.0
49.00	2521.0
50.00	12033.0
51.00	3815.0
52.00	160.0
55.00	238.0
56.00	1117.0
57.00	1900.0
60.00	591.0
61.00	3203.0
62.10	3025.0
63.00	2699.0
64.00	294.0
67.00	212.0
68.00	6483.0
69.00	6962.0
70.00	610.0
72.00	367.0
73.00	2925.0
74.00	12238.0
75.00	34464.0
76.00	2980.0
77.10	433.0
78.00	224.0
78.90	2923.0
79.90	750.0
80.90	2811.0
81.90	679.0
87.00	2455.0
88.00	2525.0
91.00	275.0
92.00	2162.0
93.00	3109.0
94.00	8257.0
95.00	67120.0
96.10	4205.0
97.00	123.0
103.90	423.0
105.90	416.0
115.90	243.0
116.90	440.0
117.90	214.0
118.90	435.0
128.00	247.0
128.80	120.0
129.80	271.0
134.90	130.0
136.80	144.0
141.00	759.0
142.90	855.0
145.90	119.0
147.90	142.0
150.00	101.0
154.90	152.0
156.80	100.0
171.90	132.0
173.10	644.0
174.00	58424.0
175.00	4552.0
176.00	56432.0
177.00	3533.0
178.00	128.0

Instrument :
MSVOA_U
ClientSampleId :
BFB16

m/z	Abundance
36.00	694.0
37.00	3082.0
38.00	2916.0
39.00	1064.0
39.90	144.0
44.00	819.0
45.00	590.0
47.00	653.0
47.90	386.0
49.00	2608.0
50.00	12209.0
51.00	3743.0
52.10	170.0
54.90	240.0
56.00	1106.0
57.00	1862.0
60.00	626.0
61.00	3211.0
62.10	2904.0
63.00	2662.0
64.00	282.0
67.00	219.0
68.00	6167.0
69.00	6803.0
70.00	604.0
72.00	323.0
73.00	2821.0
74.00	11970.0
75.00	33632.0
76.00	2982.0
77.10	408.0
78.00	248.0
78.90	2745.0
79.90	736.0
80.90	2785.0
81.90	715.0
87.00	2476.0
88.00	2477.0
90.90	283.0
92.00	2151.0
93.00	3205.0
94.00	8371.0
95.00	66176.0
96.00	4053.0
97.00	121.0
103.90	399.0
105.90	428.0
114.90	103.0
115.90	260.0
117.00	418.0
117.90	218.0
118.90	447.0
128.00	261.0
128.80	107.0
129.90	278.0
130.80	104.0
134.90	139.0
136.90	120.0
141.00	759.0
142.90	883.0
147.90	140.0
154.90	154.0
171.90	129.0
173.10	719.0
174.00	60312.0
175.00	4454.0
176.00	57408.0
177.00	3602.0
178.00	102.0

Instrument :
MSVOA_U
ClientSampleId :
BFB16