

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU060520\
 Data File : VU038592.D
 Acq On : 06 Jun 2020 01:23
 Operator : SY/MD
 Sample : L2884-05
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFXD9

Quant Time: Jun 06 02:40:00 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR053120WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Jun 06 02:36:38 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.28	114	313277	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.44	117	311128	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.82	152	149410	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.61	65	67351	3.32	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	66.40%
7) Chloroethane-d5	1.93	69	62161	3.99	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	79.80%
11) 1,1-Dichloroethene-d2	2.59	63	110483	2.77	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	55.40%#
20) 2-Butanone-d5	4.68	46	338988	55.04	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	110.08%
24) Chloroform-d	5.10	84	173306	4.55	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.00%
26) 1,2-Dichloroethane-d4	5.74	65	104608	4.84	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	96.80%
32) Benzene-d6	5.76	84	342403	4.41	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	88.20%
36) 1,2-Dichloropropane-d6	6.72	67	109667	4.59	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	91.80%
41) Toluene-d8	7.92	98	288412	4.14	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	82.80%
43) trans-1,3-Dichloropropene-	8.20	79	42578	4.14	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	82.80%
46) 2-Hexanone-d5	8.65	63	282069	55.61	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	111.22%
57) 1,1,2,2-Tetrachloroethane-	10.77	84	97273	4.80	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	96.00%
64) 1,2-Dichlorobenzene-d4	12.20	152	125068	4.85	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	97.00%

Target Compounds


					Ovalue
13) Acetone	2.68	43	8649	2.146	ug/L 95
16) Methylene chloride	3.08	84	1867	0.086	ug/L 80
35) Methylcyclohexane	6.72	83	25799	0.740	ug/L # 18
37) 1,2-Dichloropropane	6.72	63	12124	0.555	ug/L # 86
39) cis-1,3-Dichloropropene	7.59	75	3007	0.093	ug/L # 48
53) m,p-Xylene	9.71	106	6485	0.167	ug/L 94
54) o-Xylene	10.12	106	5145	0.138	ug/L 96
59) 1,2,3-Trichloropropane	11.83	75	17670	1.084	ug/L # 85
65) 1,2-Dichlorobenzene	12.22	146	4620	0.111	ug/L # 90
69) Naphthalene	14.11	128	7544	0.125	ug/L # 94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU060520\
Data File : VU038592.D
Acq On : 06 Jun 2020 01:23
Operator : SY/MD
Sample : L2884-05
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFXD9

Quant Time: Jun 06 02:40:00 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR053120WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Jun 06 02:36:38 2020
Response via : Initial Calibration




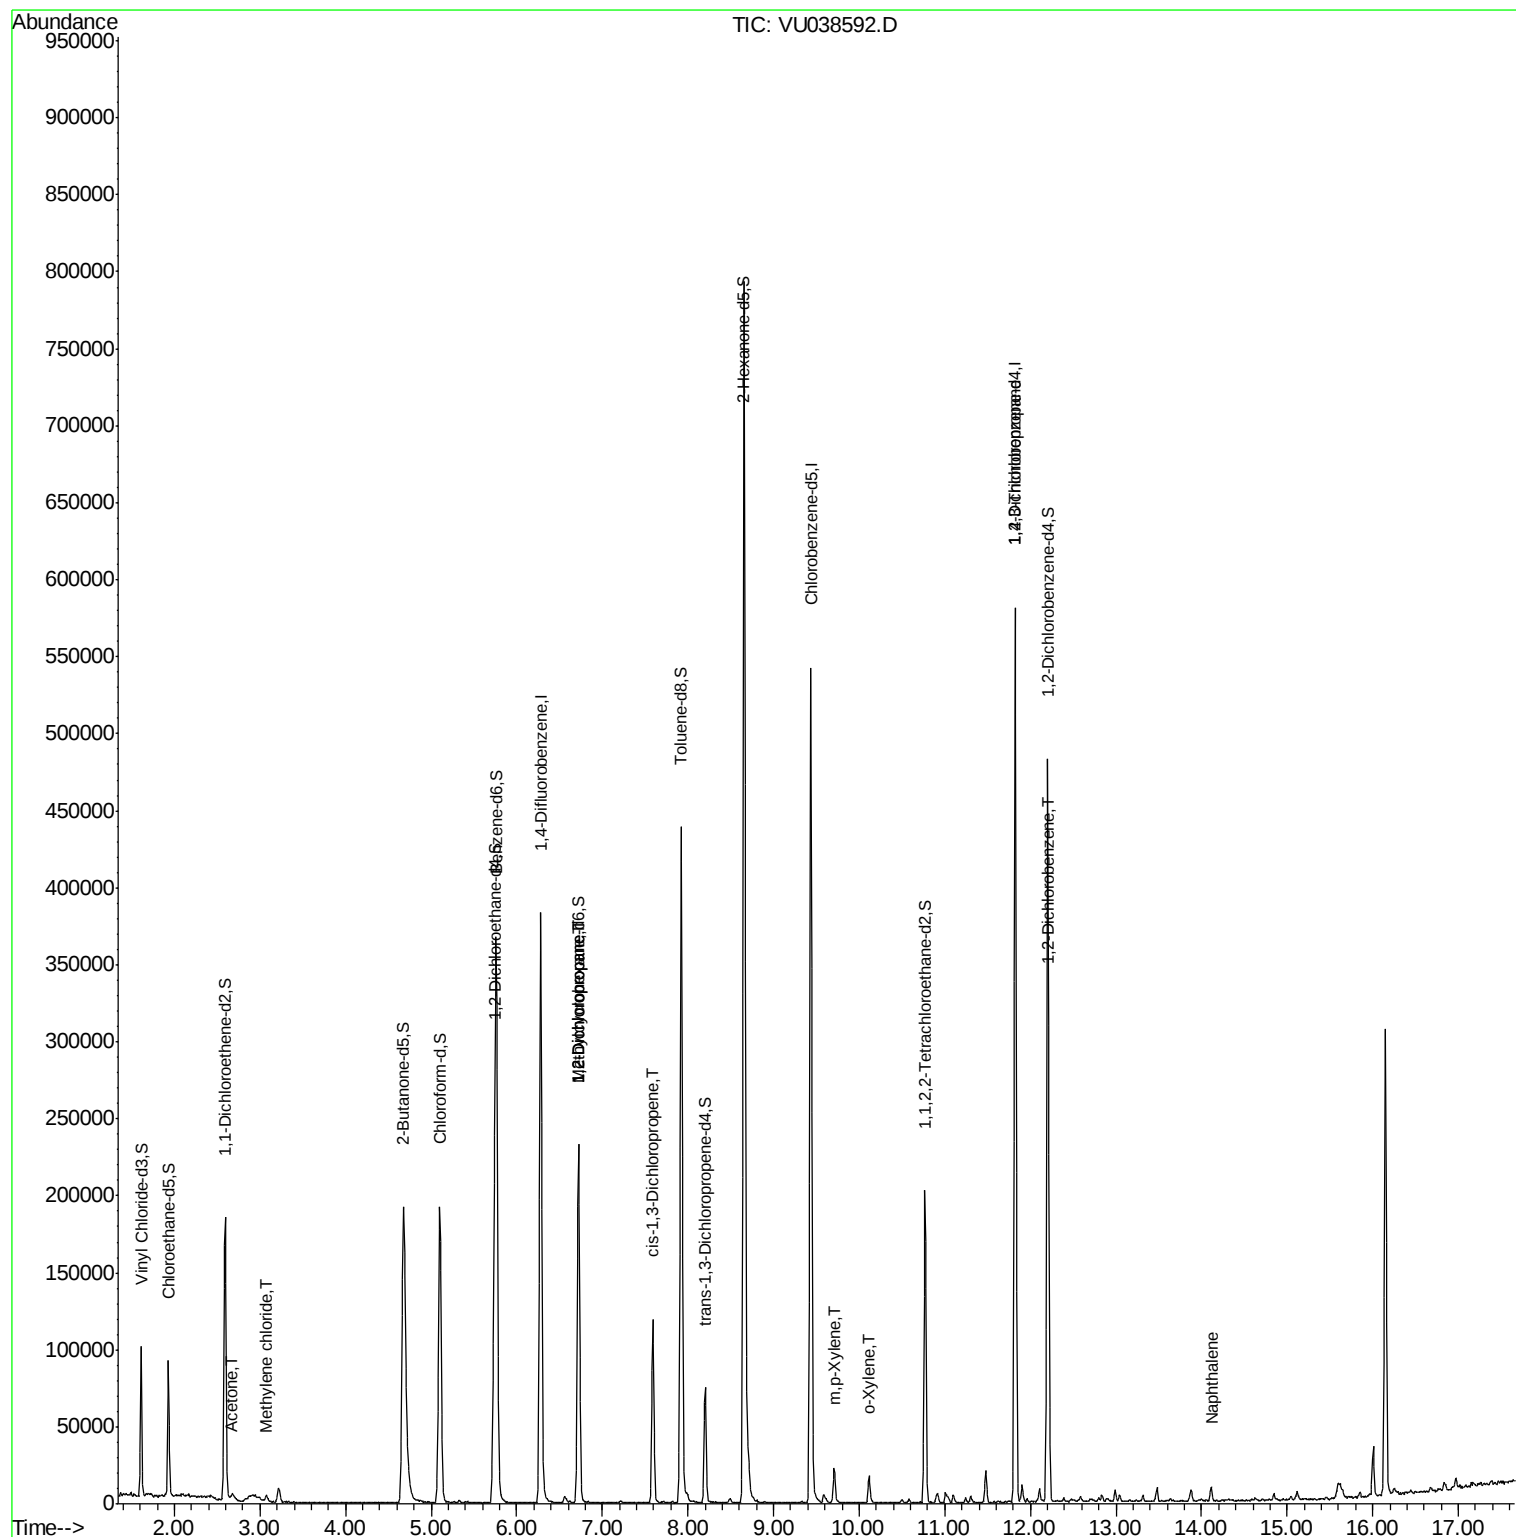


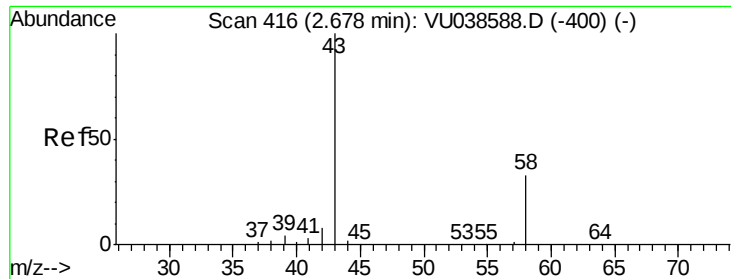

#13
Acetone
Concen: 2.146 ug/L
RT: 2.68 min Scan# 417
Delta R.T. 0.00 min
Lab File: VU038592.D
Acq: 06 Jun 2020 01:23




Instrument :
MSVOA_U
ClientSampleId :
BFXD9


Tot Ion: 43 Resp: 8649
Ion Ratio Lower Upper
43 100
58 35.5 0.0 65.6

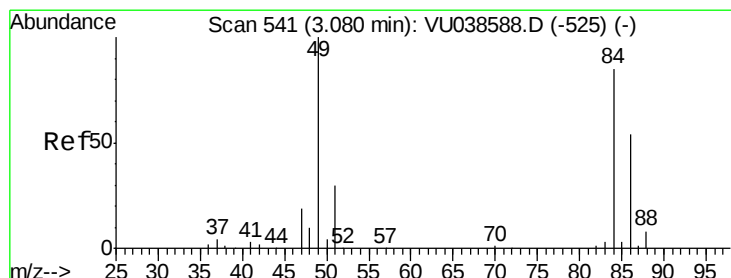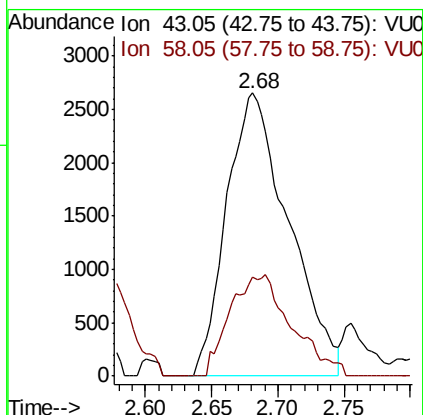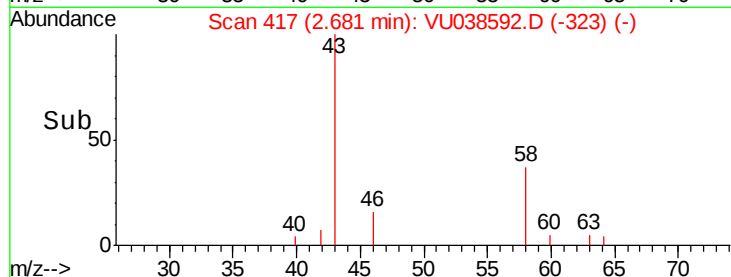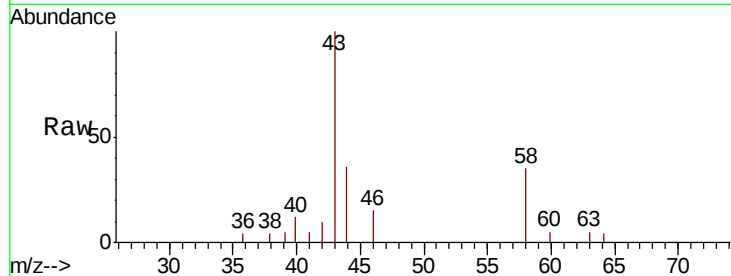

#16
Methylene chloride
Concen: 0.086 ug/L
RT: 3.08 min Scan# 540
Delta R.T. -0.00 min
Lab File: VU038592.D
Acq: 06 Jun 2020 01:23

Tgt Ion: 84 Resp: 1867
Ion Ratio Lower Upper
84 100
86 49.8 45.0 83.6
49 98.6 85.5 158.9

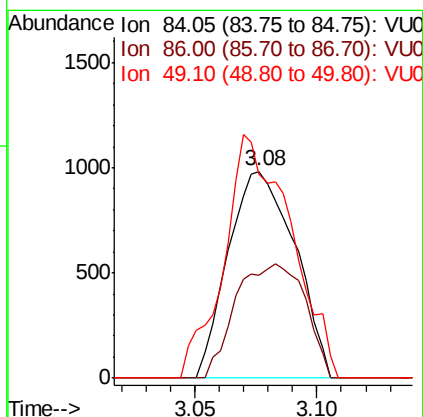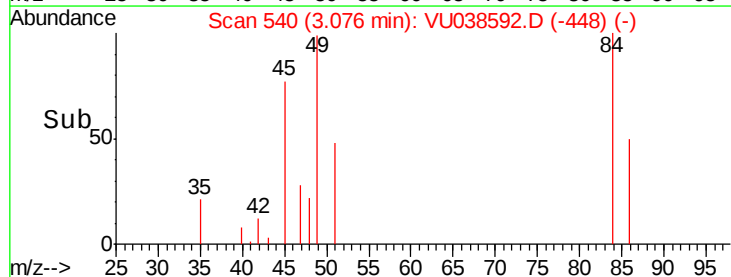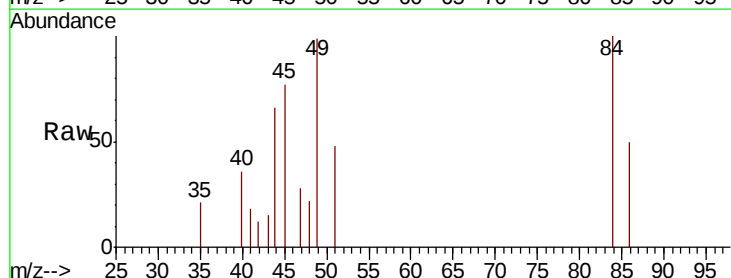


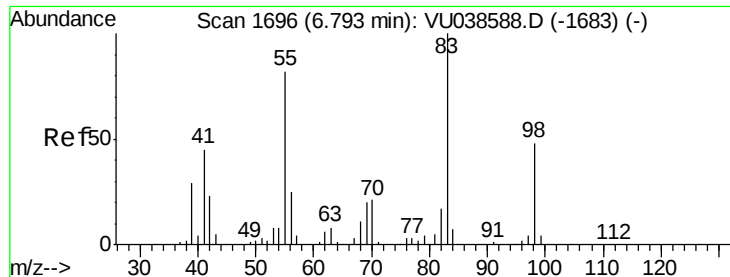




#35
Methvlcvclohexane
Concen: 0.740 ug/L
RT: 6.72 min Scan# 1674
Delta R.T. -0.07 min
Lab File: VU038592.D
Acq: 06 Jun 2020 01:23

Instrument :
MSVOA_U
ClientSampleId :
BFXD9

Tot Ion: 83 Resp: 25799
Ion Ratio Lower Upper
83 100
55 0.5 63.4 95.2#
98 1.1 39.0 58.4#

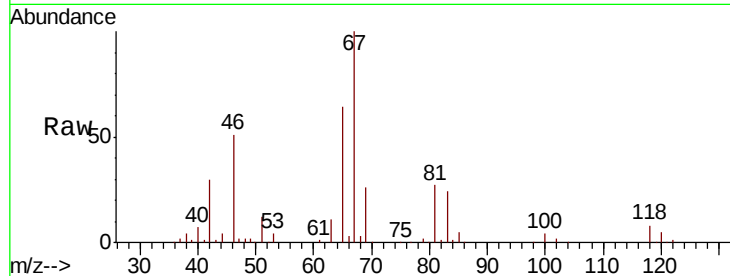


Abundance Ion 83.15 (82.85 to 83.85): VU0
Ion 55.10 (54.80 to 55.80): VU0
Ion 98.15 (97.85 to 98.85): VU0

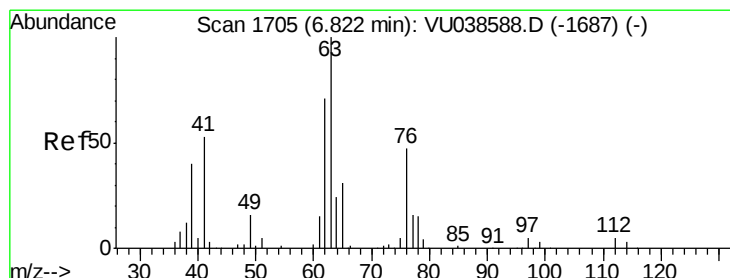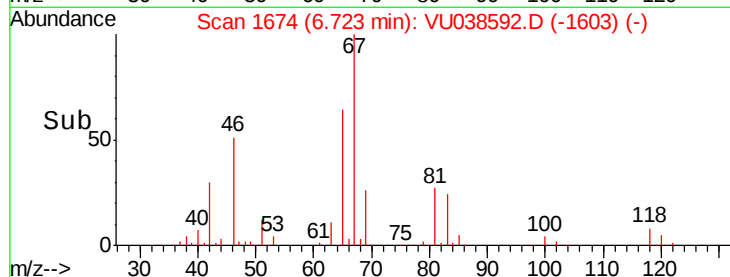
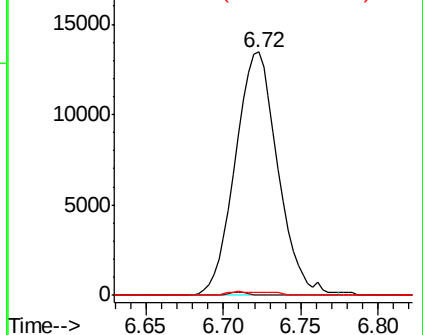



#37
1,2-Dichloropropane
Concen: 0.555 ug/L
RT: 6.72 min Scan# 1673
Delta R.T. -0.10 min
Lab File: VU038592.D
Acq: 06 Jun 2020 01:23

Tgt Ion: 63 Resp: 12124
Ion Ratio Lower Upper
63 100
112 0.0 3.7 5.5#

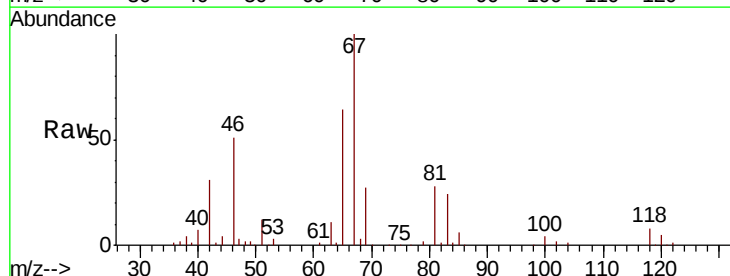

Abundance Ion 63.10 (62.80 to 63.80): VU0
Ion 112.10 (111.80 to 112.80): V

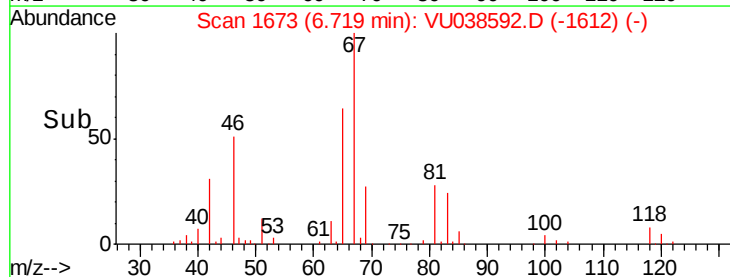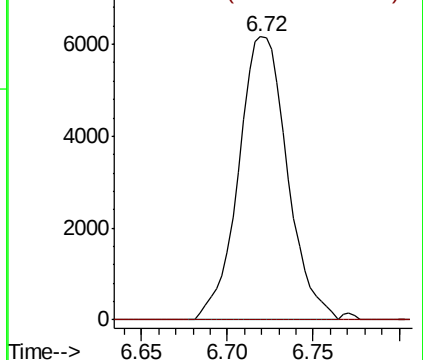

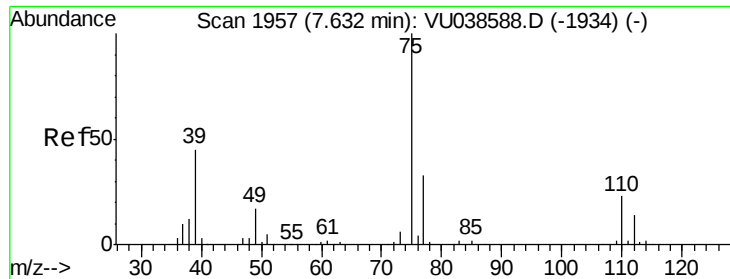

#39

cis-1,3-Dichloropropene

Concen: 0.093 ug/L

RT: 7.59 min Scan# 1944

Delta R.T. -0.04 min

Lab File: VU038592.D

Acq: 06 Jun 2020 01:23

Instrument :

MSVOA_U

ClientSampleId :


BFXD9

Tot Ion: 75 Resp: 3007

Ion Ratio Lower Upper




75 100

77 60.1 21.9 40.7#

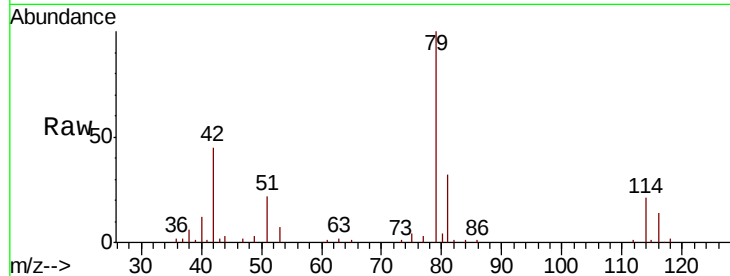

Abundance Ion 75.05 (74.75 to 75.75): VU038588.D (-1934) (-)

Ion 77.05 (76.75 to 77.75): VU038588.D (-1934) (-)

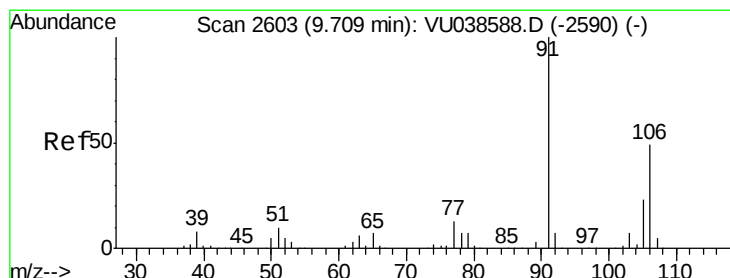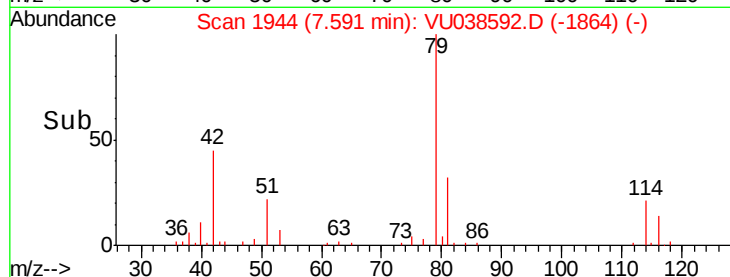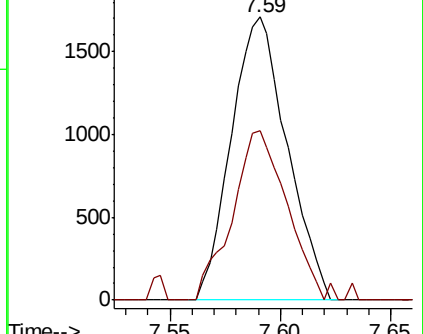

#53

m,p-Xylene

Concen: 0.167 ug/L

RT: 9.71 min Scan# 2604

Delta R.T. 0.00 min

Lab File: VU038592.D


Acq: 06 Jun 2020 01:23

Tgt Ion: 106 Resp: 6485

Ion Ratio Lower Upper



106 100


91 188.1 138.1 256.5

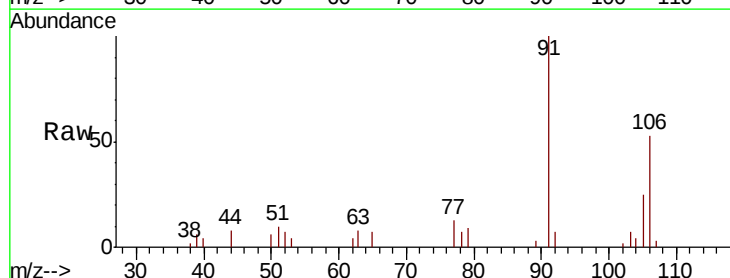

Abundance Ion 106.15 (105.85 to 106.85): VU038588.D (-2590) (-)

Ion 91.15 (90.85 to 91.85): VU038588.D (-2590) (-)

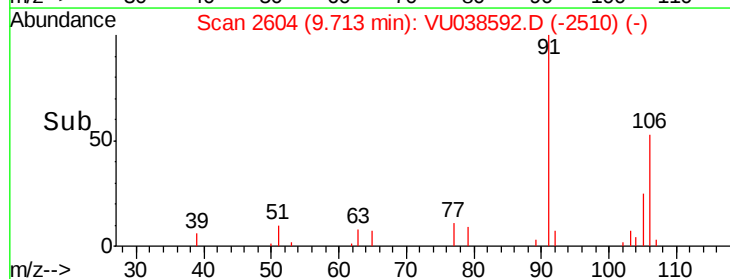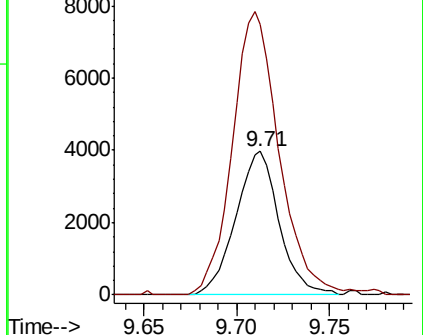


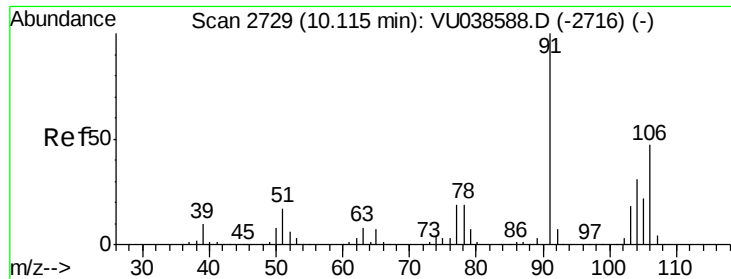




#54
o-Xylene
Concen: 0.138 ug/L
RT: 10.12 min Scan# 2730
Delta R.T. 0.00 min
Lab File: VU038592.D
Acq: 06 Jun 2020 01:23

Instrument :
MSVOA_U
ClientSampled :
BFXD9

Tot Ion:106 Resp: 5145
Ion Ratio Lower Upper
106 100
91 208.2 150.6 279.8

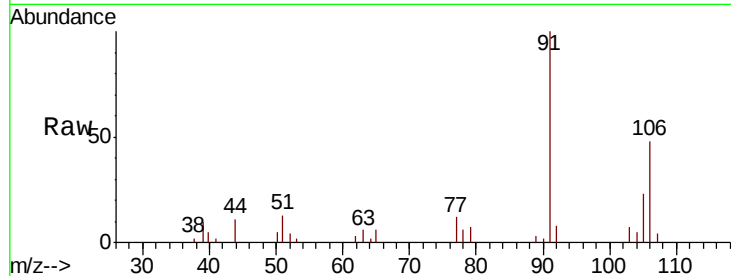


Abundance Ion 106.15 (105.85 to 106.85): VU038588.D (-2716) (-)
Ion 91.15 (90.85 to 91.85): VU038588.D (-2716) (-)

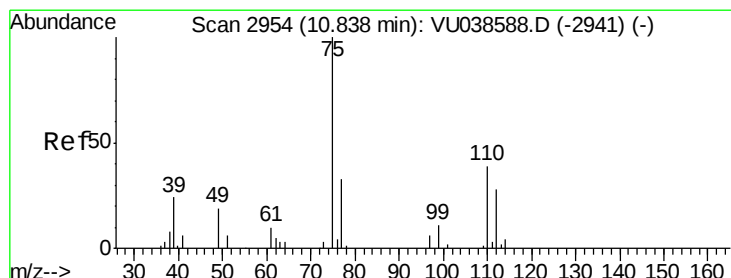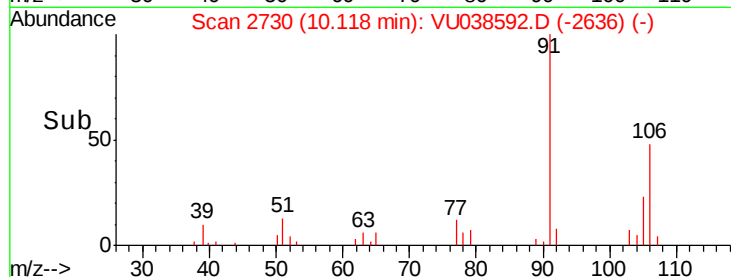
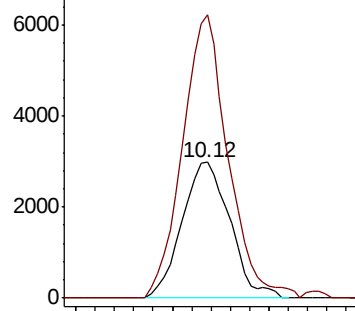



#59
1,2,3-Trichloropropane
Concen: 1.084 ug/L
RT: 11.83 min Scan# 3261
Delta R.T. 0.99 min
Lab File: VU038592.D
Acq: 06 Jun 2020 01:23

Tgt Ion: 75 Resp: 17670
Ion Ratio Lower Upper
75 100
77 40.3 25.4 38.2#

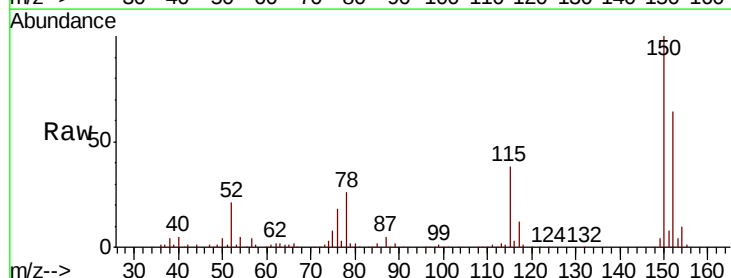

Abundance Ion 75.00 (74.70 to 75.70): VU038588.D (-2941) (-)
Ion 77.00 (76.70 to 77.70): VU038588.D (-2941) (-)

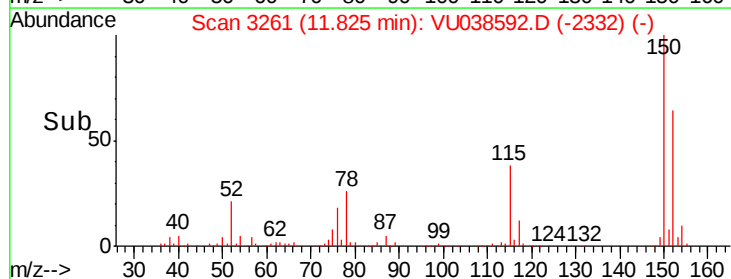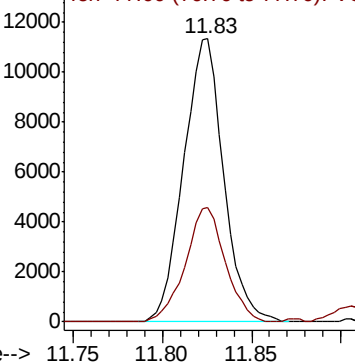

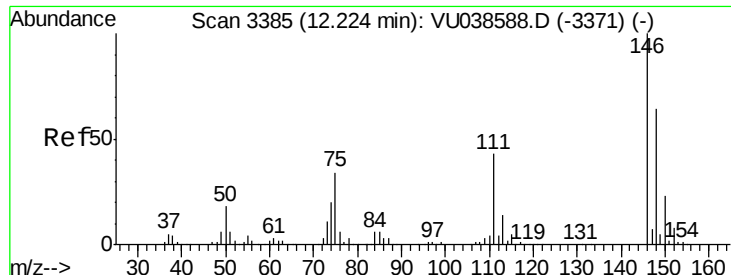

#65

1,2-Dichlorobenzene

Concen: 0.111 ug/L

RT: 12.22 min Scan# 3385

Delta R.T. 0.00 min

Lab File: VU038592.D

Acq: 06 Jun 2020 01:23

Instrument :

MSVOA_U

ClientSampled :

BFXD9


Tot Ion:146 Resp: 4620

Ion Ratio Lower Upper

146 100

111 55.0 35.1 52.7#




148 67.4 50.9 76.3

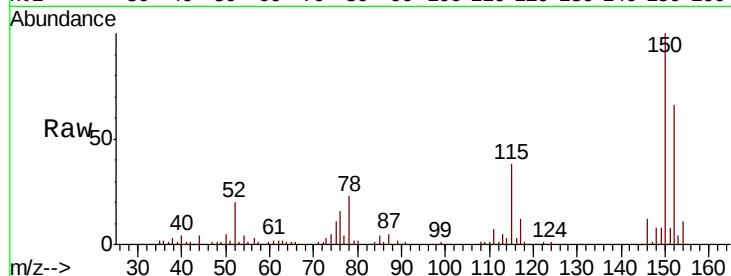

Abundance Ion 145.95 (145.65 to 146.65): V

Ion 111.00 (110.70 to 111.70): V

Ion 148.00 (147.70 to 148.70): V

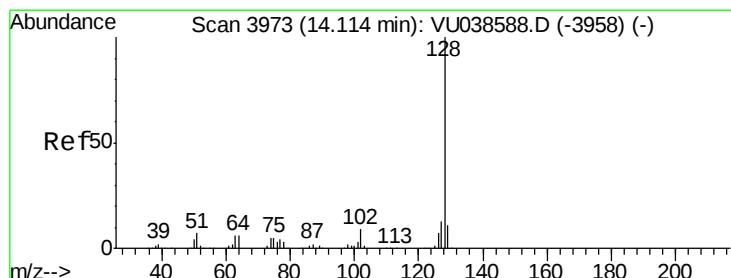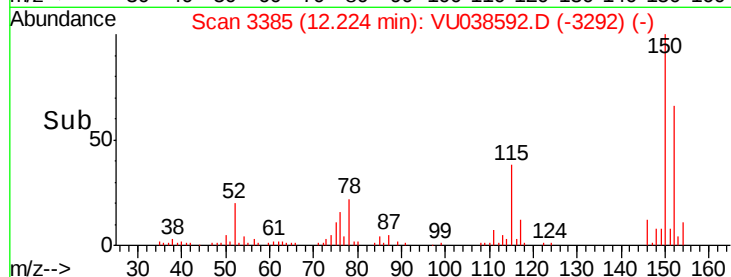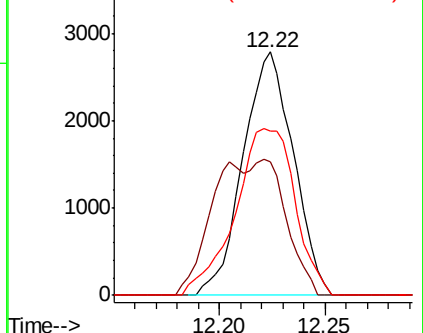

#69

Naphthalene

Concen: 0.125 ug/L

RT: 14.11 min Scan# 3973

Delta R.T. 0.00 min

Lab File: VU038592.D

Acq: 06 Jun 2020 01:23


Tgt Ion:128 Resp: 7544

Ion Ratio Lower Upper

128 100

129 10.0 8.9 13.3

127 9.1 10.2 15.4#

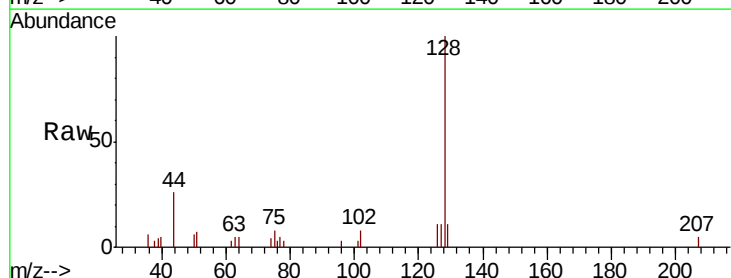

Abundance Ion 128.00 (127.70 to 128.70): V

Ion 129.00 (128.70 to 129.70): V

Ion 127.00 (126.70 to 127.70): V

