

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU060520\
 Data File : VU038586.D
 Acq On : 05 Jun 2020 20:21
 Operator : SY/MD
 Sample : L2906-05
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AG5

Quant Time: Jun 06 02:26:26 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR053120WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Jun 06 00:12:39 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.28	114	300289	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.44	117	294969	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.82	152	140475	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.61	65	63123	3.25	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	65.00%
7) Chloroethane-d5	1.93	69	60599	4.06	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	81.20%
11) 1,1-Dichloroethene-d2	2.59	63	110916	2.90	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	58.00%#
20) 2-Butanone-d5	4.67	46	298800	50.61	ug/L	-0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	101.22%
24) Chloroform-d	5.10	84	165399	4.53	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	90.60%
26) 1,2-Dichloroethane-d4	5.74	65	99756	4.81	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	96.20%
32) Benzene-d6	5.76	84	323416	4.39	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	87.80%
36) 1,2-Dichloropropane-d6	6.72	67	101744	4.49	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	89.80%
41) Toluene-d8	7.92	98	267479	4.05	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	81.00%
43) trans-1,3-Dichloropropene-	8.20	79	37968	3.90	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	78.00%
46) 2-Hexanone-d5	8.65	63	252138	52.43	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	104.86%
57) 1,1,2,2-Tetrachloroethane-	10.77	84	94419	4.91	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	98.20%
64) 1,2-Dichlorobenzene-d4	12.20	152	119171	4.92	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	98.40%


Target Compounds					Ovalue
13) Acetone	2.67	43	21993	5.692 ug/L	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU060520\
Data File : VU038586.D
Acq On : 05 Jun 2020 20:21
Operator : SY/MD
Sample : L2906-05
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AG5

Quant Time: Jun 06 02:26:26 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR053120WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Jun 06 00:12:39 2020
Response via : Initial Calibration

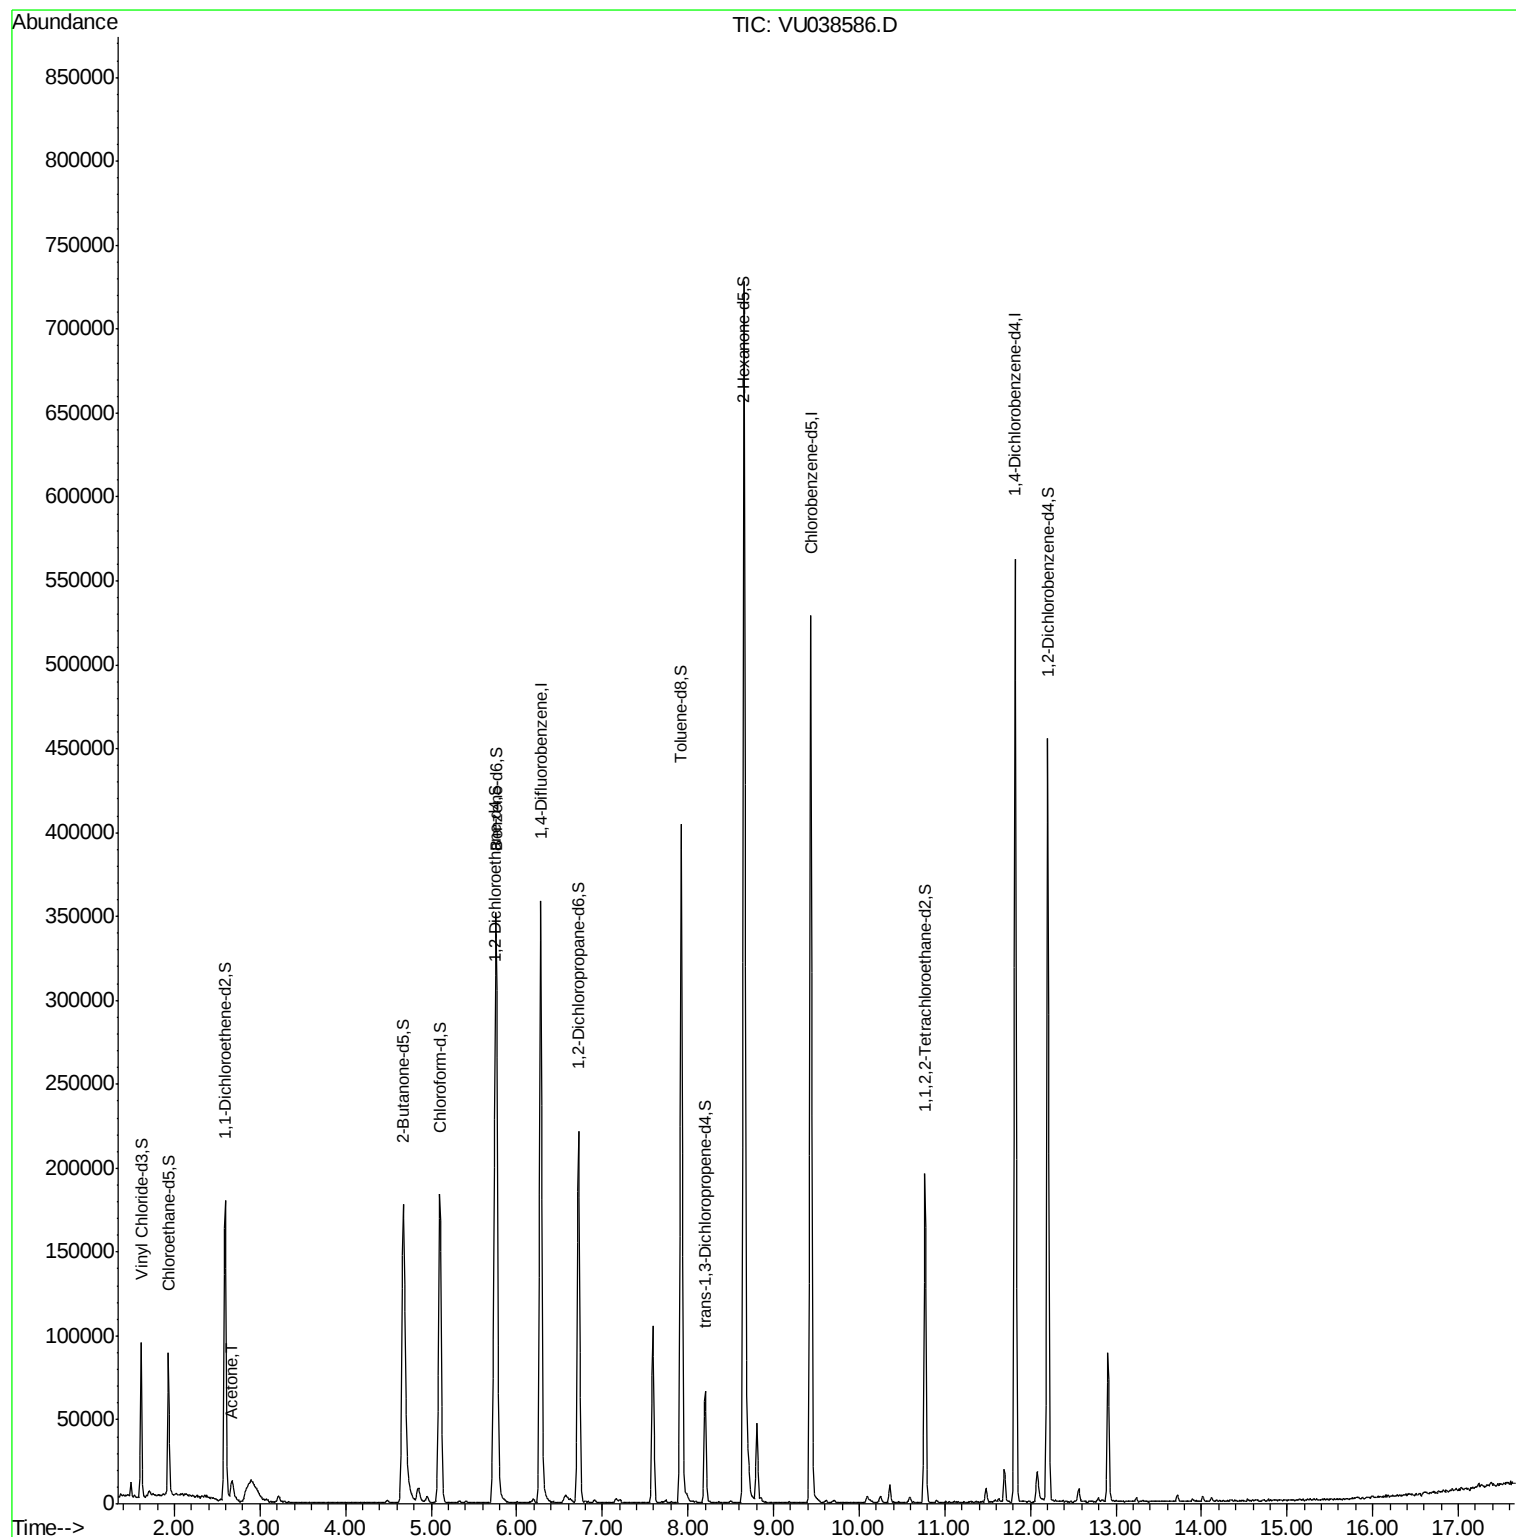

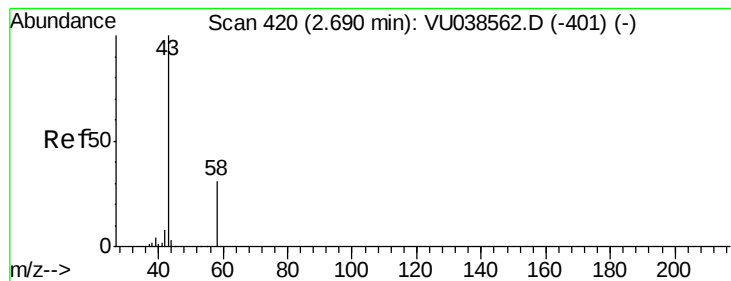

#13
 Acetone
 Concen: 5.692 ug/L
 RT: 2.67 min Scan# 413
 Delta R.T. -0.02 min
 Lab File: VU038586.D
 Acq: 05 Jun 2020 20:21

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AG5

Tot Ion: 43 Resp: 21993
 Ion Ratio Lower Upper
 43 100
 58 33.0 0.0 65.6

