

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU060520\
 Data File : VU038596.D
 Acq On : 06 Jun 2020 02:55
 Operator : SY/MD
 Sample : L2910-03
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F9D07

Quant Time: Jun 06 03:45:44 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR053120WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Jun 06 02:36:38 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.28	114	308556	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.44	117	299961	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.82	152	149438	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.61	65	63533	3.18	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	63.60%
7) Chloroethane-d5	1.93	69	59176	3.86	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	77.20%
11) 1,1-Dichloroethene-d2	2.59	63	109010	2.77	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	55.40%#
20) 2-Butanone-d5	4.67	46	312916	51.58	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	103.16%
24) Chloroform-d	5.10	84	164925	4.40	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	88.00%
26) 1,2-Dichloroethane-d4	5.74	65	99071	4.65	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	93.00%
32) Benzene-d6	5.76	84	324498	4.33	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	86.60%
36) 1,2-Dichloropropane-d6	6.72	67	103465	4.49	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	89.80%
41) Toluene-d8	7.92	98	273135	4.07	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	81.40%
43) trans-1,3-Dichloropropene-	8.20	79	41062	4.15	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	83.00%
46) 2-Hexanone-d5	8.65	63	260324	53.23	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	106.46%
57) 1,1,2,2-Tetrachloroethane-	10.77	84	95753	4.90	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	98.00%
64) 1,2-Dichlorobenzene-d4	12.20	152	120862	4.69	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	93.80%

Target Compounds


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
13) Acetone	2.68	43	37013	9.323	ug/L	97
21) 2-Butanone	4.76	43	9581	1.435	ug/L	80
27) 1,2-Dichloroethane	5.83	62	7441	0.284	ug/L	98
30) Cyclohexane	5.42	56	15755	0.473	ug/L	94
33) Benzene	5.81	78	115983	1.387	ug/L	100
42) Toluene	7.99	91	16157	0.184	ug/L	98
52) Ethylbenzene	9.59	91	58956	0.604	ug/L	98
53) m,p-Xylene	9.71	106	5489	0.146	ug/L	96
54) o-Xylene	10.12	106	5598	0.155	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU060520\
Data File : VU038596.D
Acq On : 06 Jun 2020 02:55
Operator : SY/MD
Sample : L2910-03
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F9D07

Quant Time: Jun 06 03:45:44 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR053120WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Jun 06 02:36:38 2020
Response via : Initial Calibration

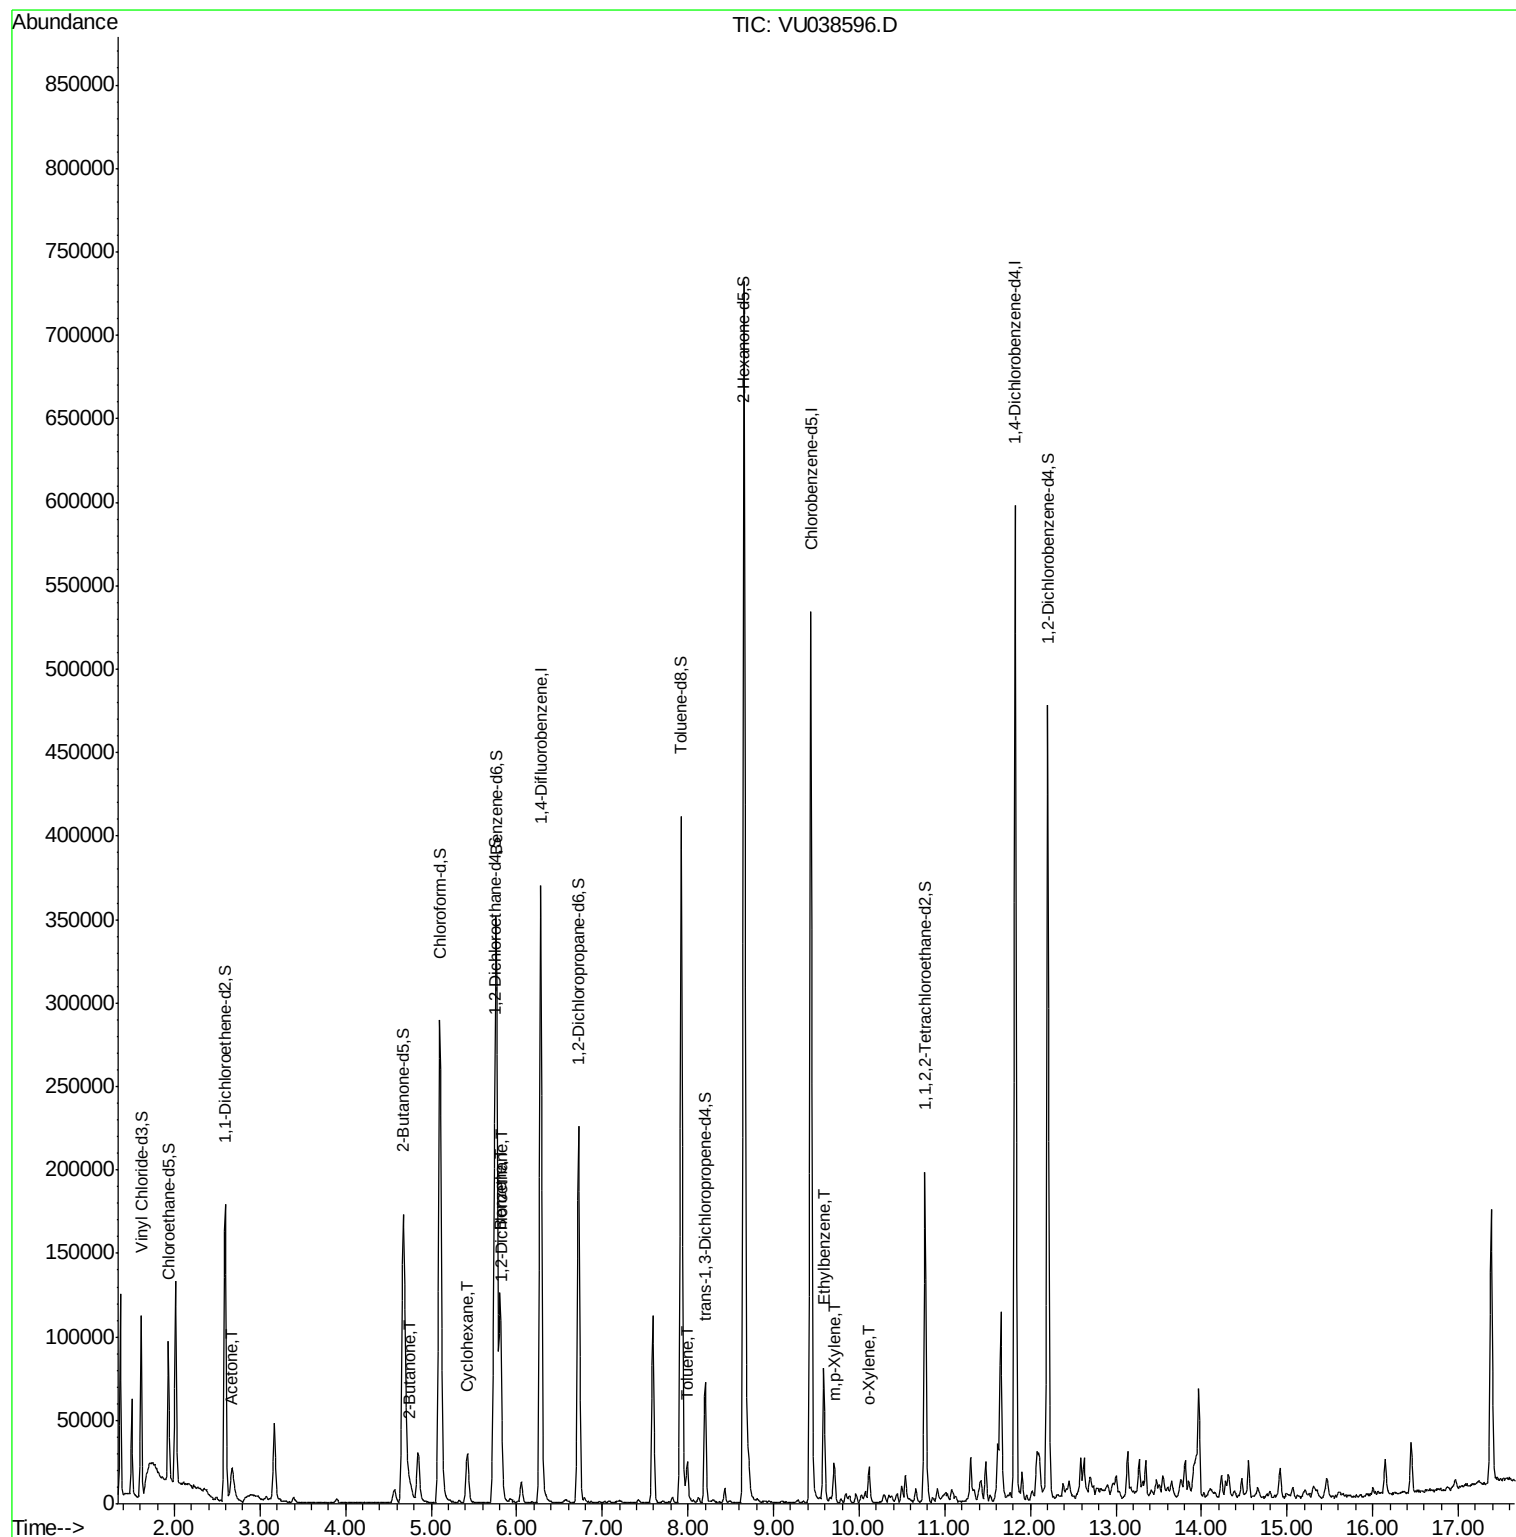

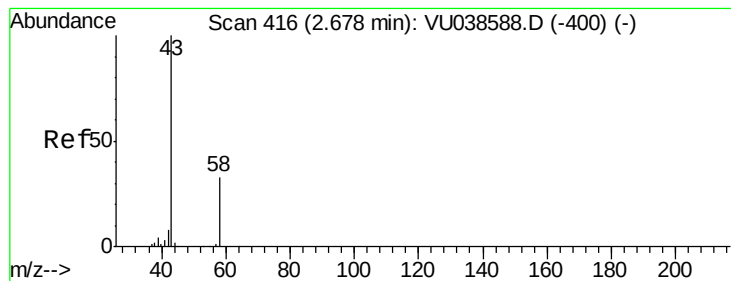

#13

Acetone

Concen: 9.323 ug/L

RT: 2.68 min Scan# 416

Delta R.T. 0.00 min

Lab File: VU038596.D

Acq: 06 Jun 2020 02:55

Instrument :

MSVOA_U

ClientSampleId :





F9D07

Tot Ion: 43 Resp: 37013

Ion Ratio Lower Upper

43 100

58 34.5 0.0 65.6

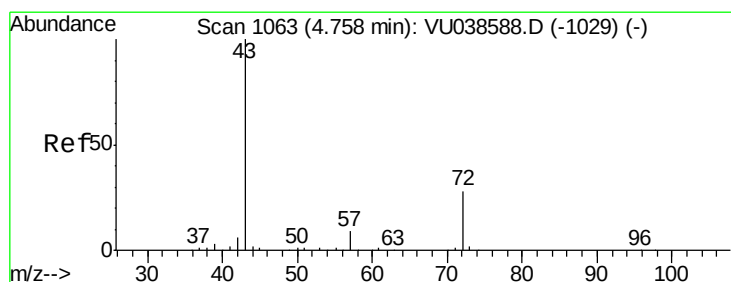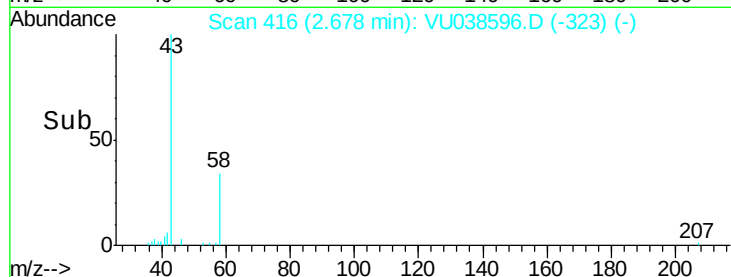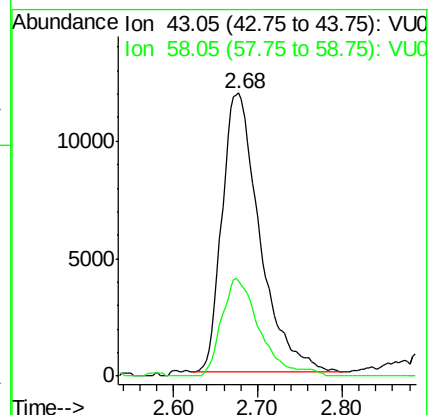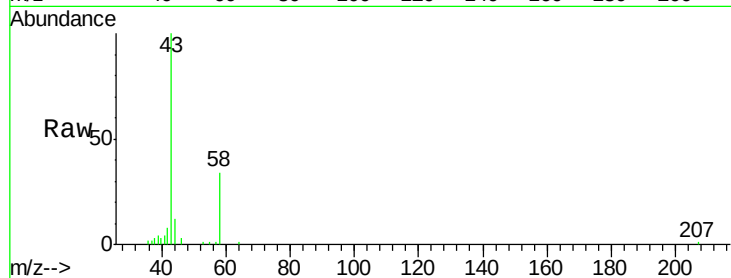

#21

2-Butanone

Concen: 1.435 ug/L

RT: 4.76 min Scan# 1064

Delta R.T. 0.00 min

Lab File: VU038596.D




Acq: 06 Jun 2020 02:55


Tgt Ion: 43 Resp: 9581

Ion Ratio Lower Upper

43 100

72 35.1 12.6 37.8

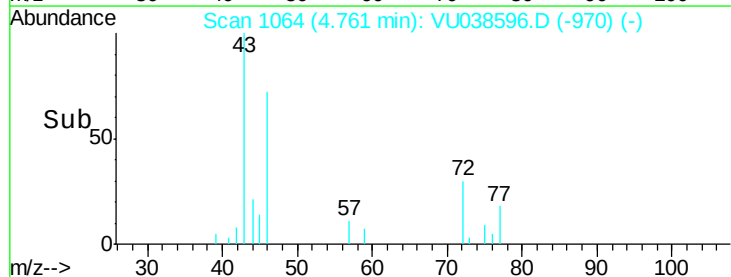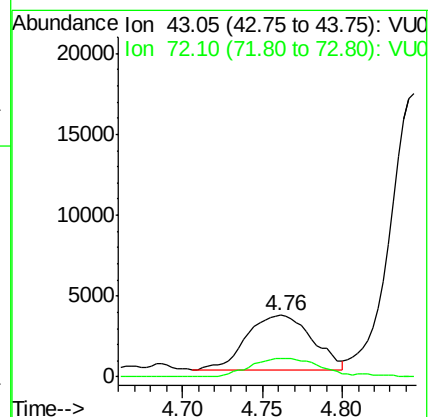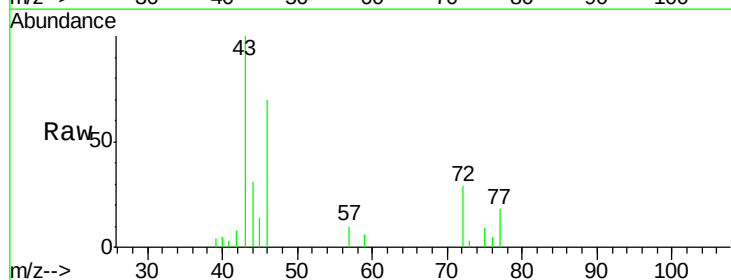

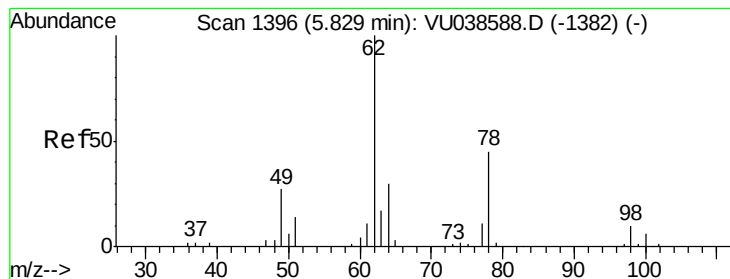

#27

1,2-Dichloroethane

Concen: 0.284 ug/L

RT: 5.83 min Scan# 1396

Delta R.T. 0.00 min

Lab File: VU038596.D

Acq: 06 Jun 2020 02:55

Instrument :

MSVOA_U

ClientSampleId :


F9D07

Tot Ion: 62 Resp: 7441

Ion Ratio Lower Upper




62 100

98 8.6 7.4 11.2

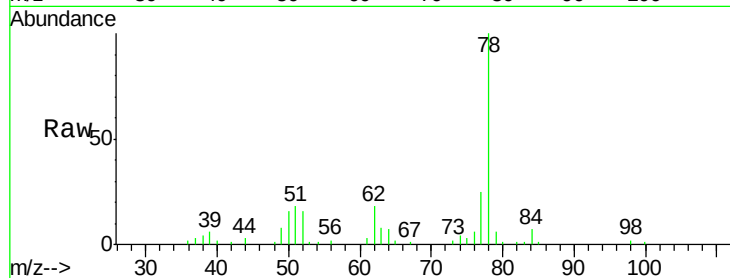

Abundance Ion 62.00 (61.70 to 62.70): VU0

Ion 98.05 (97.75 to 98.75): VU0

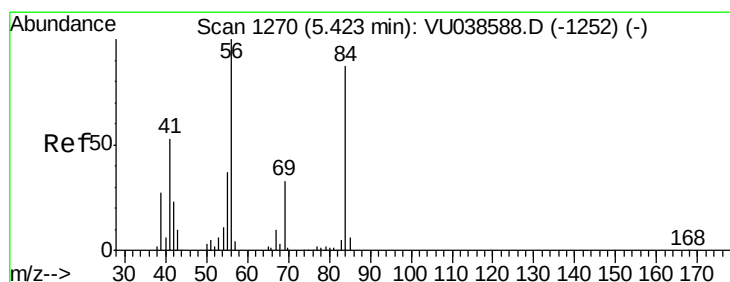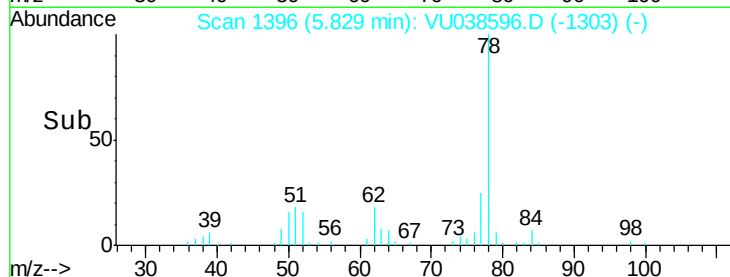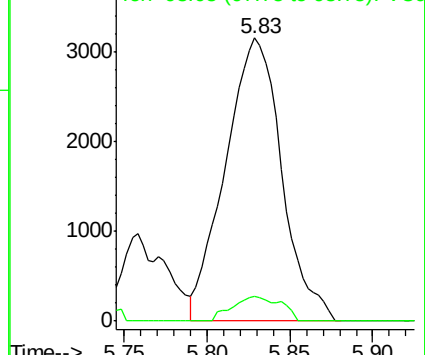

#30

Cyclohexane

Concen: 0.473 ug/L

RT: 5.42 min Scan# 1270

Delta R.T. 0.00 min

Lab File: VU038596.D

Acq: 06 Jun 2020 02:55


Tgt Ion: 56 Resp: 15755

Ion Ratio Lower Upper

56 100

69 27.9 24.2 36.4



84 82.6 70.8 106.2

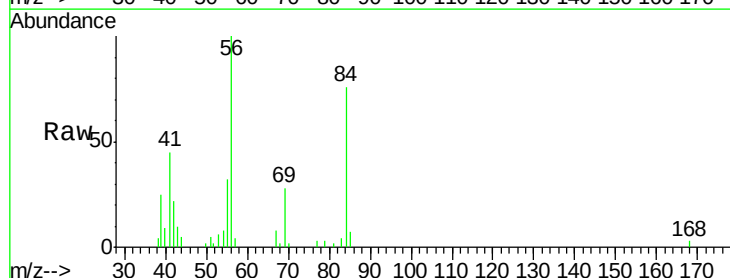


Abundance Ion 56.10 (55.80 to 56.80): VU0

Ion 69.15 (68.85 to 69.85): VU0

Ion 84.15 (83.85 to 84.85): VU0

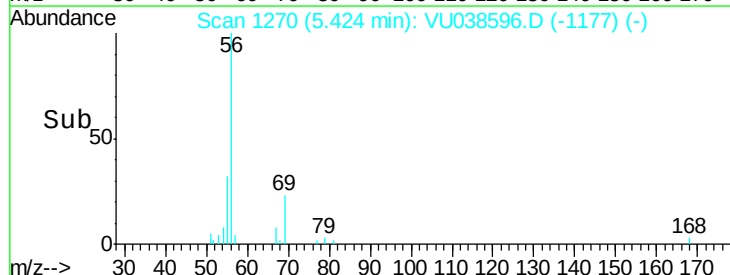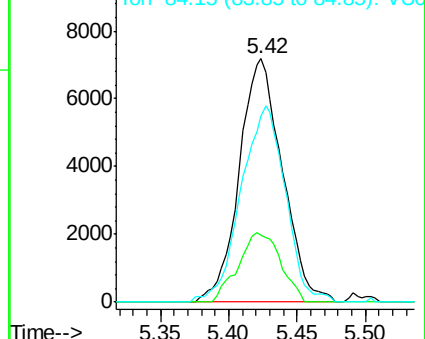

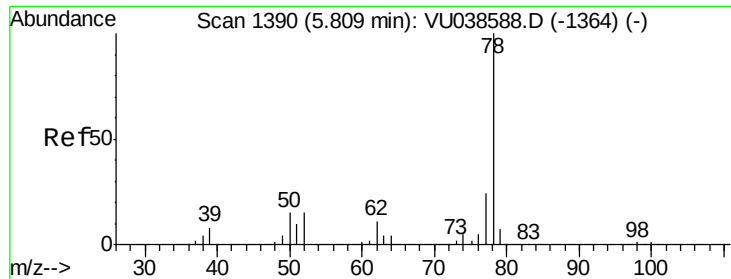

#33

Benzene

Concen: 1.387 ug/L

RT: 5.81 min Scan# 1390

Delta R.T. 0.00 min

Lab File: VU038596.D

Acq: 06 Jun 2020 02:55


Instrument :

MSVOA_U




ClientSampleId :

F9D07

Tgt Ion: 78 Resp: 115983

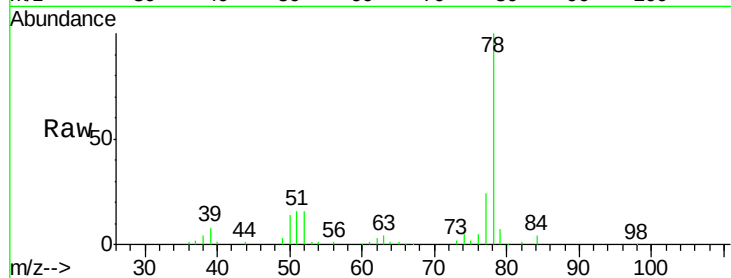

Abundance Ion 78.10 (77.80 to 78.80): VU0

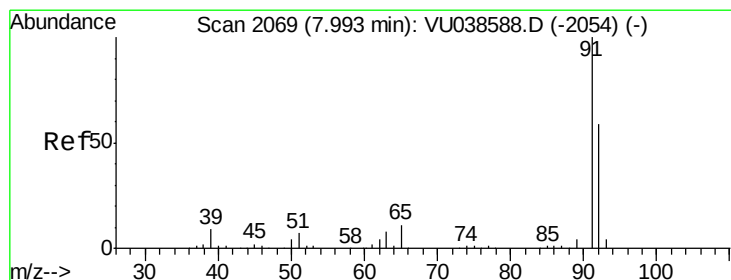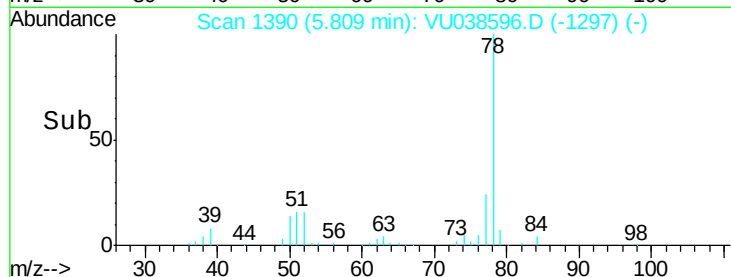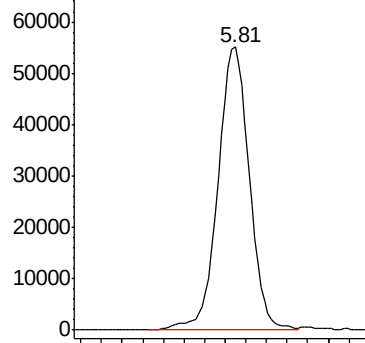

#42

Toluene

Concen: 0.184 ug/L

RT: 7.99 min Scan# 2069

Delta R.T. 0.00 min

Lab File: VU038596.D


Acq: 06 Jun 2020 02:55

Tgt Ion: 91 Resp: 16157

Ion Ratio Lower Upper



91 100


92 62.9 43.0 79.8

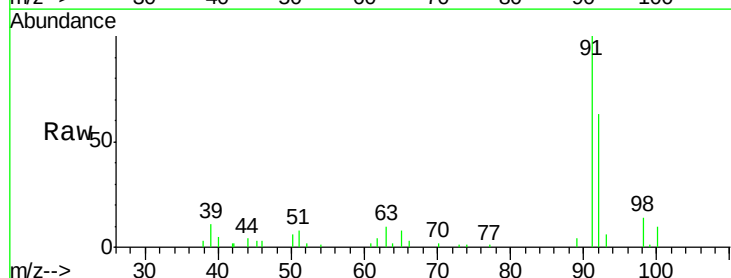

Abundance Ion 91.15 (90.85 to 91.85): VU0

Ion 92.15 (91.85 to 92.85): VU0

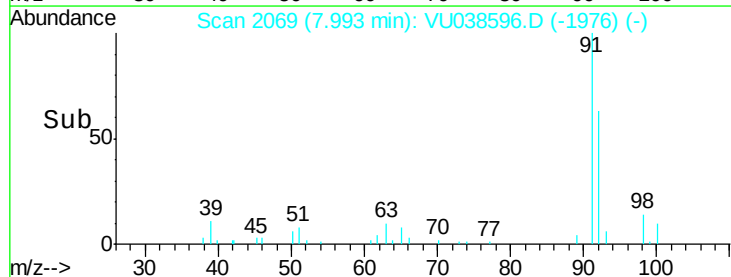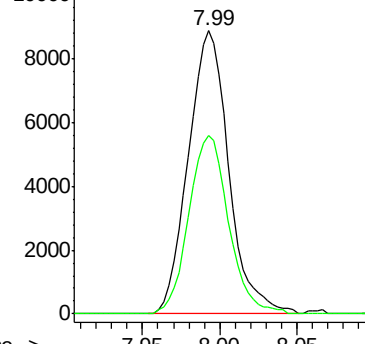

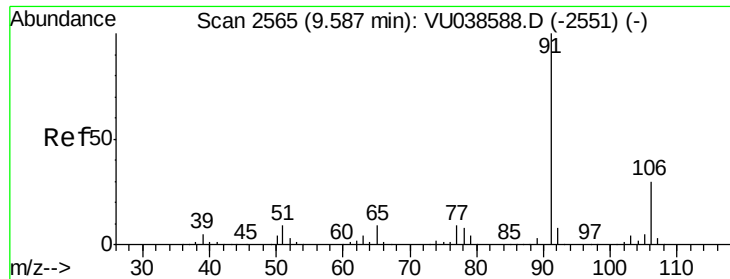

#52

Ethylbenzene

Concen: 0.604 ug/L

RT: 9.59 min Scan# 2565

Delta R.T. 0.00 min

Lab File: VU038596.D

Acq: 06 Jun 2020 02:55

Instrument :

MSVOA_U

ClientSampleId :


F9D07

Tot Ion: 91 Resp: 58956




Ion Ratio Lower Upper

91 100

106 32.4 21.7 40.3

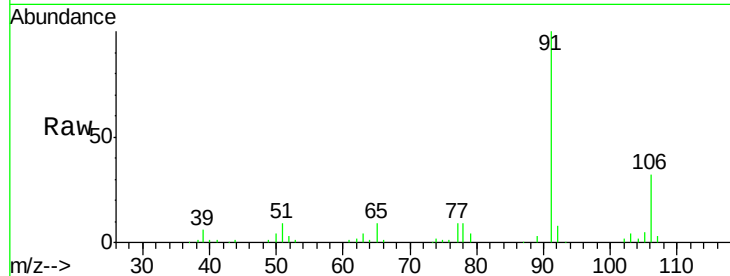

Abundance Ion 91.15 (90.85 to 91.85): VU038588.D (-2551) (-)

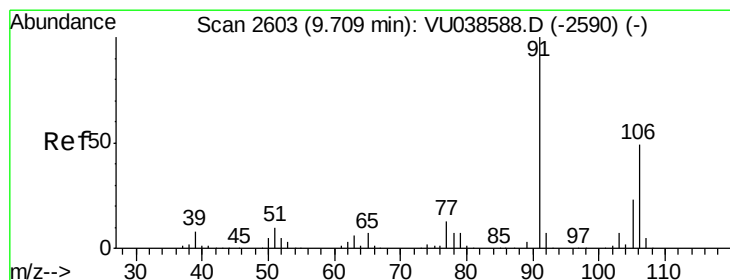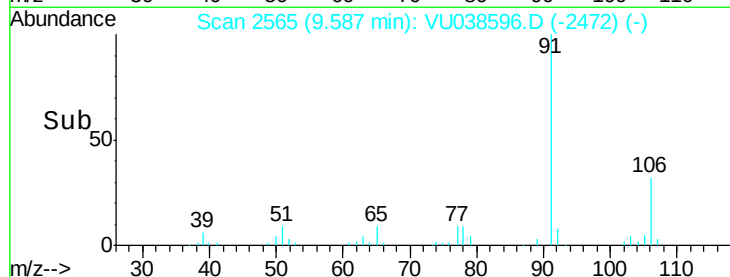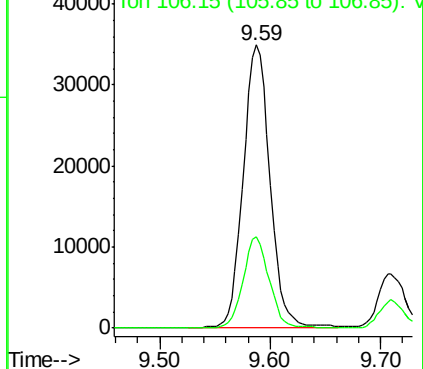

#53

m,p-Xylene

Concen: 0.146 ug/L

RT: 9.71 min Scan# 2603

Delta R.T. 0.00 min

Lab File: VU038596.D


Acq: 06 Jun 2020 02:55

Tgt Ion: 106 Resp: 5489



Ion Ratio Lower Upper


106 100

91 191.4 138.1 256.5

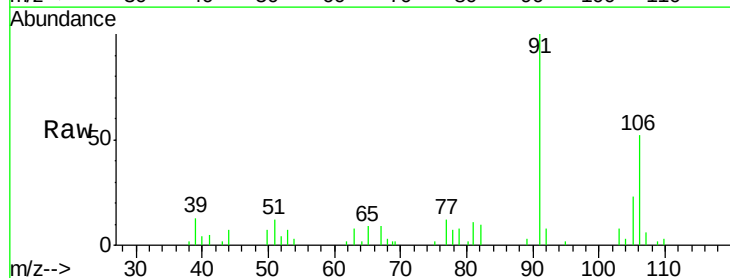

Abundance Ion 106.15 (105.85 to 106.85): VU038588.D (-2590) (-)

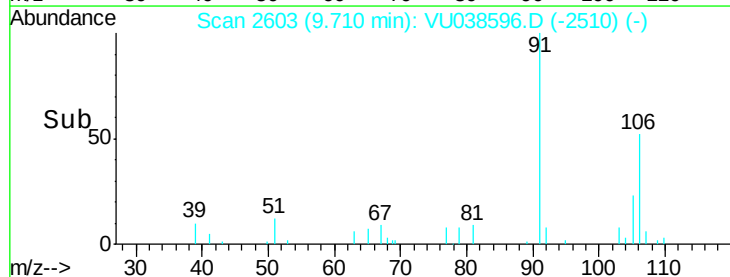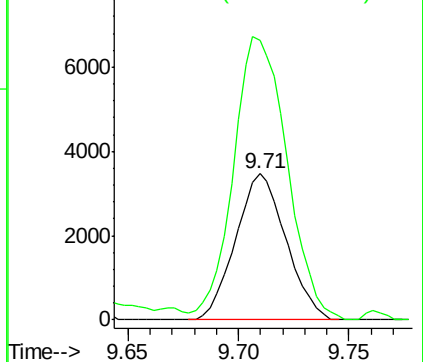

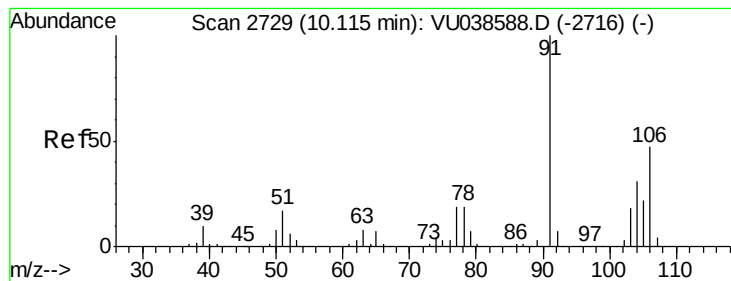

#54
 o-Xylene
 Concen: 0.155 ug/L
 RT: 10.12 min Scan# 2730
 Delta R.T. 0.00 min
 Lab File: VU038596.D
 Acq: 06 Jun 2020 02:55

Instrument :
 MSVOA_U
 ClientSampleId :
 F9D07

Tot Ion:106 Resp: 5598
 Ion Ratio Lower Upper
 106 100
 91 213.1 150.6 279.8

