


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU060520\
 Data File : VU038561.D
 Acq On : 05 Jun 2020 09:47
 Operator : SY/MD
 Sample : BFB08
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB08

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR053120WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Mon Jun 08 02:53:04 2020

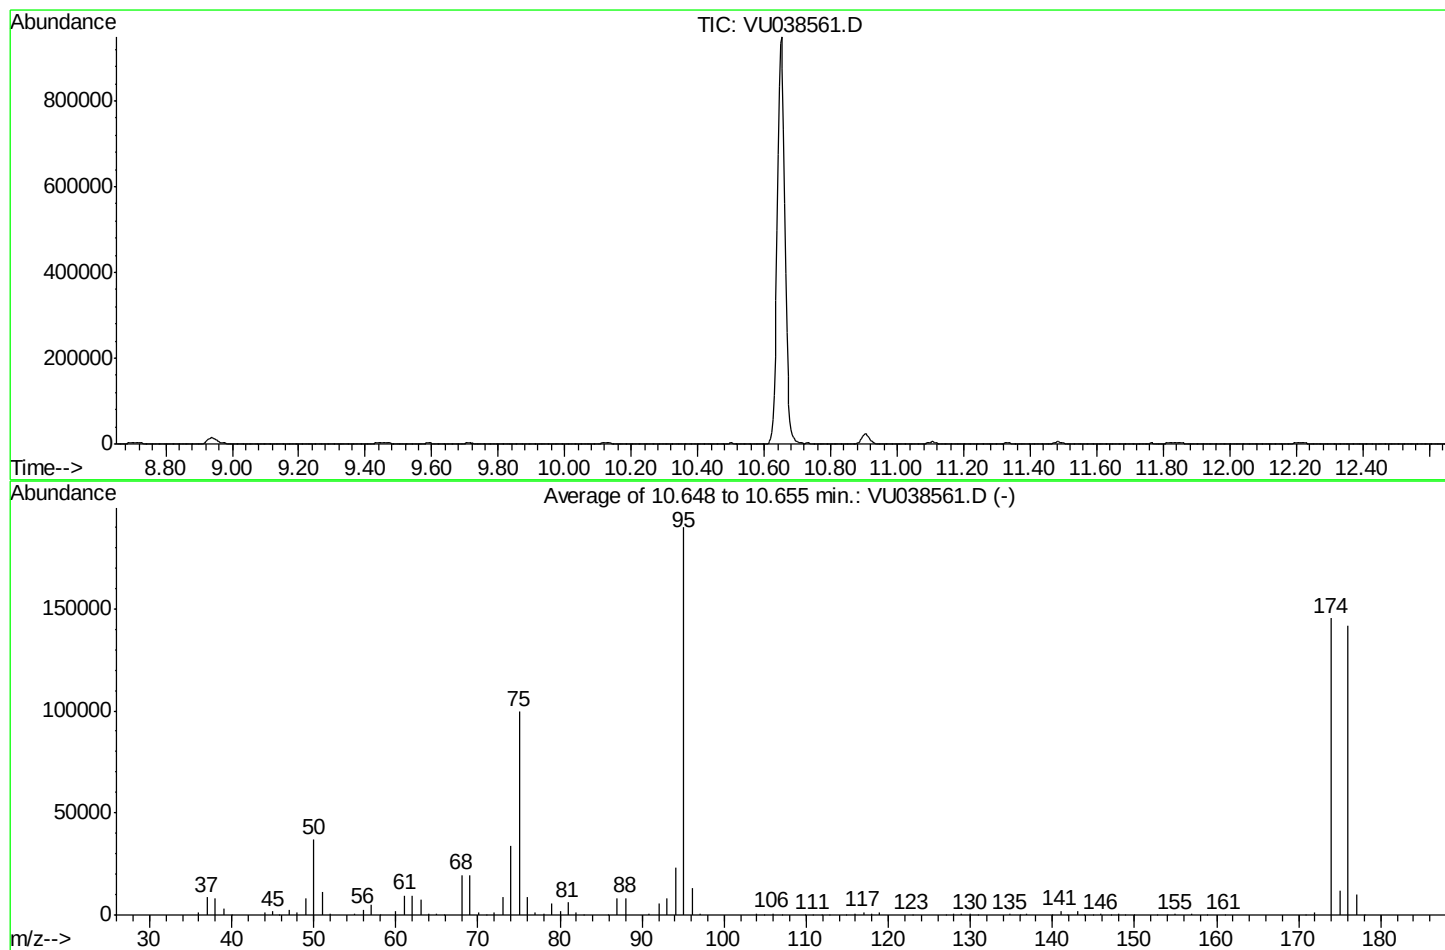

AutoFind: Scans 2895, 2896, 2897; Background Corrected with Scan 2880

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.5	36978	PASS
75	95	30	80	52.4	99437	PASS
95	95	100	100	100.0	189866	PASS
96	95	5	9	7.0	13337	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	76.6	145429	PASS
175	174	5	9	8.2	11866	PASS
176	174	95	101	97.3	141546	PASS
177	176	5	9	6.9	9775	PASS

m/z	Abundance
35.90	1565.0
37.00	8940.0
38.00	8563.0
39.00	3586.0
39.90	307.0
44.00	2021.0
45.00	1670.0
47.00	2218.0
48.00	1172.0
49.00	8404.0
50.00	37480.0
51.00	11533.0
52.00	432.0
54.90	533.0
56.00	2967.0
57.00	5140.0
58.00	193.0
60.00	1869.0
61.00	9750.0
62.00	9540.0
63.00	7392.0
63.90	919.0
65.00	1051.0
65.80	175.0
68.00	20216.0
69.00	19976.0
70.00	1507.0
72.00	1234.0
73.00	8725.0
74.00	35216.0
75.00	102520.0
76.00	9397.0
76.90	1455.0
78.00	731.0
78.90	5993.0
80.00	1701.0
80.90	6274.0
81.90	1372.0
82.90	150.0
85.90	267.0
87.00	8199.0
88.00	8404.0
90.90	901.0
92.00	5884.0
93.00	7915.0
94.10	23464.0
95.10	194368.0
96.10	13815.0
97.00	391.0
104.00	823.0
104.90	244.0
105.90	912.0
107.00	212.0
109.80	124.0
110.90	211.0
111.90	160.0
112.80	155.0
114.90	275.0
115.90	856.0
117.00	1402.0
117.90	750.0
118.90	1147.0
122.90	122.0
127.00	190.0
128.00	581.0
129.00	246.0
130.00	605.0
130.90	244.0
134.80	368.0
136.90	376.0
139.90	202.0
141.00	2186.0
141.90	233.0
143.00	2058.0
143.80	173.0
144.90	351.0
145.90	411.0
147.10	130.0
148.00	298.0
148.90	155.0
150.00	130.0
153.90	131.0
154.90	387.0
156.90	333.0
158.90	258.0
161.00	170.0
170.80	303.0
172.00	1353.0
174.00	145600.0
175.10	11710.0
176.00	140480.0
177.00	9590.0

Instrument :
MSVOA_U
ClientSampleId :
BFB08

178.00

183.0

Instrument :
MSVOA_U
ClientSampleId :
BFB08

m/z	Abundance
36.00	1505.0
37.00	8998.0
38.00	8657.0
39.00	3520.0
40.00	302.0
44.00	1864.0
45.00	1765.0
47.10	2298.0
47.90	1080.0
49.00	8295.0
50.00	38400.0
51.00	11727.0
52.00	412.0
54.90	586.0
56.10	2753.0
57.00	4965.0
58.00	246.0
60.00	1913.0
61.00	9949.0
62.00	9453.0
63.00	7697.0
64.00	885.0
65.00	930.0
65.90	168.0
68.00	20376.0
69.00	19968.0
70.00	1319.0
72.00	1224.0
73.00	8716.0
74.00	34944.0
75.00	102576.0
76.00	8646.0
76.90	1329.0
78.00	779.0
78.90	6052.0
80.00	1795.0
80.90	6346.0
81.90	1551.0
82.80	141.0
85.80	302.0
87.00	8233.0
88.00	8535.0
90.90	884.0
92.00	5938.0
93.00	8287.0
94.10	23984.0
95.10	196032.0
96.10	13842.0
97.00	367.0
104.00	841.0
104.90	230.0
106.00	977.0
107.10	176.0
109.80	107.0
110.80	257.0
111.90	145.0
112.80	146.0
114.90	304.0
115.90	910.0
117.00	1464.0
117.90	773.0
118.90	1177.0
122.90	104.0
127.00	183.0
128.00	539.0
129.00	362.0
130.00	622.0
130.90	210.0
134.80	355.0
136.90	334.0
139.90	263.0
141.00	2182.0
141.90	220.0
143.00	2094.0
143.80	160.0
144.90	330.0
145.90	360.0
147.10	125.0
148.00	341.0
148.90	185.0
150.00	143.0
152.70	130.0
154.00	109.0
155.00	430.0
157.00	333.0
158.90	218.0
160.90	123.0
170.80	239.0
172.00	1331.0
174.00	150080.0
175.10	12318.0
176.00	146048.0

Instrument :
MSVOA_U
ClientSampleId :
BFB08

177.0010156.0

178.00229.0

Instrument :
MSVOA_U

ClientSampleId :
BFB08

m/z	Abundance
36.00	1298.0
37.00	8250.0
38.00	7644.0
39.00	3040.0
40.00	313.0
44.00	1664.0
45.00	1679.0
45.80	165.0
47.10	2136.0
47.90	969.0
49.00	7385.0
50.00	35056.0
51.00	10587.0
52.00	337.0
54.90	572.0
56.10	2574.0
57.00	4711.0
58.00	245.0
60.00	1702.0
61.10	8871.0
62.00	8819.0
63.00	7106.0
64.00	852.0
65.00	716.0
65.90	121.0
68.00	18568.0
69.00	18272.0
70.10	1148.0
71.00	104.0
72.00	1097.0
73.00	8213.0
74.00	31528.0
75.00	93216.0
76.00	7569.0
77.00	1084.0
78.00	757.0
78.90	5520.0
80.00	1709.0
81.00	5880.0
81.90	1489.0
82.80	121.0
85.80	312.0
87.00	7448.0
88.00	7771.0
90.90	699.0
92.00	5396.0
93.00	8015.0
94.10	22056.0
95.10	179200.0
96.10	12354.0
97.00	297.0
104.00	783.0
104.80	207.0
105.90	847.0
107.00	143.0
110.80	244.0
111.90	114.0
112.70	149.0
114.90	315.0
115.90	877.0
117.00	1361.0
117.90	719.0
118.90	1029.0
127.00	110.0
128.00	476.0
128.90	435.0
130.00	589.0
130.90	173.0
134.90	315.0
136.00	113.0
136.90	325.0
139.90	282.0
141.00	1994.0
141.90	192.0
143.00	1990.0
143.80	130.0
144.90	306.0
145.90	279.0
147.10	108.0
148.00	388.0
148.90	189.0
149.90	132.0
152.80	163.0
155.10	386.0
157.00	373.0
158.70	142.0
159.00	150.0
170.80	174.0
172.00	1161.0
174.00	140608.0
175.10	11570.0
176.00	138112.0

Instrument :
MSVOA_U
ClientSampleId :
BFB08

177.009581.0

178.00226.0

Instrument :
MSVOA_U
ClientSampleId :
BFB08

Scan 2880 (10.600 min): VU038561.D
BFB08

m/z	Abundance
40.00	170.0
44.00	730.0

Instrument :
MSVOA_U
ClientSampleId :
BFB08