

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060524\
 Data File : VU059153.D
 Acq On : 05 Jun 2024 17:14
 Operator : MD/SY
 Sample : VU0605WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0605WBL01

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U060524DW.M

Title : METHOD 524.2 VOLATILES DRINKING WATER

Signal : TIC: VU059153.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.785	457	465	478	rVB2	1397	2360	2.89%	0.993%
2	3.039	535	544	555	rBV2	4444	8175	10.01%	3.441%
3	4.634	1034	1040	1043	rBV3	1070	1334	1.63%	0.561%
4	4.653	1043	1046	1058	rVB5	993	1769	2.17%	0.745%
5	6.110	1487	1499	1519	rBV2	40364	81646	100.00%	34.365%
6	7.975	2073	2079	2083	rBV3	923	1102	1.35%	0.464%
7	9.434	2522	2533	2535	rBV3	933	1245	1.52%	0.524%
8	9.701	2610	2616	2626	rBV4	1080	1829	2.24%	0.770%
9	10.489	2853	2861	2867	rBV3	682	1031	1.26%	0.434%
10	10.634	2896	2906	2933	rBV3	27990	50909	62.35%	21.427%
11	10.991	3011	3017	3025	rVB3	670	881	1.08%	0.371%
12	11.753	3249	3254	3255	rBV2	1165	901	1.10%	0.379%
13	11.823	3271	3276	3277	rBV3	1437	1013	1.24%	0.426%
14	11.843	3277	3282	3293	rVB4	1950	3317	4.06%	1.396%
15	12.193	3380	3391	3413	rBV2	39319	71604	87.70%	30.138%
16	13.852	3901	3907	3911	rBV5	1390	1766	2.16%	0.743%
17	14.113	3977	3988	3996	rBV2	1152	2475	3.03%	1.042%
18	14.334	4048	4057	4058	rBV2	1232	1268	1.55%	0.534%
19	17.080	4907	4911	4917	rBV5	993	1219	1.49%	0.513%
20	17.141	4927	4930	4935	rBV4	870	842	1.03%	0.354%
21	17.215	4950	4953	4958	rVB4	956	902	1.10%	0.380%




Sum of corrected areas: 237588

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060524\
Data File : VU059153.D
Acq On : 05 Jun 2024 17:14
Operator : MD/SY
Sample : VU0605WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0605WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U060524DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

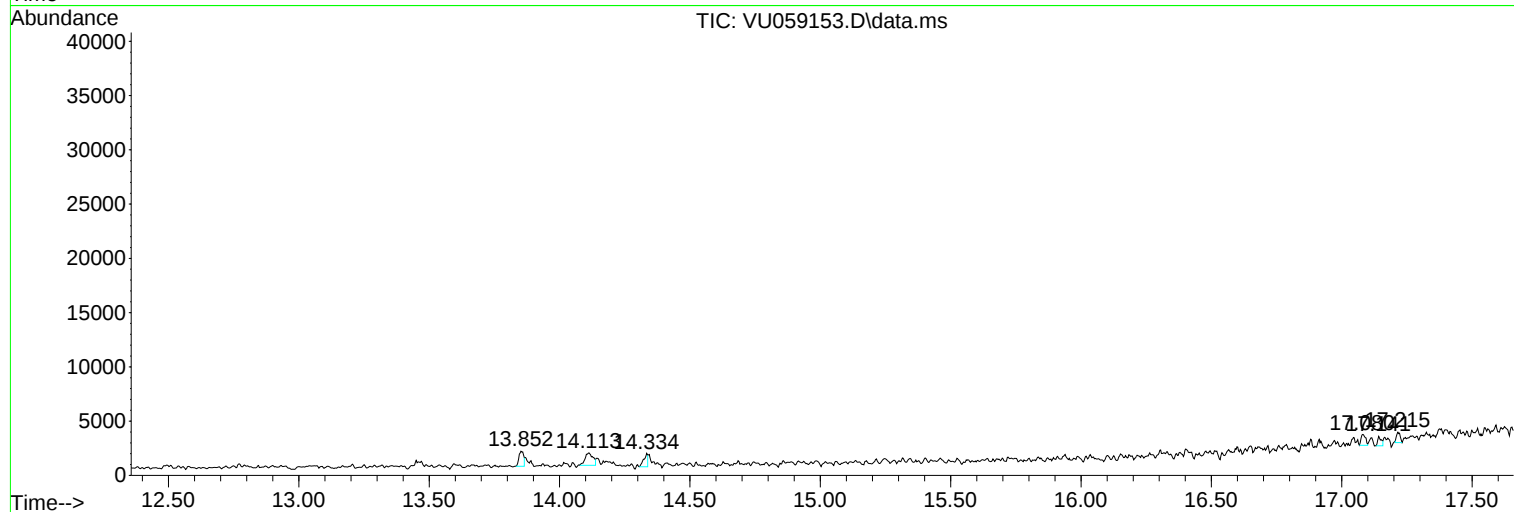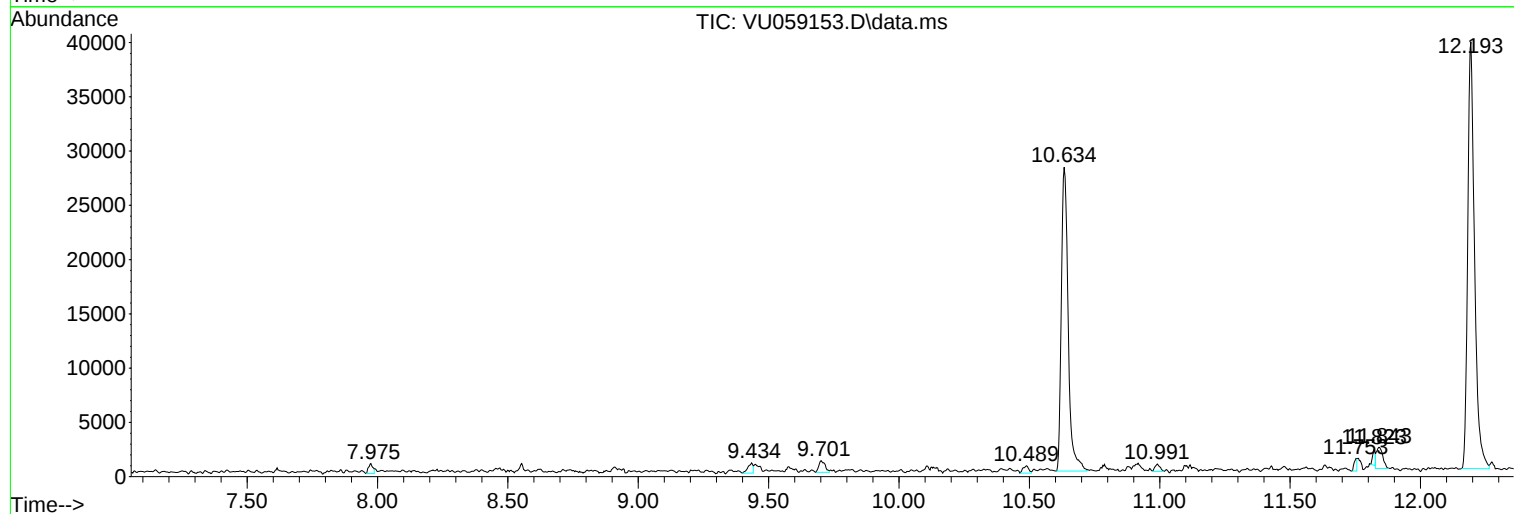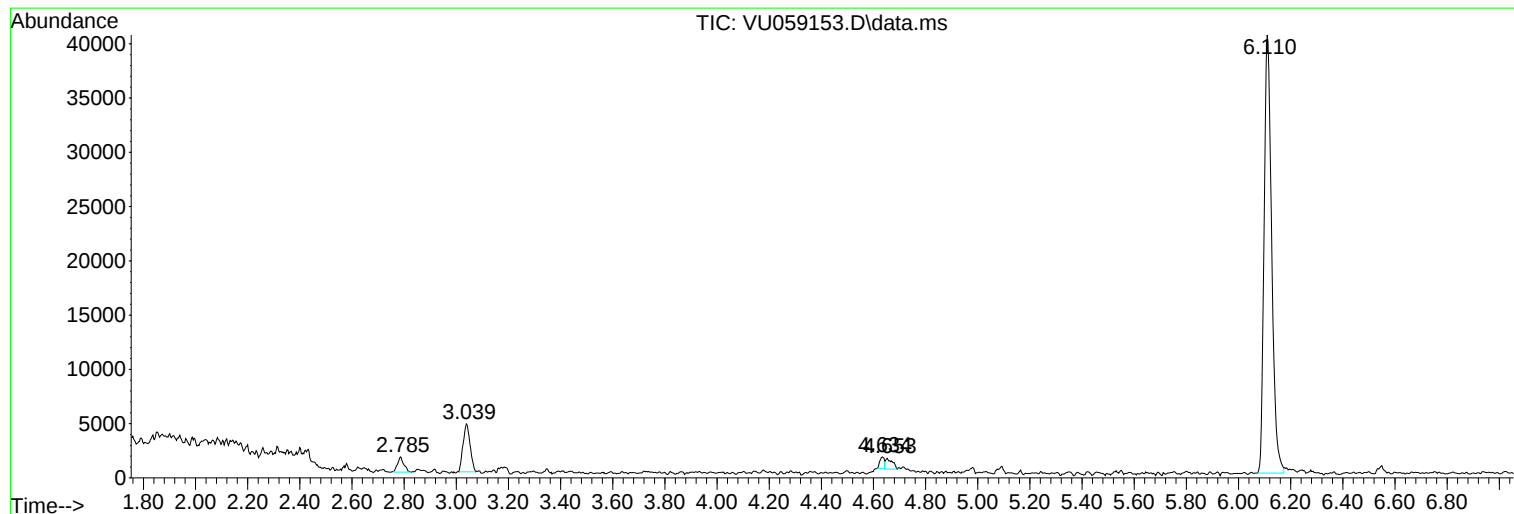

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060524\
Data File : VU059153.D
Acq On : 05 Jun 2024 17:14
Operator : MD/SY
Sample : VU0605WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0605WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U060524DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060524\
Data File : VU059153.D
Acq On : 05 Jun 2024 17:14
Operator : MD/SY
Sample : VU0605WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0605WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U060524DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------