


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060524\
Data File : VU059143.D
Acq On : 05 Jun 2024 08:27
Operator : MD/SY
Sample : BFB
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U060524DW.M
Title : METHOD 524.2 VOLATILES DRINKING WATER
Last Update : Thu Jun 06 08:51:44 2024

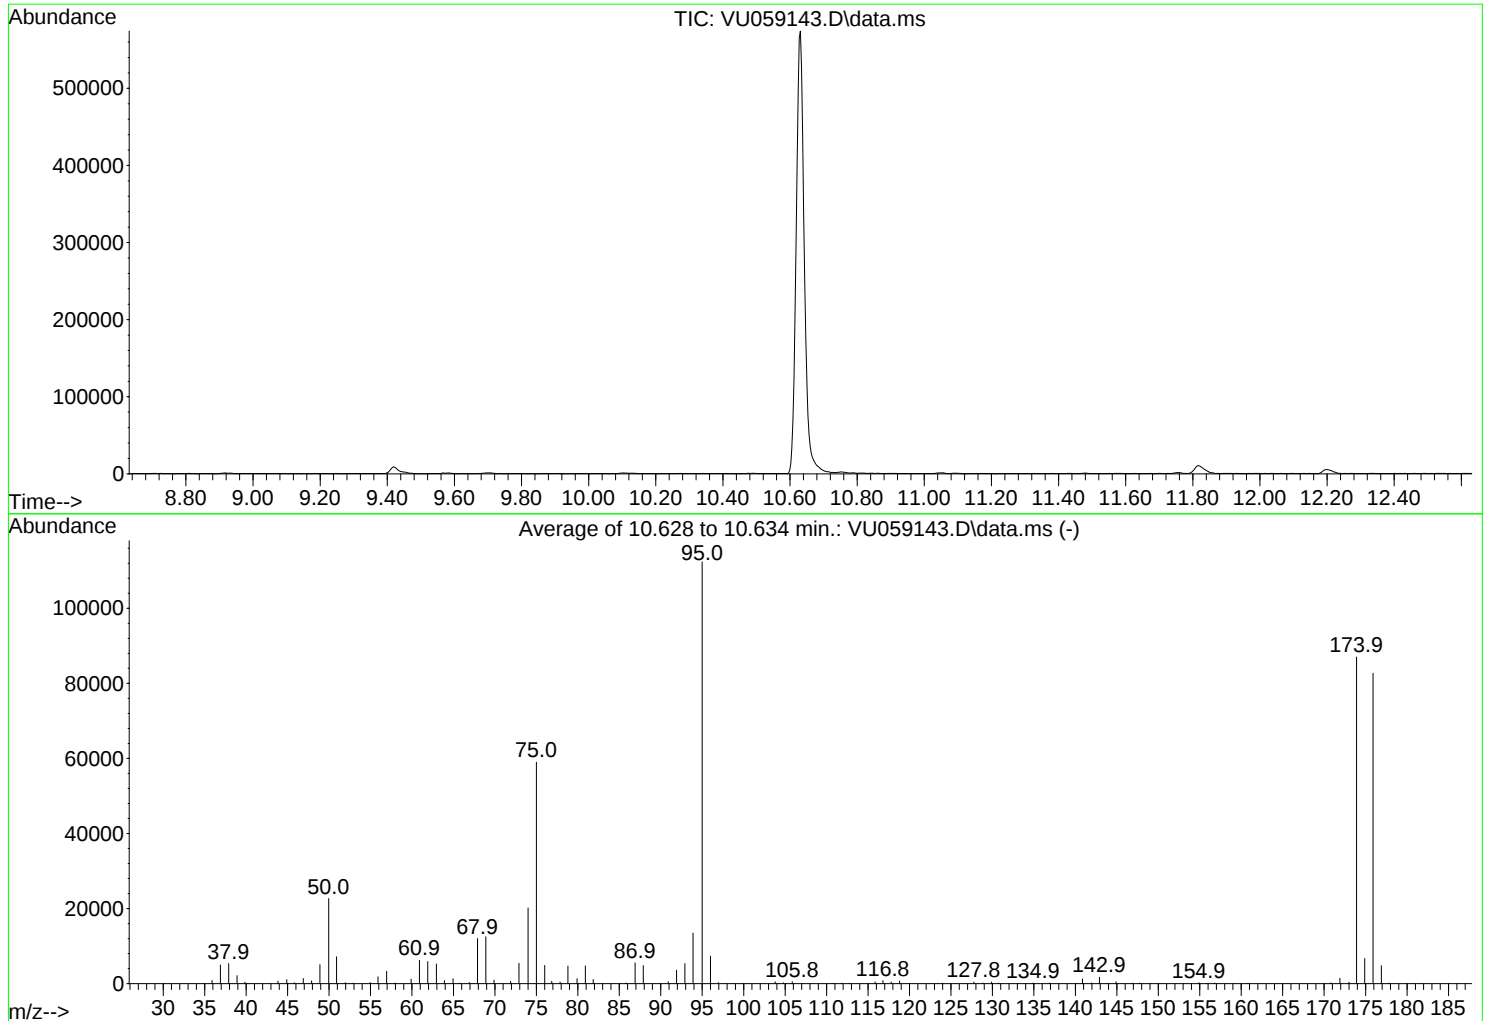

AutoFind: Scans 2904, 2905, 2906; Background Corrected with Scan 2891

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.2	22680	PASS
75	95	30	60	52.5	59019	PASS
95	95	100	100	100.0	112376	PASS
96	95	5	9	6.5	7355	PASS
173	174	0.00	2	0.4	377	PASS
174	95	50	100	77.4	86997	PASS
175	174	5	9	7.7	6691	PASS
176	174	95	101	95.0	82688	PASS
177	176	5	9	5.8	4794	PASS