

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU060619\
 Data File : VU032472.D
 Acq On : 05 Jun 2019 19:43
 Operator : JC/SP
 Sample : K3213-10 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DB8K0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060619WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.396	88	95	104	rVB	82728	83463	11.85%	1.431%
2	1.672	175	181	196	rVB	68318	85497	12.14%	1.466%
3	2.267	357	366	379	rVB	145429	222780	31.64%	3.819%
4	2.412	410	411	414	rVB2	315	136	0.02%	0.002%
5	2.601	467	470	472	rVB	310	138	0.02%	0.002%
6	2.640	480	482	484	rVB	269	89	0.01%	0.002%
7	2.695	495	499	503	rBV3	530	363	0.05%	0.006%
8	2.830	529	541	557	rVB2	5628	11879	1.69%	0.204%
9	3.039	604	606	610	rBV	180	132	0.02%	0.002%
10	3.080	617	619	621	rBV	130	89	0.01%	0.002%
11	3.177	642	649	651	rBV3	686	826	0.12%	0.014%
12	3.244	667	670	674	rBV2	235	216	0.03%	0.004%
13	3.550	760	765	767	rBV	189	123	0.02%	0.002%
14	3.653	789	797	800	rBV	100	141	0.02%	0.002%
15	3.682	803	806	810	rVB	213	136	0.02%	0.002%
16	3.875	864	866	869	rVV	181	100	0.01%	0.002%
17	3.897	871	873	877	rVV	293	123	0.02%	0.002%
18	3.920	877	880	884	rVB	206	121	0.02%	0.002%
19	3.994	892	903	923	rBV6	4761	13423	1.91%	0.230%
20	4.170	947	958	995	rBV	69280	189053	26.85%	3.241%
21	4.640	1088	1104	1126	rBV	113967	271723	38.59%	4.658%
22	4.842	1164	1167	1169	rBV2	415	272	0.04%	0.005%
23	4.926	1190	1193	1198	rBV2	169	165	0.02%	0.003%
24	4.965	1202	1205	1210	rBV2	225	170	0.02%	0.003%
25	5.003	1214	1217	1219	rBV2	119	98	0.01%	0.002%
26	5.087	1242	1243	1248	rVB	208	126	0.02%	0.002%
27	5.122	1249	1254	1256	rBV	159	133	0.02%	0.002%
28	5.177	1266	1271	1275	rBV	162	135	0.02%	0.002%
29	5.334	1297	1320	1348	rBV2	240960	704218	100.00%	12.071%
30	5.717	1436	1439	1443	rBV2	276	238	0.03%	0.004%
31	5.781	1456	1459	1463	rVB2	237	152	0.02%	0.003%
32	5.826	1471	1473	1475	rBV	168	97	0.01%	0.002%
33	5.881	1477	1490	1512	rBV	233856	459079	65.19%	7.869%
34	6.177	1573	1582	1596	rVB5	3575	7253	1.03%	0.124%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\U060619\
 Data File : VU032472.D
 Acq On : 05 Jun 2019 19:43
 Operator : JC/SP
 Sample : K3213-10 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DB8K0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060619WMA.M
 Title : VOC Analysis

35	6.325	1614	1628	1653	rVV	157994	316448	44.94%	5.424%
36	6.530	1688	1692	1697	rBV3	214	172	0.02%	0.003%
37	6.627	1718	1722	1726	rVV	245	243	0.03%	0.004%
38	6.662	1729	1733	1737	rBV2	196	218	0.03%	0.004%
39	6.752	1758	1761	1765	rBV2	172	140	0.02%	0.002%
40	6.984	1831	1833	1838	rBV	197	131	0.02%	0.002%
41	7.032	1843	1848	1850	rBV2	180	196	0.03%	0.003%
42	7.071	1856	1860	1866	rVB2	260	226	0.03%	0.004%
43	7.222	1896	1907	1931	rBV	91079	167828	23.83%	2.877%
44	7.405	1961	1964	1966	rBV	231	184	0.03%	0.003%
45	7.476	1984	1986	1990	rBV2	205	105	0.01%	0.002%
46	7.498	1990	1993	1995	rBV2	131	91	0.01%	0.002%
47	7.559	1999	2012	2031	rBV	339088	590148	83.80%	10.116%
48	7.846	2091	2101	2125	rBV	62653	110478	15.69%	1.894%
49	8.058	2165	2167	2170	rBV	130	96	0.01%	0.002%
50	8.241	2221	2224	2228	rBV	113	88	0.01%	0.002%
51	8.264	2229	2231	2234	rVB	206	96	0.01%	0.002%
52	8.305	2234	2244	2280	rBV	210478	395246	56.13%	6.775%
53	8.569	2323	2326	2332	rVB3	376	413	0.06%	0.007%
54	8.614	2332	2340	2349	rVB4	1246	2170	0.31%	0.037%
55	8.739	2376	2379	2381	rBV2	178	134	0.02%	0.002%
56	8.755	2381	2384	2388	rVV	162	144	0.02%	0.002%
57	8.794	2393	2396	2400	rBV2	137	144	0.02%	0.002%
58	8.887	2420	2425	2429	rVB2	238	243	0.03%	0.004%
59	8.942	2439	2442	2444	rBV2	211	152	0.02%	0.003%
60	9.083	2474	2486	2523	rBV	341351	575624	81.74%	9.867%
61	9.302	2549	2554	2556	rBV3	313	336	0.05%	0.006%
62	9.370	2566	2575	2588	rVB4	5866	10724	1.52%	0.184%
63	9.421	2588	2591	2593	rVB	272	149	0.02%	0.003%
64	9.527	2621	2624	2626	rBV	178	149	0.02%	0.003%
65	9.611	2644	2650	2651	rBV2	279	244	0.03%	0.004%
66	9.797	2706	2708	2709	rBV2	303	153	0.02%	0.003%
67	9.890	2735	2737	2740	rBV2	143	88	0.01%	0.002%
68	10.019	2772	2777	2779	rBV	172	178	0.03%	0.003%
69	10.074	2790	2794	2797	rBV	204	188	0.03%	0.003%
70	10.125	2809	2810	2815	rVB	225	89	0.01%	0.002%
71	10.157	2816	2820	2823	rBV2	389	336	0.05%	0.006%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU060619\
 Data File : VU032472.D
 Acq On : 05 Jun 2019 19:43
 Operator : JC/SP
 Sample : K3213-10 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DB8K0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060619WMA.M
 Title : VOC Analysis

72	10.189	2827	2830	2834	rVB	176	98	0.01%	0.002%
73	10.228	2839	2842	2845	rVB	189	109	0.02%	0.002%
74	10.247	2845	2848	2849	rBV2	154	87	0.01%	0.001%
75	10.427	2883	2904	2921	rBV	230020	396935	56.37%	6.804%
76	10.543	2937	2940	2942	rBV	157	101	0.01%	0.002%
77	10.640	2968	2970	2979	rVB3	484	598	0.08%	0.010%
78	10.675	2979	2981	2983	rBV	296	158	0.02%	0.003%
79	10.781	3006	3014	3023	rVB3	4149	5908	0.84%	0.101%
80	10.829	3023	3029	3032	rBV2	307	267	0.04%	0.005%
81	10.951	3064	3067	3071	rVV2	209	169	0.02%	0.003%
82	11.141	3124	3126	3128	rBV2	246	87	0.01%	0.001%
83	11.196	3139	3143	3149	rBV	351	315	0.04%	0.005%
84	11.222	3149	3151	3153	rVV	215	105	0.01%	0.002%
85	11.405	3202	3208	3215	rBV7	1705	2345	0.33%	0.040%
86	11.479	3219	3231	3241	rBV	352334	573465	81.43%	9.830%
87	11.723	3300	3307	3315	rBV3	4507	6717	0.95%	0.115%
88	11.855	3336	3348	3362	rBV	353058	573040	81.37%	9.823%
89	12.151	3438	3440	3441	rVB	426	144	0.02%	0.002%
90	12.257	3468	3473	3477	rBV3	1311	1334	0.19%	0.023%
91	12.405	3516	3519	3532	rVB4	1211	2268	0.32%	0.039%
92	12.495	3540	3547	3549	rBV3	1263	1317	0.19%	0.023%
93	12.691	3594	3608	3620	rBV2	6941	11895	1.69%	0.204%
94	12.784	3626	3637	3649	rBV4	6139	10589	1.50%	0.182%
95	12.865	3660	3662	3663	rBV4	362	155	0.02%	0.003%
96	13.109	3734	3738	3741	rBV3	395	282	0.04%	0.005%
97	13.167	3751	3756	3764	rVB5	1718	2267	0.32%	0.039%
98	13.218	3769	3772	3774	rVB2	415	209	0.03%	0.004%
99	13.588	3884	3887	3890	rBV2	470	369	0.05%	0.006%
100	13.649	3897	3906	3920	rBV2	9586	16127	2.29%	0.276%


Sum of corrected areas: 5833939

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU060619\
Data File : VU032472.D
Acq On : 05 Jun 2019 19:43
Operator : JC/SP
Sample : K3213-10 50X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DB8K0

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060619WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

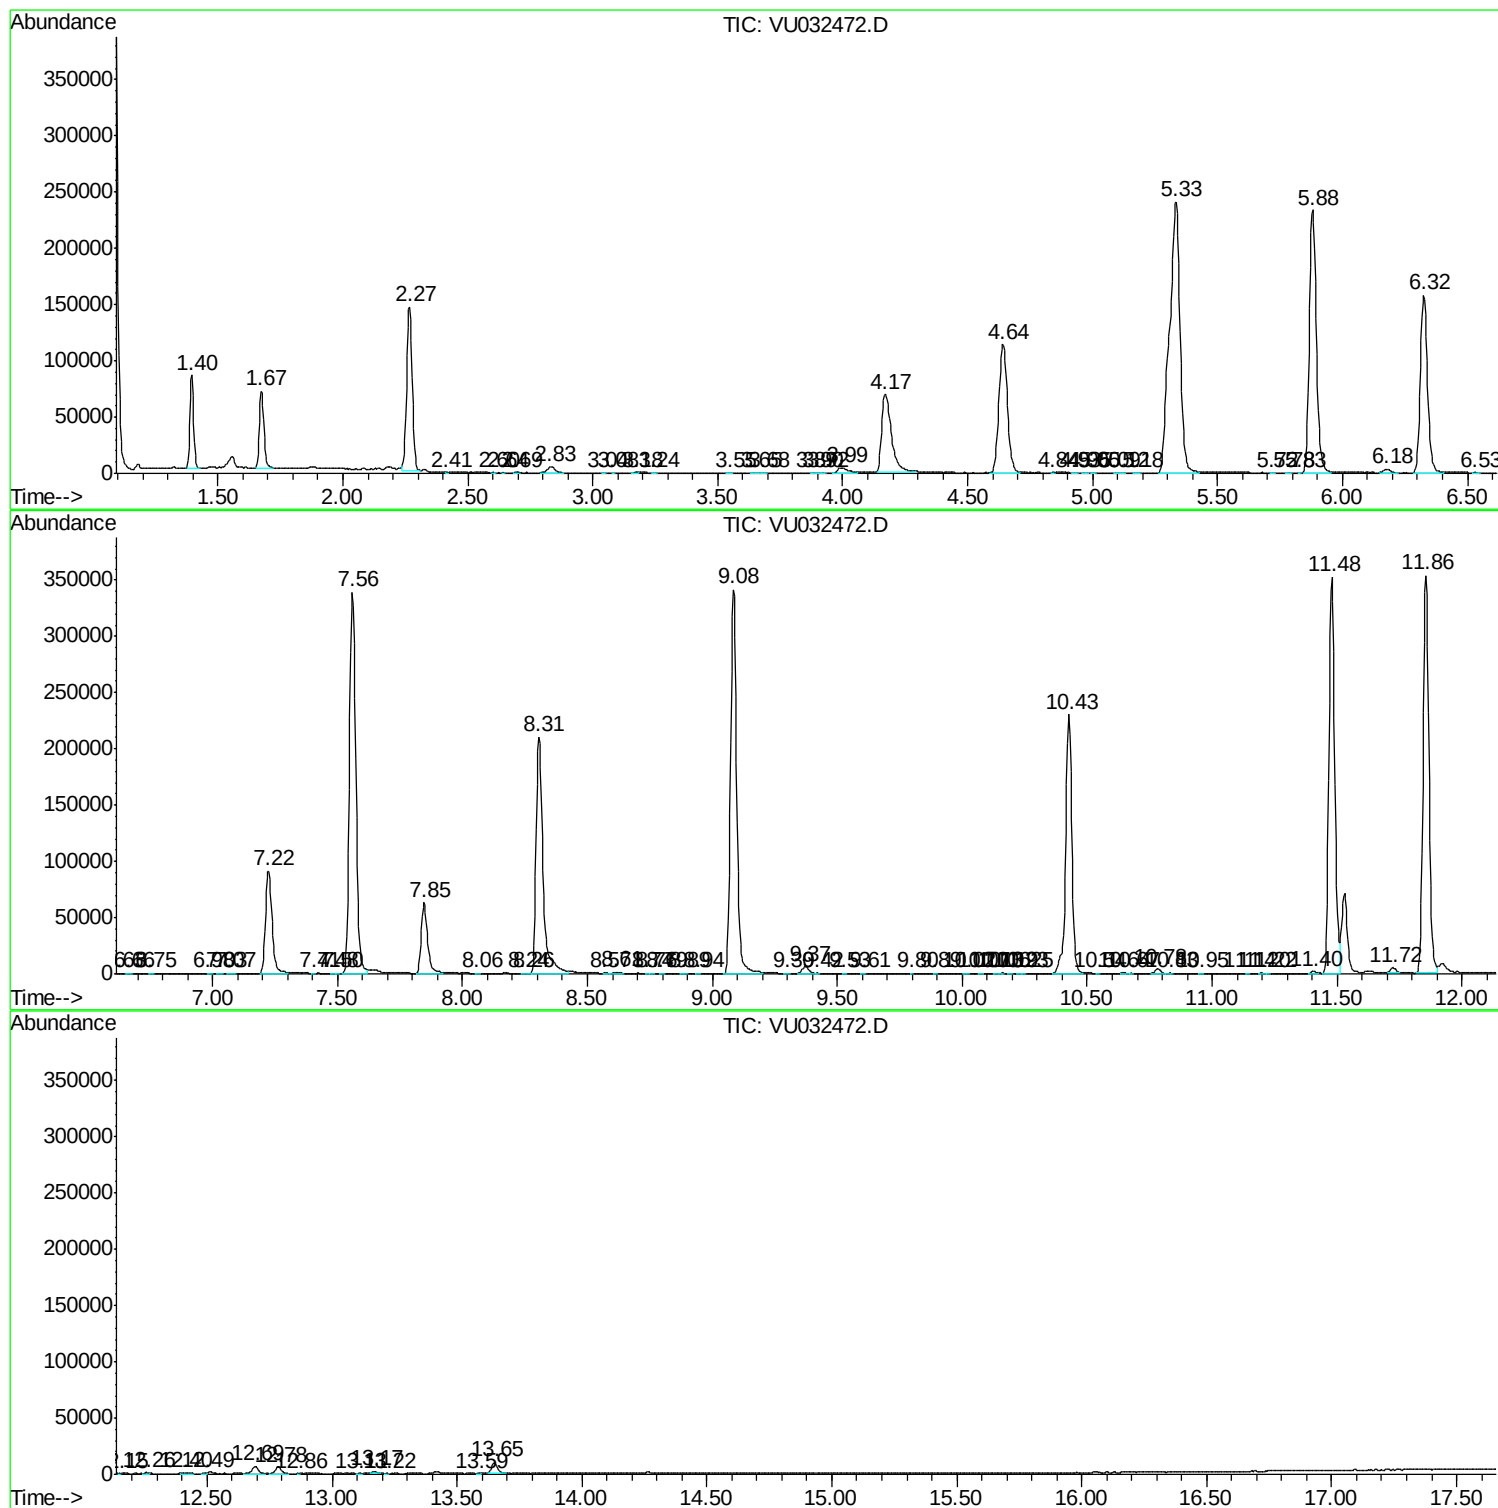

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU060619\
Data File : VU032472.D
Acq On : 05 Jun 2019 19:43
Operator : JC/SP
Sample : K3213-10 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DB8K0

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060619WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU060619\
Data File : VU032472.D
Acq On : 05 Jun 2019 19:43
Operator : JC/SP
Sample : K3213-10 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DB8K0

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060619WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
