

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU060619\
 Data File : VU032476.D
 Acq On : 05 Jun 2019 21:15
 Operator : JC/SP
 Sample : K3213-14 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DB8K5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060619WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.392	88	94	107	rBV	78648	84125	11.98%	1.457%
2	1.672	175	181	194	rVB	68658	84204	11.99%	1.459%
3	2.267	356	366	378	rVB	144364	221641	31.56%	3.839%
4	2.830	532	541	562	rVB	7052	15092	2.15%	0.261%
5	2.904	562	564	567	rBV2	148	69	0.01%	0.001%
6	2.974	584	586	590	rBV	291	134	0.02%	0.002%
7	3.035	604	605	609	rBV	137	68	0.01%	0.001%
8	3.125	630	633	634	rBV	127	80	0.01%	0.001%
9	3.215	658	661	662	rBV	163	97	0.01%	0.002%
10	3.611	782	784	787	rBV	114	76	0.01%	0.001%
11	3.662	798	800	804	rVB2	168	95	0.01%	0.002%
12	3.688	805	808	810	rVV	195	126	0.02%	0.002%
13	3.704	810	813	819	rVV	249	207	0.03%	0.004%
14	3.730	819	821	823	rVV2	193	110	0.02%	0.002%
15	3.746	823	826	829	rVV	211	163	0.02%	0.003%
16	3.775	833	835	840	rVB	210	116	0.02%	0.002%
17	3.868	860	864	870	rVB	259	236	0.03%	0.004%
18	3.910	874	877	885	rVB	353	350	0.05%	0.006%
19	3.952	887	890	893	rBV	202	118	0.02%	0.002%
20	4.055	920	922	925	rVB2	119	69	0.01%	0.001%
21	4.084	929	931	935	rVB	221	140	0.02%	0.002%
22	4.116	937	941	942	rBV	129	84	0.01%	0.001%
23	4.170	944	958	987	rBV	75029	204835	29.17%	3.548%
24	4.640	1088	1104	1129	rBV	115572	270601	38.54%	4.687%
25	4.794	1150	1152	1158	rBV2	318	275	0.04%	0.005%
26	4.932	1193	1195	1198	rBV	264	193	0.03%	0.003%
27	5.174	1267	1270	1274	rBV2	174	150	0.02%	0.003%
28	5.212	1277	1282	1286	rVB	158	158	0.02%	0.003%
29	5.247	1290	1293	1296	rBV	97	61	0.01%	0.001%
30	5.334	1296	1320	1348	rBV2	239986	702198	100.00%	12.163%
31	5.727	1438	1442	1443	rVV	150	97	0.01%	0.002%
32	5.752	1448	1450	1452	rBV	160	63	0.01%	0.001%
33	5.775	1455	1457	1462	rVB	175	107	0.02%	0.002%
34	5.794	1462	1463	1467	rBV2	228	153	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU060619\
 Data File : VU032476.D
 Acq On : 05 Jun 2019 21:15
 Operator : JC/SP
 Sample : K3213-14 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DB8K5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060619WMA.M
 Title : VOC Analysis

35	5.881	1476	1490	1516	rBV	240000	470030	66.94%	8.142%
36	6.173	1573	1581	1593	rVB2	2978	6131	0.87%	0.106%
37	6.325	1613	1628	1648	rBV	158574	315357	44.91%	5.463%
38	6.424	1657	1659	1665	rVB3	396	401	0.06%	0.007%
39	6.456	1665	1669	1672	rBV3	270	206	0.03%	0.004%
40	6.566	1700	1703	1706	rBV2	262	218	0.03%	0.004%
41	6.608	1712	1716	1717	rBV2	191	127	0.02%	0.002%
42	6.727	1750	1753	1756	rVB	128	89	0.01%	0.002%
43	6.768	1759	1766	1769	rBV2	254	265	0.04%	0.005%
44	6.810	1775	1779	1780	rBV	172	75	0.01%	0.001%
45	6.833	1784	1786	1790	rVB	179	100	0.01%	0.002%
46	6.855	1790	1793	1797	rBV	102	82	0.01%	0.001%
47	6.894	1802	1805	1808	rBV2	215	212	0.03%	0.004%
48	6.929	1813	1816	1817	rBV	145	90	0.01%	0.002%
49	7.112	1870	1873	1878	rBV	100	89	0.01%	0.002%
50	7.222	1896	1907	1927	rBV	92106	168028	23.93%	2.911%
51	7.482	1984	1988	1992	rBV	317	235	0.03%	0.004%
52	7.559	1999	2012	2036	rBV	335925	582796	83.00%	10.095%
53	7.800	2086	2087	2089	rVB	281	91	0.01%	0.002%
54	7.845	2090	2101	2123	rBV	62389	109981	15.66%	1.905%
55	8.077	2169	2173	2174	rBV	119	86	0.01%	0.001%
56	8.222	2217	2218	2222	rBV2	222	101	0.01%	0.002%
57	8.257	2226	2229	2231	rBV	212	161	0.02%	0.003%
58	8.305	2234	2244	2290	rBV	219372	409178	58.27%	7.088%
59	8.543	2316	2318	2320	rVB2	428	193	0.03%	0.003%
60	8.617	2334	2341	2347	rBV3	1650	2671	0.38%	0.046%
61	8.665	2353	2356	2363	rVB2	200	161	0.02%	0.003%
62	8.707	2363	2369	2370	rBV	212	182	0.03%	0.003%
63	8.794	2392	2396	2397	rBV	164	128	0.02%	0.002%
64	8.839	2407	2410	2411	rBV	185	111	0.02%	0.002%
65	8.929	2436	2438	2440	rBV	144	85	0.01%	0.001%
66	9.083	2474	2486	2527	rBV	348207	582122	82.90%	10.083%
67	9.392	2577	2582	2583	rBV2	249	172	0.02%	0.003%
68	9.405	2583	2586	2589	rVB	156	93	0.01%	0.002%
69	9.424	2589	2592	2594	rBV2	200	149	0.02%	0.003%
70	9.505	2614	2617	2622	rBV2	202	238	0.03%	0.004%
71	9.633	2655	2657	2658	rBV2	192	84	0.01%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU060619\
 Data File : VU032476.D
 Acq On : 05 Jun 2019 21:15
 Operator : JC/SP
 Sample : K3213-14 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DB8K5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060619WMA.M
 Title : VOC Analysis

72	9.662	2663	2666	2669	rVV2	193	122	0.02%	0.002%
73	9.688	2671	2674	2682	rVB2	144	141	0.02%	0.002%
74	9.746	2689	2692	2695	rBV	192	168	0.02%	0.003%
75	9.826	2714	2717	2718	rBV	150	86	0.01%	0.001%
76	9.932	2746	2750	2753	rVB	173	141	0.02%	0.002%
77	9.951	2753	2756	2759	rVB	242	124	0.02%	0.002%
78	10.000	2767	2771	2780	rVB2	256	328	0.05%	0.006%
79	10.058	2786	2789	2793	rVB	212	144	0.02%	0.002%
80	10.080	2794	2796	2802	rVB2	215	190	0.03%	0.003%
81	10.109	2802	2805	2808	rVB	220	142	0.02%	0.002%
82	10.144	2808	2816	2819	rBV2	339	406	0.06%	0.007%
83	10.209	2834	2836	2839	rBV	173	128	0.02%	0.002%
84	10.344	2875	2878	2881	rVB	271	198	0.03%	0.003%
85	10.427	2892	2904	2929	rBV	235385	379197	54.00%	6.568%
86	10.537	2936	2938	2943	rVB	244	161	0.02%	0.003%
87	10.585	2950	2953	2954	rBV	274	126	0.02%	0.002%
88	10.665	2976	2978	2983	rVB2	207	142	0.02%	0.002%
89	10.707	2987	2991	2996	rVB	238	238	0.03%	0.004%
90	10.781	3012	3014	3017	rBV2	172	86	0.01%	0.001%
91	10.836	3029	3031	3034	rBV	161	72	0.01%	0.001%
92	11.074	3103	3105	3110	rVB	266	241	0.03%	0.004%
93	11.347	3188	3190	3193	rBV	164	119	0.02%	0.002%
94	11.363	3193	3195	3201	rVV	216	128	0.02%	0.002%
95	11.424	3212	3214	3218	rVB2	152	103	0.01%	0.002%
96	11.479	3219	3231	3257	rBV	359232	581011	82.74%	10.064%
97	11.855	3335	3348	3375	rBV	345682	571896	81.44%	9.906%
98	12.295	3483	3485	3488	rVB	218	85	0.01%	0.001%
99	12.318	3488	3492	3493	rBV	256	156	0.02%	0.003%
100	13.209	3767	3769	3772	rBV	310	181	0.03%	0.003%


Sum of corrected areas: 5773069

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU060619\
Data File : VU032476.D
Acq On : 05 Jun 2019 21:15
Operator : JC/SP
Sample : K3213-14 50X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DB8K5

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060619WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

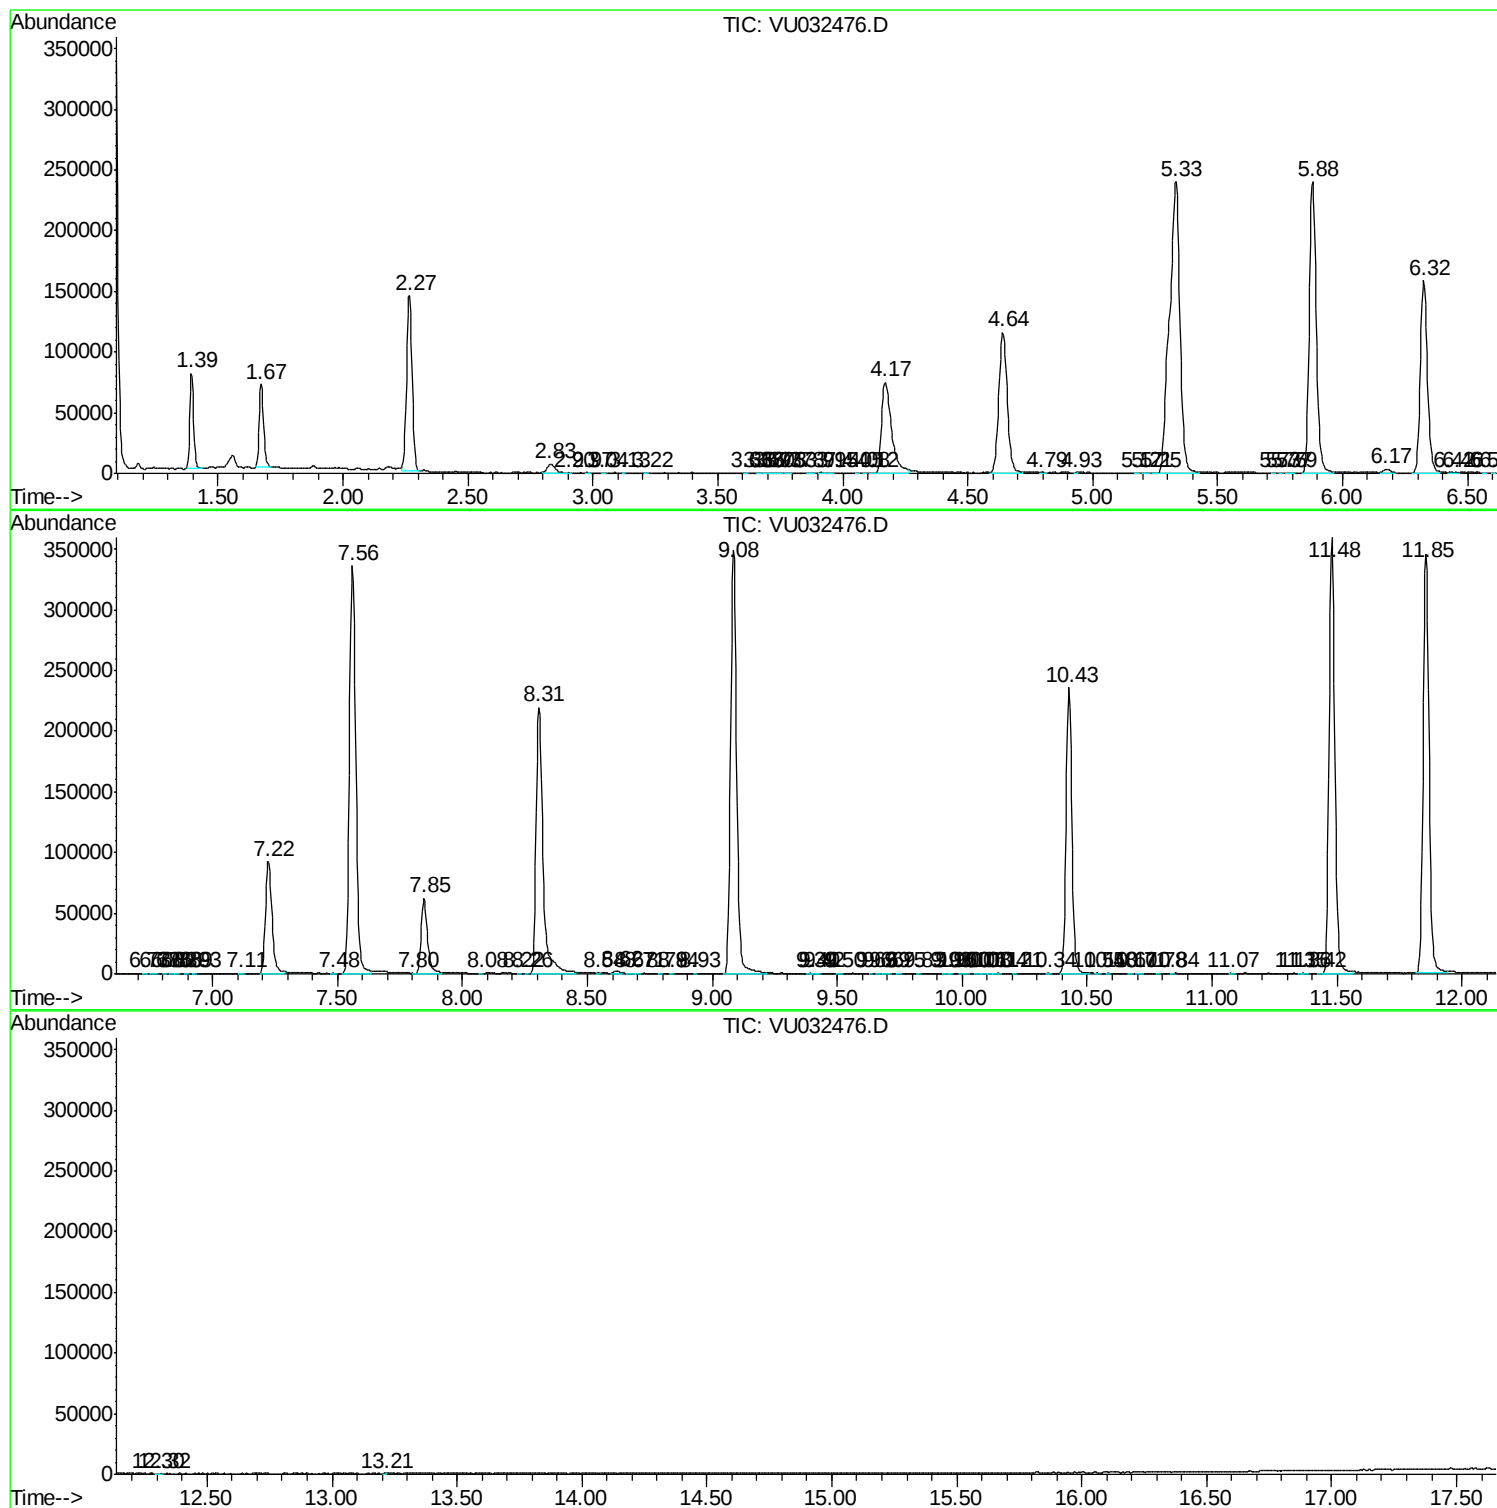

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU060619\
Data File : VU032476.D
Acq On : 05 Jun 2019 21:15
Operator : JC/SP
Sample : K3213-14 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DB8K5

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060619WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU060619\
Data File : VU032476.D
Acq On : 05 Jun 2019 21:15
Operator : JC/SP
Sample : K3213-14 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DB8K5

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060619WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc