

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU060619\
 Data File : VU032487.D
 Acq On : 06 Jun 2019 11:26
 Operator : JC/SP
 Sample : K3213-05
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DB8H8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060619WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.396	89	95	112	rVB	77687	81780	11.58%	1.423%
2	1.675	176	182	195	rVB	68314	83222	11.79%	1.449%
3	2.267	357	366	379	rVB	148231	222136	31.46%	3.867%
4	2.447	414	422	425	rBV6	714	1047	0.15%	0.018%
5	2.694	496	499	501	rBV	455	268	0.04%	0.005%
6	2.752	513	517	520	rBV2	259	227	0.03%	0.004%
7	2.894	559	561	564	rBV	148	110	0.02%	0.002%
8	2.971	583	585	586	rBV	274	70	0.01%	0.001%
9	3.000	592	594	596	rBV2	152	89	0.01%	0.002%
10	3.064	609	614	618	rBV2	234	232	0.03%	0.004%
11	3.309	687	690	692	rVB2	135	77	0.01%	0.001%
12	3.389	713	715	718	rVB	274	127	0.02%	0.002%
13	3.424	723	726	727	rBV	196	113	0.02%	0.002%
14	3.447	730	733	736	rVV	343	206	0.03%	0.004%
15	3.489	741	746	749	rBV	194	223	0.03%	0.004%
16	3.569	770	771	776	rVB	140	71	0.01%	0.001%
17	3.595	776	779	782	rBV	163	95	0.01%	0.002%
18	3.614	782	785	789	rBV	144	103	0.01%	0.002%
19	3.637	789	792	795	rBV2	146	141	0.02%	0.002%
20	3.739	822	824	827	rVB2	129	75	0.01%	0.001%
21	3.765	827	832	837	rVB2	231	215	0.03%	0.004%
22	3.810	840	846	848	rBV	111	90	0.01%	0.002%
23	3.826	848	851	854	rBV2	265	210	0.03%	0.004%
24	4.167	945	957	991	rBV	63523	168732	23.90%	2.937%
25	4.640	1087	1104	1127	rBV	116235	272618	38.61%	4.745%
26	4.839	1164	1166	1171	rBV2	382	285	0.04%	0.005%
27	4.874	1173	1177	1183	rBV4	612	801	0.11%	0.014%
28	5.035	1225	1227	1228	rBV4	217	96	0.01%	0.002%
29	5.083	1237	1242	1245	rBV2	210	194	0.03%	0.003%
30	5.186	1271	1274	1278	rBV	88	84	0.01%	0.001%
31	5.209	1278	1281	1284	rBV	129	86	0.01%	0.001%
32	5.257	1293	1296	1297	rBV	129	78	0.01%	0.001%
33	5.331	1297	1319	1350	rBV2	240253	705996	100.00%	12.289%
34	5.878	1477	1489	1521	rBV	245755	484227	68.59%	8.429%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU060619\
 Data File : VU032487.D
 Acq On : 06 Jun 2019 11:26
 Operator : JC/SP
 Sample : K3213-05
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DB8H8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060619WMA.M
 Title : VOC Analysis

35	6.180	1573	1583	1594	rVB6	3251	7082	1.00%	0.123%
36	6.325	1614	1628	1656	rBV	157904	315055	44.63%	5.484%
37	6.617	1715	1719	1722	rVB	131	79	0.01%	0.001%
38	6.704	1744	1746	1749	rBV	126	74	0.01%	0.001%
39	6.749	1756	1760	1763	rVB2	159	144	0.02%	0.003%
40	6.826	1780	1784	1787	rBV	181	130	0.02%	0.002%
41	6.855	1790	1793	1799	rBV	66	85	0.01%	0.001%
42	6.903	1805	1808	1816	rVB	238	327	0.05%	0.006%
43	6.980	1829	1832	1836	rBV	252	170	0.02%	0.003%
44	7.019	1839	1844	1849	rBV2	214	188	0.03%	0.003%
45	7.045	1849	1852	1855	rBV	117	89	0.01%	0.002%
46	7.071	1859	1860	1863	rVB	218	90	0.01%	0.002%
47	7.103	1863	1870	1872	rBV	93	98	0.01%	0.002%
48	7.151	1883	1885	1888	rVB2	137	80	0.01%	0.001%
49	7.183	1891	1895	1896	rBV2	229	157	0.02%	0.003%
50	7.222	1896	1907	1934	rBV2	93066	171546	24.30%	2.986%
51	7.559	1999	2012	2034	rBV	342088	594117	84.15%	10.341%
52	7.845	2088	2101	2124	rBV	63890	114792	16.26%	1.998%
53	8.067	2167	2170	2171	rBV	323	167	0.02%	0.003%
54	8.135	2188	2191	2193	rVB	166	97	0.01%	0.002%
55	8.193	2206	2209	2214	rVB3	388	318	0.05%	0.006%
56	8.228	2214	2220	2228	rBV3	1057	1122	0.16%	0.020%
57	8.305	2233	2244	2287	rBV	194708	378075	53.55%	6.581%
58	8.556	2319	2322	2326	rVB2	340	332	0.05%	0.006%
59	8.578	2326	2329	2332	rBV2	147	95	0.01%	0.002%
60	8.607	2332	2338	2342	rVB3	332	312	0.04%	0.005%
61	8.636	2343	2347	2350	rBV	254	189	0.03%	0.003%
62	8.710	2367	2370	2377	rVB	284	256	0.04%	0.004%
63	8.746	2377	2381	2383	rBV	132	102	0.01%	0.002%
64	8.759	2383	2385	2387	rBV	111	78	0.01%	0.001%
65	8.804	2397	2399	2403	rVB	129	78	0.01%	0.001%
66	8.842	2406	2411	2414	rVV2	210	192	0.03%	0.003%
67	8.926	2434	2437	2439	rBV	196	91	0.01%	0.002%
68	8.945	2439	2443	2449	rVB2	210	251	0.04%	0.004%
69	9.083	2474	2486	2534	rBV	352793	598334	84.75%	10.415%
70	9.283	2543	2548	2552	rBV3	291	328	0.05%	0.006%
71	9.344	2565	2567	2572	rVB2	195	153	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU060619\
 Data File : VU032487.D
 Acq On : 06 Jun 2019 11:26
 Operator : JC/SP
 Sample : K3213-05
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DB8H8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060619WMA.M
 Title : VOC Analysis

72	9.382	2577	2579	2580	rBV2	239	95	0.01%	0.002%
73	9.402	2582	2585	2588	rVV2	199	124	0.02%	0.002%
74	9.424	2588	2592	2596	rVB	136	94	0.01%	0.002%
75	9.453	2597	2601	2605	rVB2	187	173	0.02%	0.003%
76	9.505	2615	2617	2618	rBV	131	74	0.01%	0.001%
77	9.562	2633	2635	2639	rVB	210	87	0.01%	0.002%
78	9.816	2711	2714	2720	rVB2	225	201	0.03%	0.003%
79	9.845	2720	2723	2725	rVB2	201	115	0.02%	0.002%
80	9.874	2729	2732	2736	rVB2	275	226	0.03%	0.004%
81	9.903	2737	2741	2743	rBV	158	143	0.02%	0.002%
82	10.177	2824	2826	2830	rBV2	184	133	0.02%	0.002%
83	10.331	2870	2874	2876	rBV	163	86	0.01%	0.001%
84	10.427	2892	2904	2928	rBV	226822	369153	52.29%	6.426%
85	10.611	2956	2961	2963	rBV	222	204	0.03%	0.004%
86	10.668	2977	2979	2983	rVB	153	72	0.01%	0.001%
87	10.823	3025	3027	3030	rBV	176	127	0.02%	0.002%
88	10.906	3050	3053	3056	rVB2	179	130	0.02%	0.002%
89	10.951	3063	3067	3068	rBV2	223	105	0.01%	0.002%
90	11.151	3122	3129	3140	rBV3	2429	3425	0.49%	0.060%
91	11.218	3147	3150	3152	rBV	226	110	0.02%	0.002%
92	11.379	3196	3200	3201	rBV	262	206	0.03%	0.004%
93	11.479	3219	3231	3259	rBV	365784	593230	84.03%	10.326%
94	11.800	3328	3331	3332	rBV2	405	261	0.04%	0.005%
95	11.855	3336	3348	3366	rBV	341589	566479	80.24%	9.860%
96	12.424	3520	3525	3529	rBV	310	330	0.05%	0.006%
97	12.553	3562	3565	3568	rBV	182	121	0.02%	0.002%
98	12.630	3587	3589	3594	rVB	199	193	0.03%	0.003%
99	12.980	3696	3698	3701	rBV3	316	200	0.03%	0.003%
100	13.328	3804	3806	3810	rBV2	274	172	0.02%	0.003%


Sum of corrected areas: 5745066

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU060619\
Data File : VU032487.D
Acq On : 06 Jun 2019 11:26
Operator : JC/SP
Sample : K3213-05
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DB8H8

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060619WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

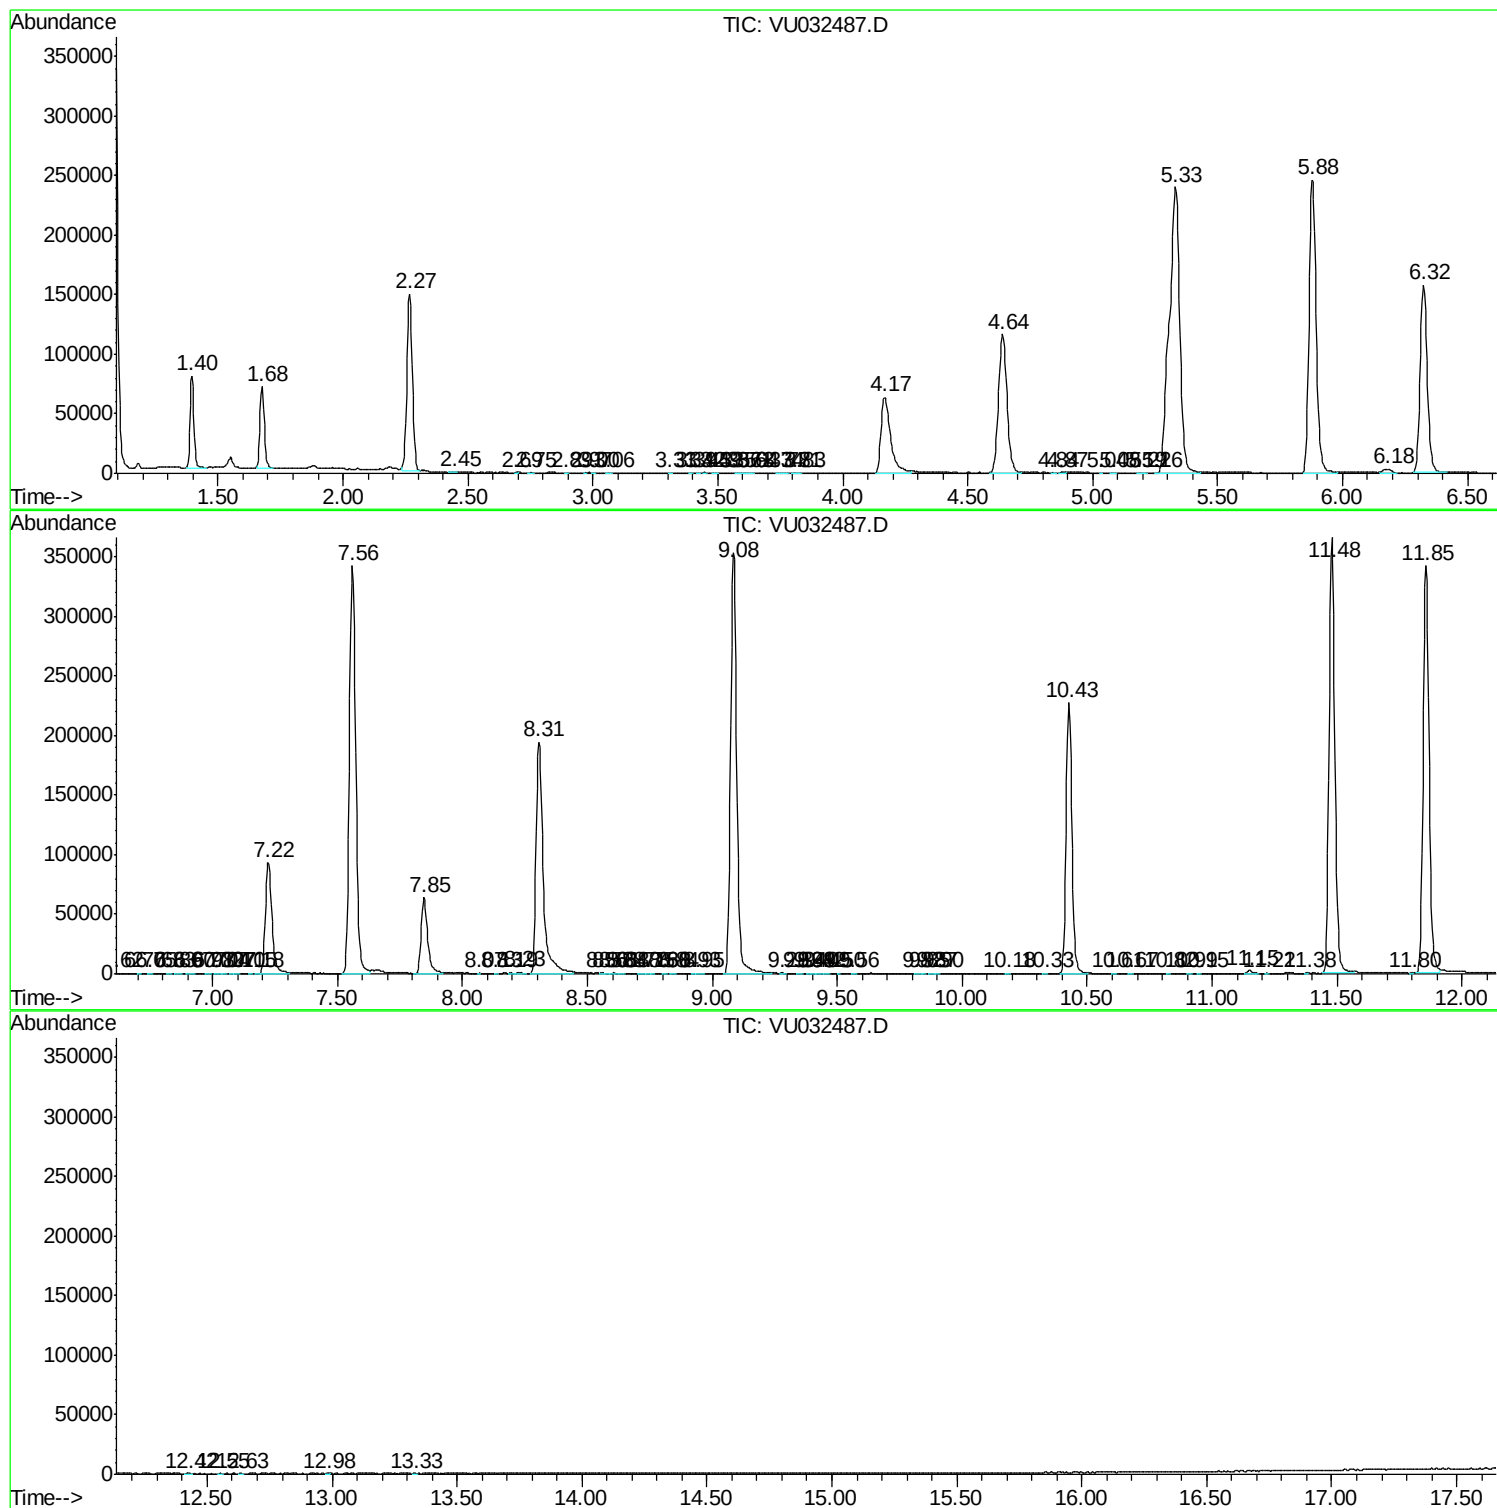

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU060619\
Data File : VU032487.D
Acq On : 06 Jun 2019 11:26
Operator : JC/SP
Sample : K3213-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DB8H8

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060619WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU060619\
Data File : VU032487.D
Acq On : 06 Jun 2019 11:26
Operator : JC/SP
Sample : K3213-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DB8H8

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060619WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc