

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU060619\
 Data File : VU032504.D
 Acq On : 06 Jun 2019 18:06
 Operator : JC/SP
 Sample : K3213-14
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DB8K5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060619WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.395	89	95	109	rVB	76434	81183	11.17%	1.375%
2	1.675	176	182	198	rVB	69344	85859	11.81%	1.454%
3	2.267	357	366	378	rVB	146923	218941	30.12%	3.709%
4	2.817	534	537	539	rBV	330	215	0.03%	0.004%
5	2.907	563	565	568	rVB2	299	167	0.02%	0.003%
6	2.990	588	591	593	rVB	183	99	0.01%	0.002%
7	3.006	594	596	600	rVV	203	115	0.02%	0.002%
8	3.067	613	615	617	rBV2	188	109	0.01%	0.002%
9	3.138	633	637	640	rBV2	169	107	0.01%	0.002%
10	3.157	640	643	645	rBV	156	102	0.01%	0.002%
11	3.193	651	654	656	rBV2	232	155	0.02%	0.003%
12	3.209	657	659	662	rBV	173	121	0.02%	0.002%
13	3.315	690	692	695	rBV2	169	102	0.01%	0.002%
14	3.428	723	727	729	rBV	256	154	0.02%	0.003%
15	3.530	754	759	761	rBV3	231	201	0.03%	0.003%
16	3.707	811	814	815	rBV	175	82	0.01%	0.001%
17	3.762	827	831	834	rBV2	236	198	0.03%	0.003%
18	3.781	834	837	840	rBV	101	84	0.01%	0.001%
19	3.868	861	864	866	rBV	101	81	0.01%	0.001%
20	3.900	871	874	877	rBV2	181	119	0.02%	0.002%
21	3.919	878	880	885	rVB	210	118	0.02%	0.002%
22	3.968	892	895	900	rBV	205	178	0.02%	0.003%
23	4.013	906	909	911	rBV2	264	140	0.02%	0.002%
24	4.048	917	920	921	rBV	171	117	0.02%	0.002%
25	4.170	947	958	995	rBV	68907	183119	25.19%	3.102%
26	4.640	1088	1104	1125	rBV	119450	279406	38.43%	4.733%
27	4.797	1149	1153	1155	rVB2	262	168	0.02%	0.003%
28	4.817	1158	1159	1162	rBV	212	115	0.02%	0.002%
29	4.849	1166	1169	1171	rVB	136	75	0.01%	0.001%
30	4.881	1172	1179	1182	rBV2	531	556	0.08%	0.009%
31	4.916	1188	1190	1193	rBV	129	74	0.01%	0.001%
32	4.948	1198	1200	1202	rBV	113	77	0.01%	0.001%
33	5.029	1220	1225	1226	rBV	346	275	0.04%	0.005%
34	5.161	1263	1266	1268	rBV2	162	94	0.01%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU060619\
 Data File : VU032504.D
 Acq On : 06 Jun 2019 18:06
 Operator : JC/SP
 Sample : K3213-14
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DB8K5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060619WMA.M
 Title : VOC Analysis

35	5.212	1280	1282	1284	rBV	171	71	0.01%	0.001%
36	5.244	1289	1292	1298	rBV	86	72	0.01%	0.001%
37	5.334	1298	1320	1351	rBV2	247509	726996	100.00%	12.314%
38	5.611	1403	1406	1408	rBV2	156	137	0.02%	0.002%
39	5.781	1456	1459	1463	rBV2	359	282	0.04%	0.005%
40	5.881	1477	1490	1511	rBV	249437	490604	67.48%	8.310%
41	6.325	1614	1628	1650	rBV	162794	327295	45.02%	5.544%
42	6.460	1667	1670	1674	rBV4	401	286	0.04%	0.005%
43	6.524	1687	1690	1692	rBV	400	302	0.04%	0.005%
44	6.681	1733	1739	1742	rVB2	271	209	0.03%	0.004%
45	6.701	1742	1745	1748	rBV	110	73	0.01%	0.001%
46	6.723	1748	1752	1756	rBV2	223	208	0.03%	0.004%
47	6.800	1772	1776	1778	rBV	152	104	0.01%	0.002%
48	6.897	1803	1806	1808	rVB2	135	86	0.01%	0.001%
49	6.945	1818	1821	1825	rVB2	311	204	0.03%	0.003%
50	6.974	1827	1830	1832	rVB2	264	142	0.02%	0.002%
51	7.032	1845	1848	1852	rVB	171	120	0.02%	0.002%
52	7.061	1852	1857	1859	rBV	146	87	0.01%	0.001%
53	7.096	1864	1868	1873	rVB	178	161	0.02%	0.003%
54	7.122	1873	1876	1881	rBV	214	164	0.02%	0.003%
55	7.148	1881	1884	1888	rVB	120	91	0.01%	0.002%
56	7.222	1897	1907	1930	rBV	91426	168911	23.23%	2.861%
57	7.418	1965	1968	1970	rBV2	435	228	0.03%	0.004%
58	7.559	1999	2012	2034	rBV	351518	609299	83.81%	10.321%
59	7.845	2092	2101	2122	rBV	63231	111181	15.29%	1.883%
60	8.305	2234	2244	2282	rBV	215223	408678	56.21%	6.922%
61	8.604	2336	2337	2342	rVB	340	245	0.03%	0.004%
62	8.643	2342	2349	2350	rBV2	546	422	0.06%	0.007%
63	8.765	2384	2387	2389	rBV2	163	134	0.02%	0.002%
64	8.913	2431	2433	2435	rVB	139	75	0.01%	0.001%
65	8.958	2444	2447	2450	rBV	102	84	0.01%	0.001%
66	9.003	2460	2461	2466	rVB	225	139	0.02%	0.002%
67	9.083	2474	2486	2505	rBV	359612	601058	82.68%	10.181%
68	9.292	2547	2551	2553	rBV2	320	248	0.03%	0.004%
69	9.337	2561	2565	2566	rVB	226	123	0.02%	0.002%
70	9.357	2567	2571	2574	rVB	165	123	0.02%	0.002%
71	9.386	2577	2580	2583	rBV2	170	126	0.02%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU060619\
 Data File : VU032504.D
 Acq On : 06 Jun 2019 18:06
 Operator : JC/SP
 Sample : K3213-14
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DB8K5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060619WMA.M
 Title : VOC Analysis

72	9.424	2588	2592	2594	rBV2	198	178	0.02%	0.003%
73	9.466	2602	2605	2608	rBB	99	86	0.01%	0.001%
74	9.620	2649	2653	2655	rBV	175	93	0.01%	0.002%
75	9.649	2658	2662	2669	rVV2	262	386	0.05%	0.007%
76	9.688	2672	2674	2678	rVB	211	92	0.01%	0.002%
77	9.758	2690	2696	2698	rBV	261	284	0.04%	0.005%
78	9.784	2702	2704	2706	rVB	172	69	0.01%	0.001%
79	9.832	2715	2719	2721	rBV2	205	177	0.02%	0.003%
80	9.926	2745	2748	2754	rVB2	248	227	0.03%	0.004%
81	10.266	2851	2854	2855	rBV	294	147	0.02%	0.002%
82	10.382	2887	2890	2892	rBV	166	135	0.02%	0.002%
83	10.427	2892	2904	2933	rVV	239005	391548	53.86%	6.632%
84	10.681	2981	2983	2988	rVB2	155	108	0.01%	0.002%
85	10.839	3030	3032	3036	rBV	104	89	0.01%	0.002%
86	10.858	3036	3038	3043	rVB	220	151	0.02%	0.003%
87	10.884	3044	3046	3050	rBV	140	107	0.01%	0.002%
88	11.000	3079	3082	3085	rVB2	249	155	0.02%	0.003%
89	11.029	3085	3091	3094	rBV	273	348	0.05%	0.006%
90	11.131	3121	3123	3128	rVB2	223	188	0.03%	0.003%
91	11.167	3131	3134	3138	rBV2	264	206	0.03%	0.003%
92	11.302	3173	3176	3177	rBV	170	118	0.02%	0.002%
93	11.427	3212	3215	3219	rBV3	336	221	0.03%	0.004%
94	11.479	3219	3231	3263	rBV	381017	612895	84.31%	10.382%
95	11.855	3336	3348	3372	rBV	360746	592931	81.56%	10.043%
96	12.205	3455	3457	3460	rBV3	257	197	0.03%	0.003%
97	12.321	3490	3493	3495	rBV2	428	308	0.04%	0.005%
98	13.218	3769	3772	3774	rBV	347	195	0.03%	0.003%
99	13.360	3812	3816	3819	rBV2	320	302	0.04%	0.005%
100	13.697	3916	3921	3922	rBV2	323	280	0.04%	0.005%


Sum of corrected areas: 5903695

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU060619\
Data File : VU032504.D
Acq On : 06 Jun 2019 18:06
Operator : JC/SP
Sample : K3213-14
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DB8K5

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060619WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

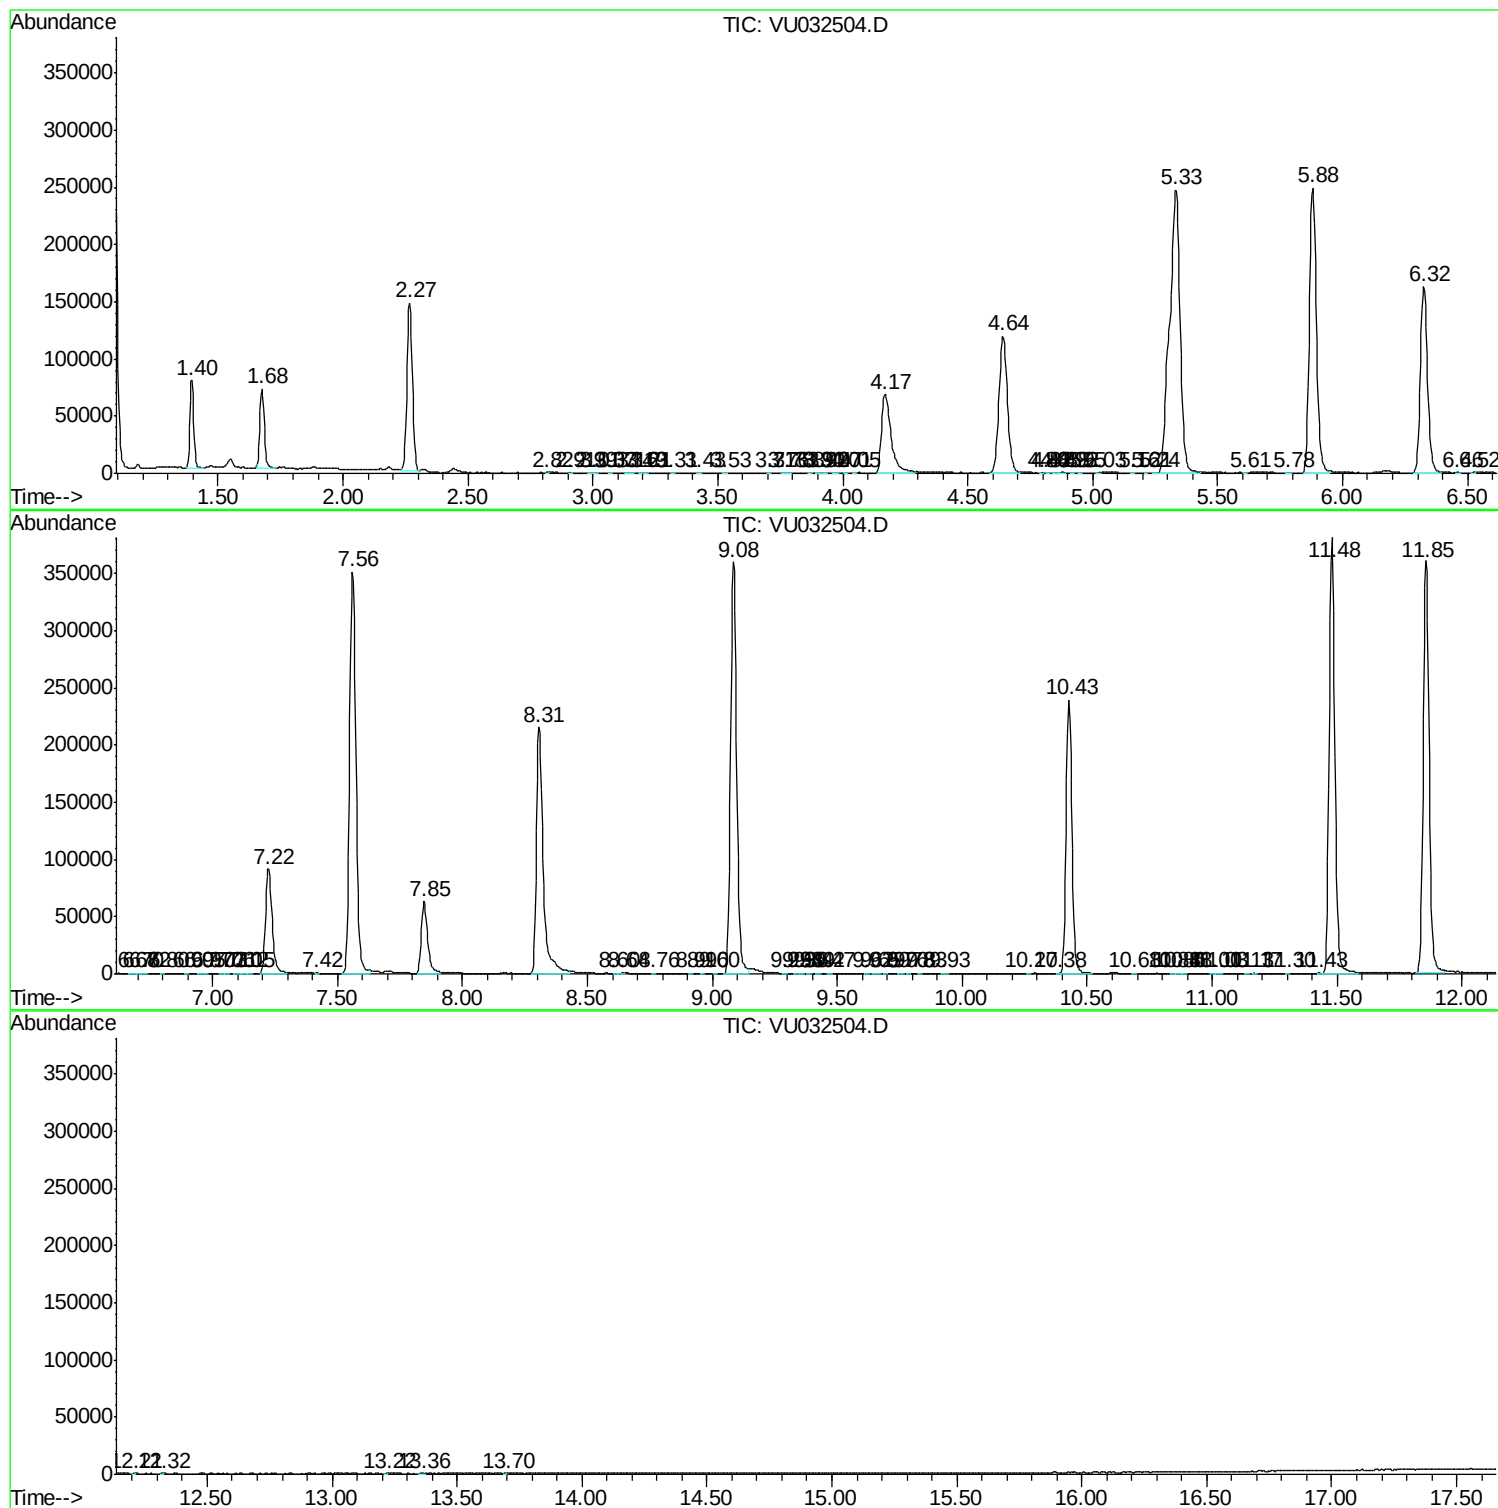

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU060619\
Data File : VU032504.D
Acq On : 06 Jun 2019 18:06
Operator : JC/SP
Sample : K3213-14
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DB8K5

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060619WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU060619\
Data File : VU032504.D
Acq On : 06 Jun 2019 18:06
Operator : JC/SP
Sample : K3213-14
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DB8K5

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060619WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc